

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
 Data File : FF011372.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2022 10:48
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 03:21:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2094385	18.685 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.954	52830	0.431 ug/ml
13) N-TRIACONTANE	17.839	144943	1.201 ug/ml
14) N-DOTRIACONTANE	18.670	200996	1.699 ug/ml
15) N-TETRATRIACONTANE	19.451	147603	1.293 ug/ml
16) N-HEXATRIACONTANE	20.189	101170	0.951 ug/ml
17) N-OCTATRIACONTANE	20.894	61550	0.592 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011372.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 10:48
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:21:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

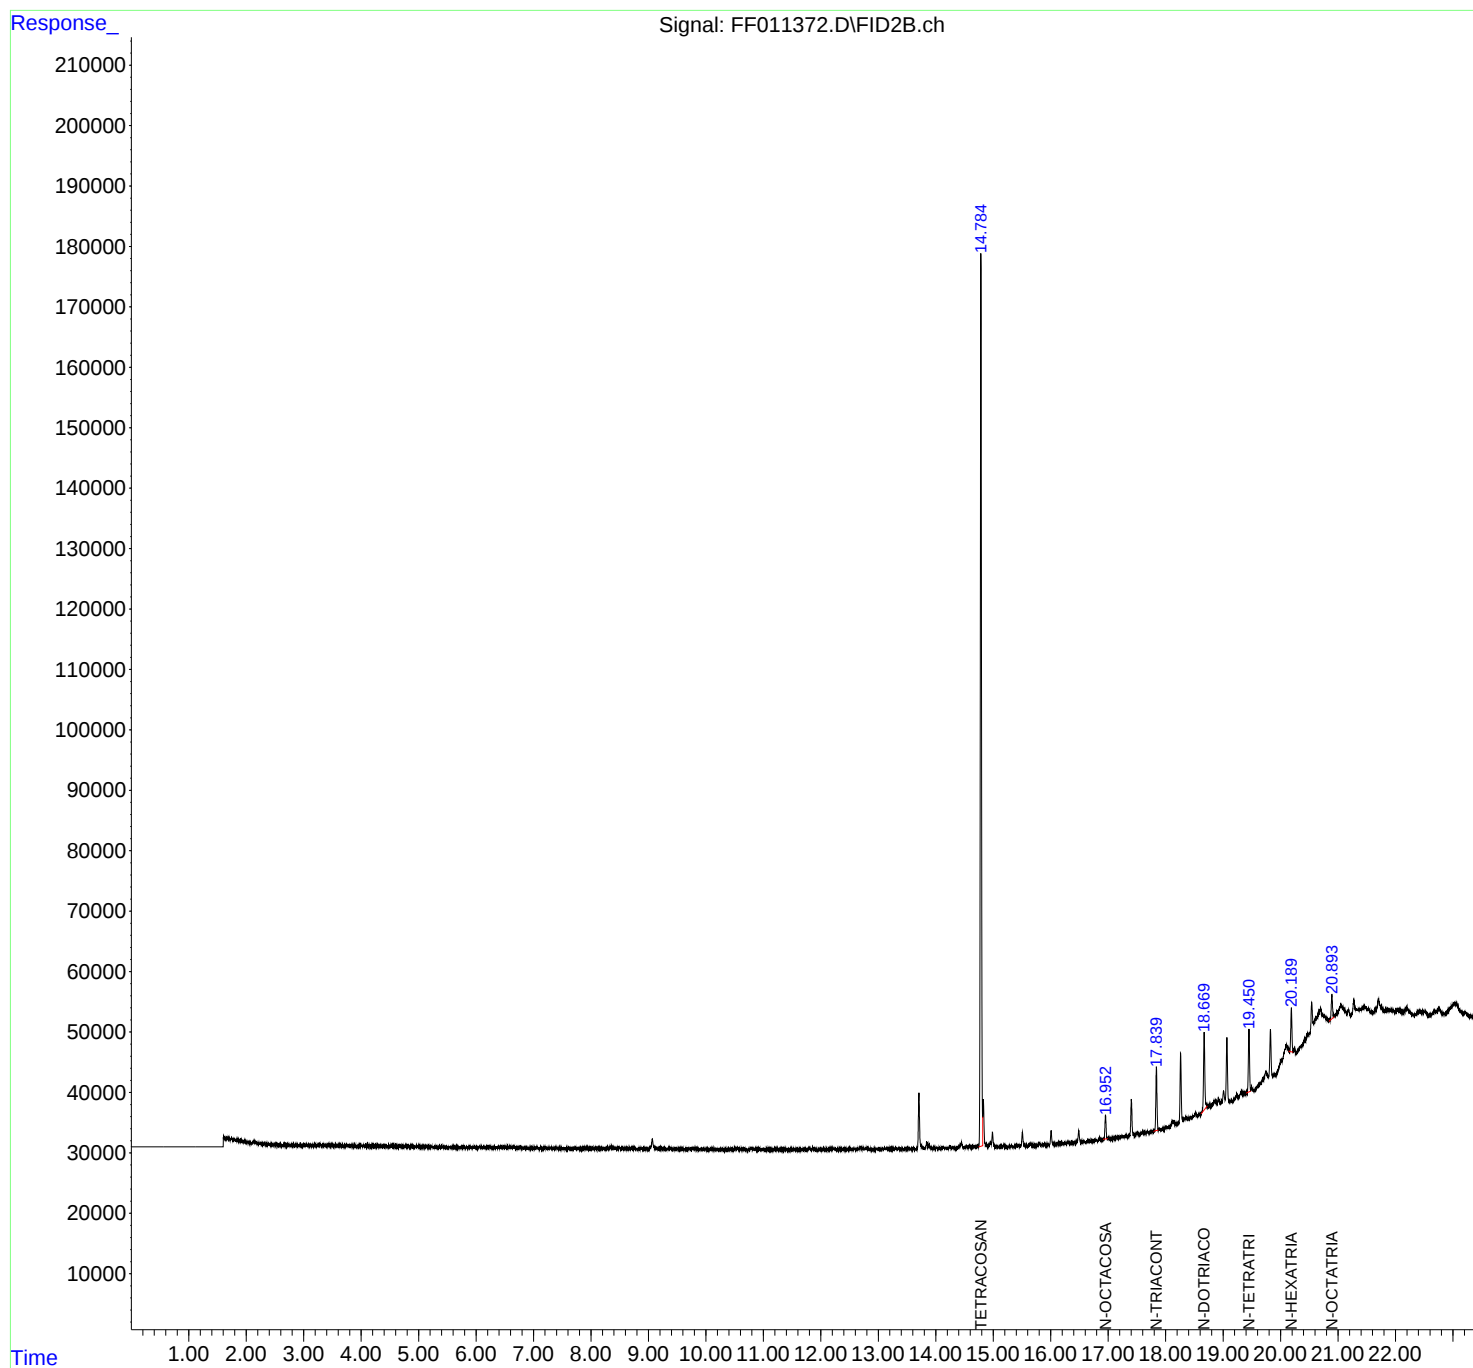


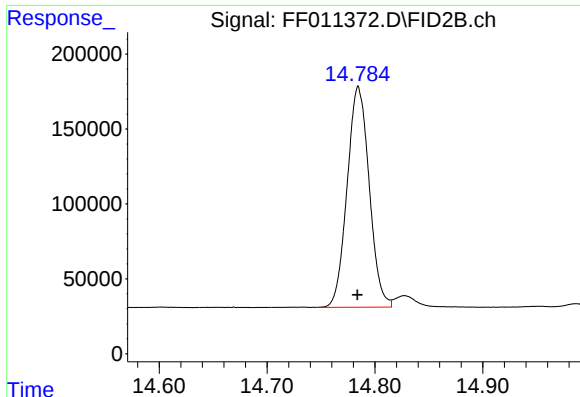

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 2094385
Conc: 18.69 ug/ml

Instrument :
FID_F
ClientSampleId :

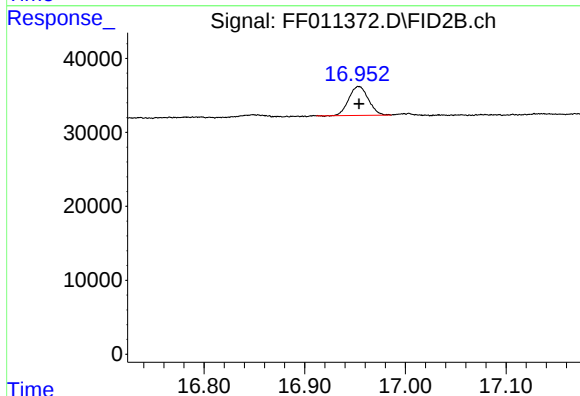


#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.000 min
Response: 52830
Conc: 0.43 ug/ml

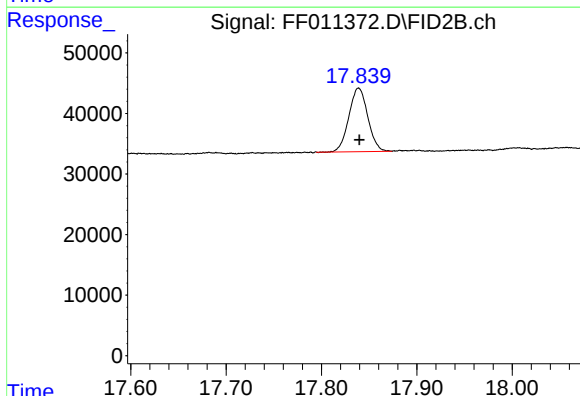


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: 0.000 min
Response: 144943
Conc: 1.20 ug/ml

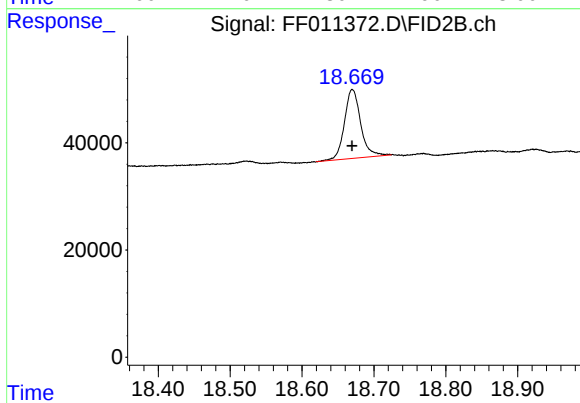

#14 N-DOTRIACONTANE


R.T.: 18.670 min
Delta R.T.: 0.000 min
Response: 200996
Conc: 1.70 ug/ml

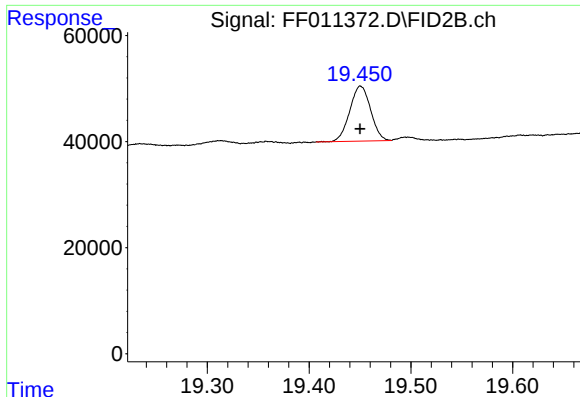

#15 N-TETRATRIACONTANE


R.T.: 19.451 min
Delta R.T.: 0.000 min
Response: 147603
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :

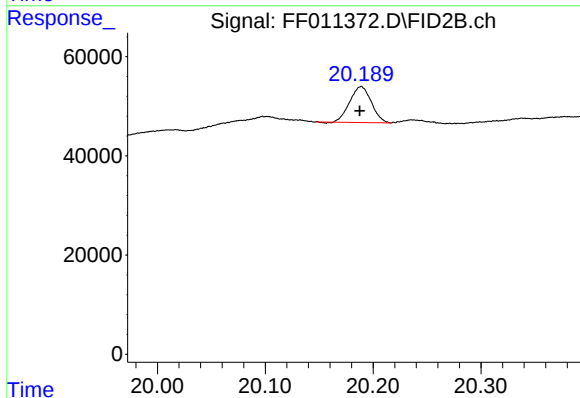

#16 N-HEXATRIACONTANE

R.T.: 20.189 min
Delta R.T.: 0.001 min
Response: 101170
Conc: 0.95 ug/ml

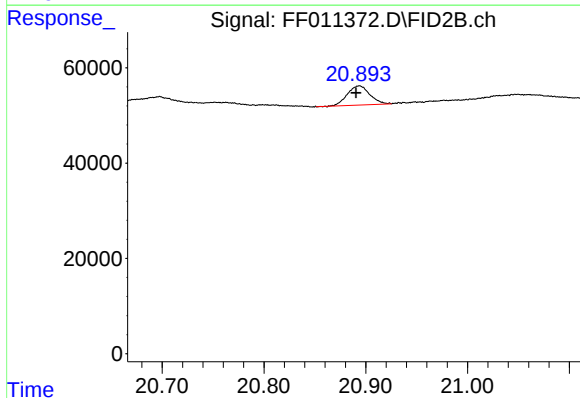

#17 N-OCTATRIACONTANE

R.T.: 20.894 min
Delta R.T.: 0.003 min
Response: 61550
Conc: 0.59 ug/ml