

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
 Data File : FF011374.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2022 12:23
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 03:21:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.516	2724750	20.808 ug/ml
12)	N-OCTACOSANE	16.955	2548046	20.802 ug/ml
13)	N-TRIACONTANE	17.840	151549	1.256 ug/ml
14)	N-DOTRIACONTANE	18.669	217776	1.841 ug/ml
15)	N-TETRATRIACONTANE	19.449	194151	1.701 ug/ml
16)	N-HEXATRIACONTANE	20.187	136863	1.286 ug/ml
17)	N-OCTATRIACONTANE	20.891	92647	0.891 ug/ml
18)	N-TETRACONTANE	21.705	68335	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011374.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 12:23
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:21:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

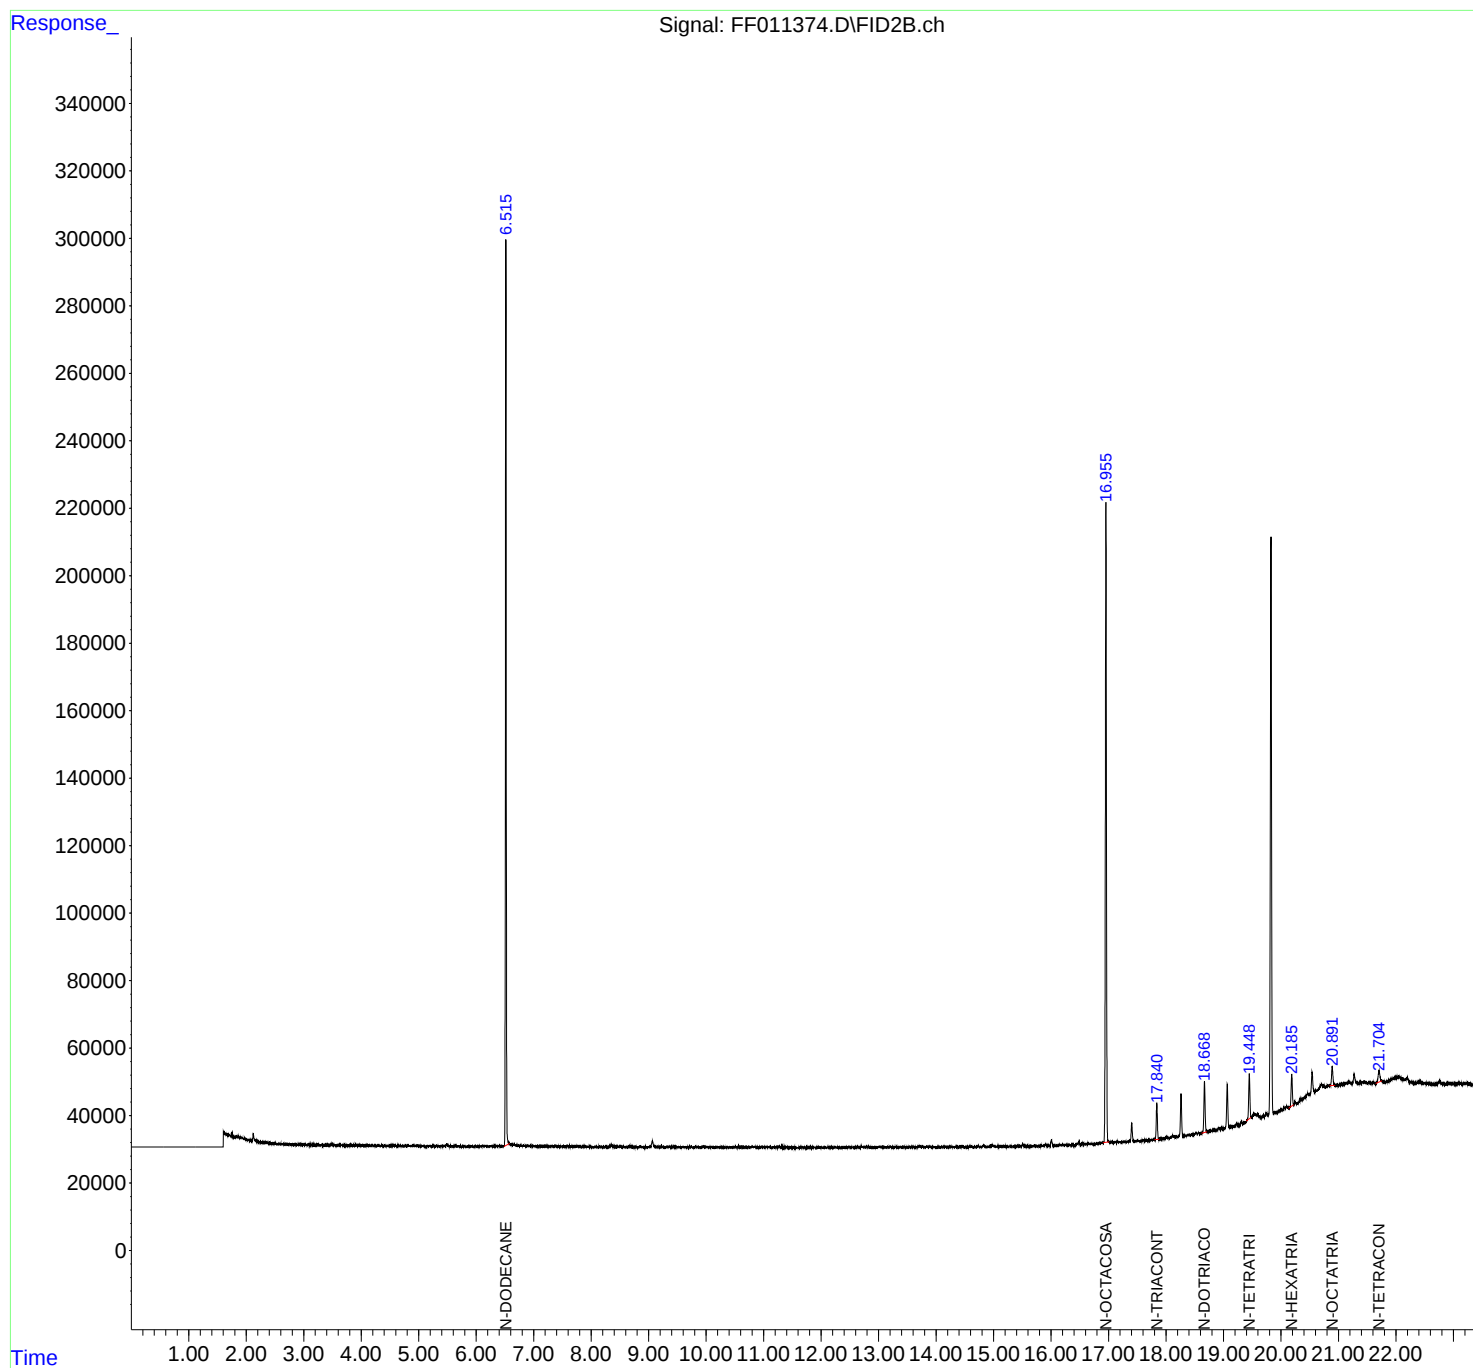


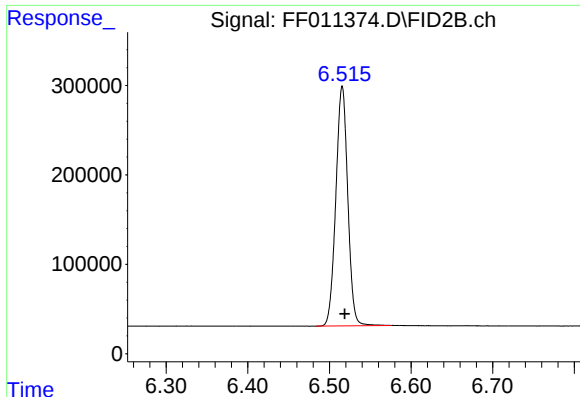

#3 N-DODECANE


R.T.: 6.516 min
Delta R.T.: -0.003 min
Response: 2724750
Conc: 20.81 ug/ml

Instrument :
FID_F
ClientSampleId :

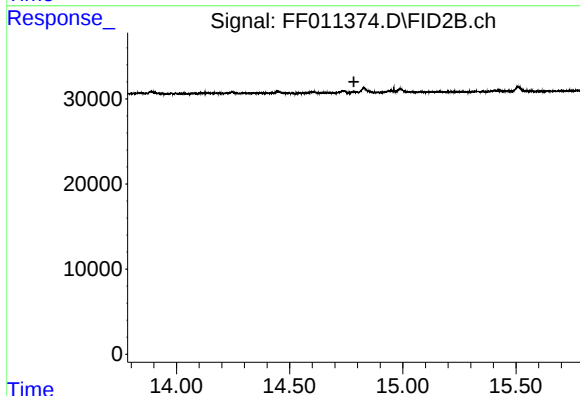


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

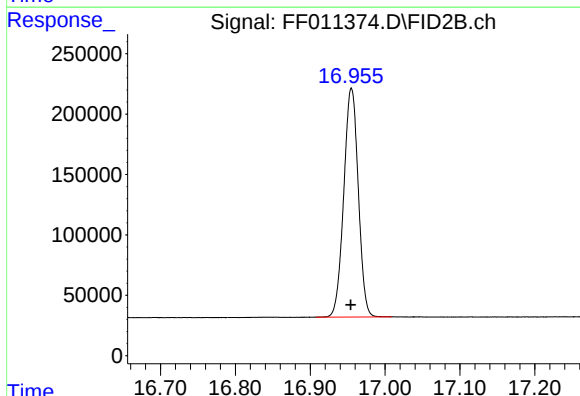


#12 N-OCTACOSANE

R.T.: 16.955 min
Delta R.T.: 0.001 min
Response: 2548046
Conc: 20.80 ug/ml

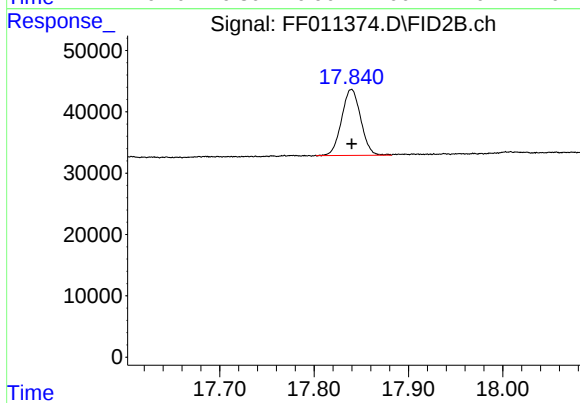

#13 N-TRIACONTANE


R.T.: 17.840 min
Delta R.T.: 0.000 min
Response: 151549
Conc: 1.26 ug/ml

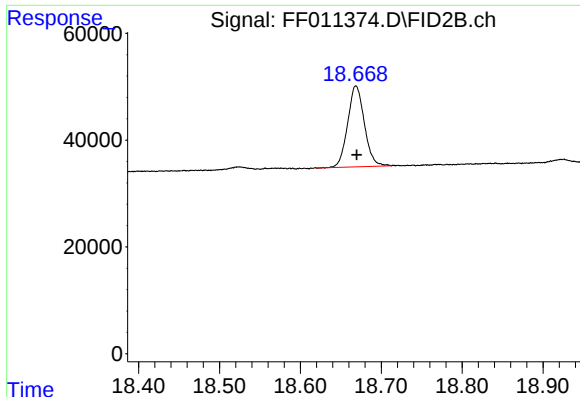

#14 N-DOTRIACONTANE


R.T.: 18.669 min
Delta R.T.: 0.000 min
Response: 217776
Conc: 1.84 ug/ml

Instrument :
FID_F
ClientSampleId :

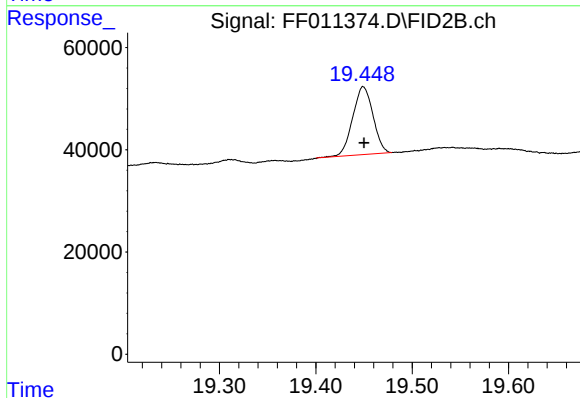


#15 N-TETRATRIACONTANE

R.T.: 19.449 min
Delta R.T.: 0.000 min
Response: 194151
Conc: 1.70 ug/ml

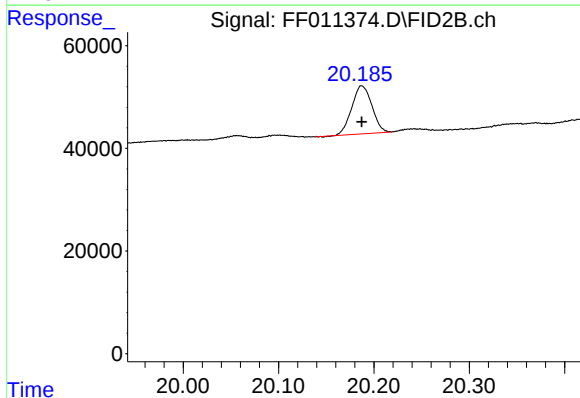


#16 N-HEXATRIACONTANE

R.T.: 20.187 min
Delta R.T.: 0.000 min
Response: 136863
Conc: 1.29 ug/ml

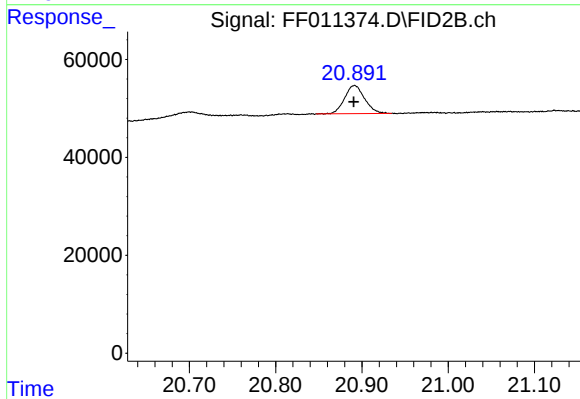

#17 N-OCTATRIACONTANE

R.T.: 20.891 min
Delta R.T.: 0.000 min
Response: 92647
Conc: 0.89 ug/ml

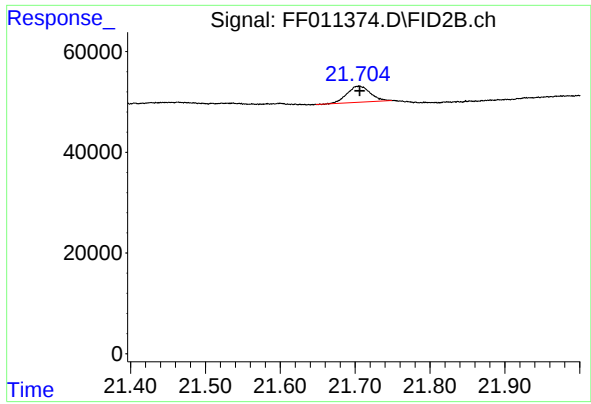

#18 N-TETRACONTANE

R.T.: 21.705 min
Delta R.T.: -0.001 min
Response: 68335
Conc: 0.65 ug/ml

Instrument :

FID_F

ClientSampleId :