

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
 Data File : FF011377.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2022 16:43
 Operator : YP\AJ
 Sample : N4500-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 03:21:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	1620901	14.461 ug/ml
Target Compounds			
7) N-EICOSANE	12.733	205476	1.562 ug/ml
10) N-TETRACOSANE	14.983	72296	0.568 ug/ml
11) N-HEXACOSANE	16.004	90368	0.724 ug/ml
12) N-OCTACOSANE	16.951	123129	1.005 ug/ml
13) N-TRIACONTANE	17.838	115536	0.958 ug/ml
14) N-DOTRIACONTANE	18.667	85397	0.722 ug/ml
15) N-TETRATRIACONTANE	19.449	44627	0.391 ug/ml
18) N-TETRACONTANE	21.701	87959	0.834 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011377.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 16:43
Operator : YP\AJ
Sample : N4500-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:21:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

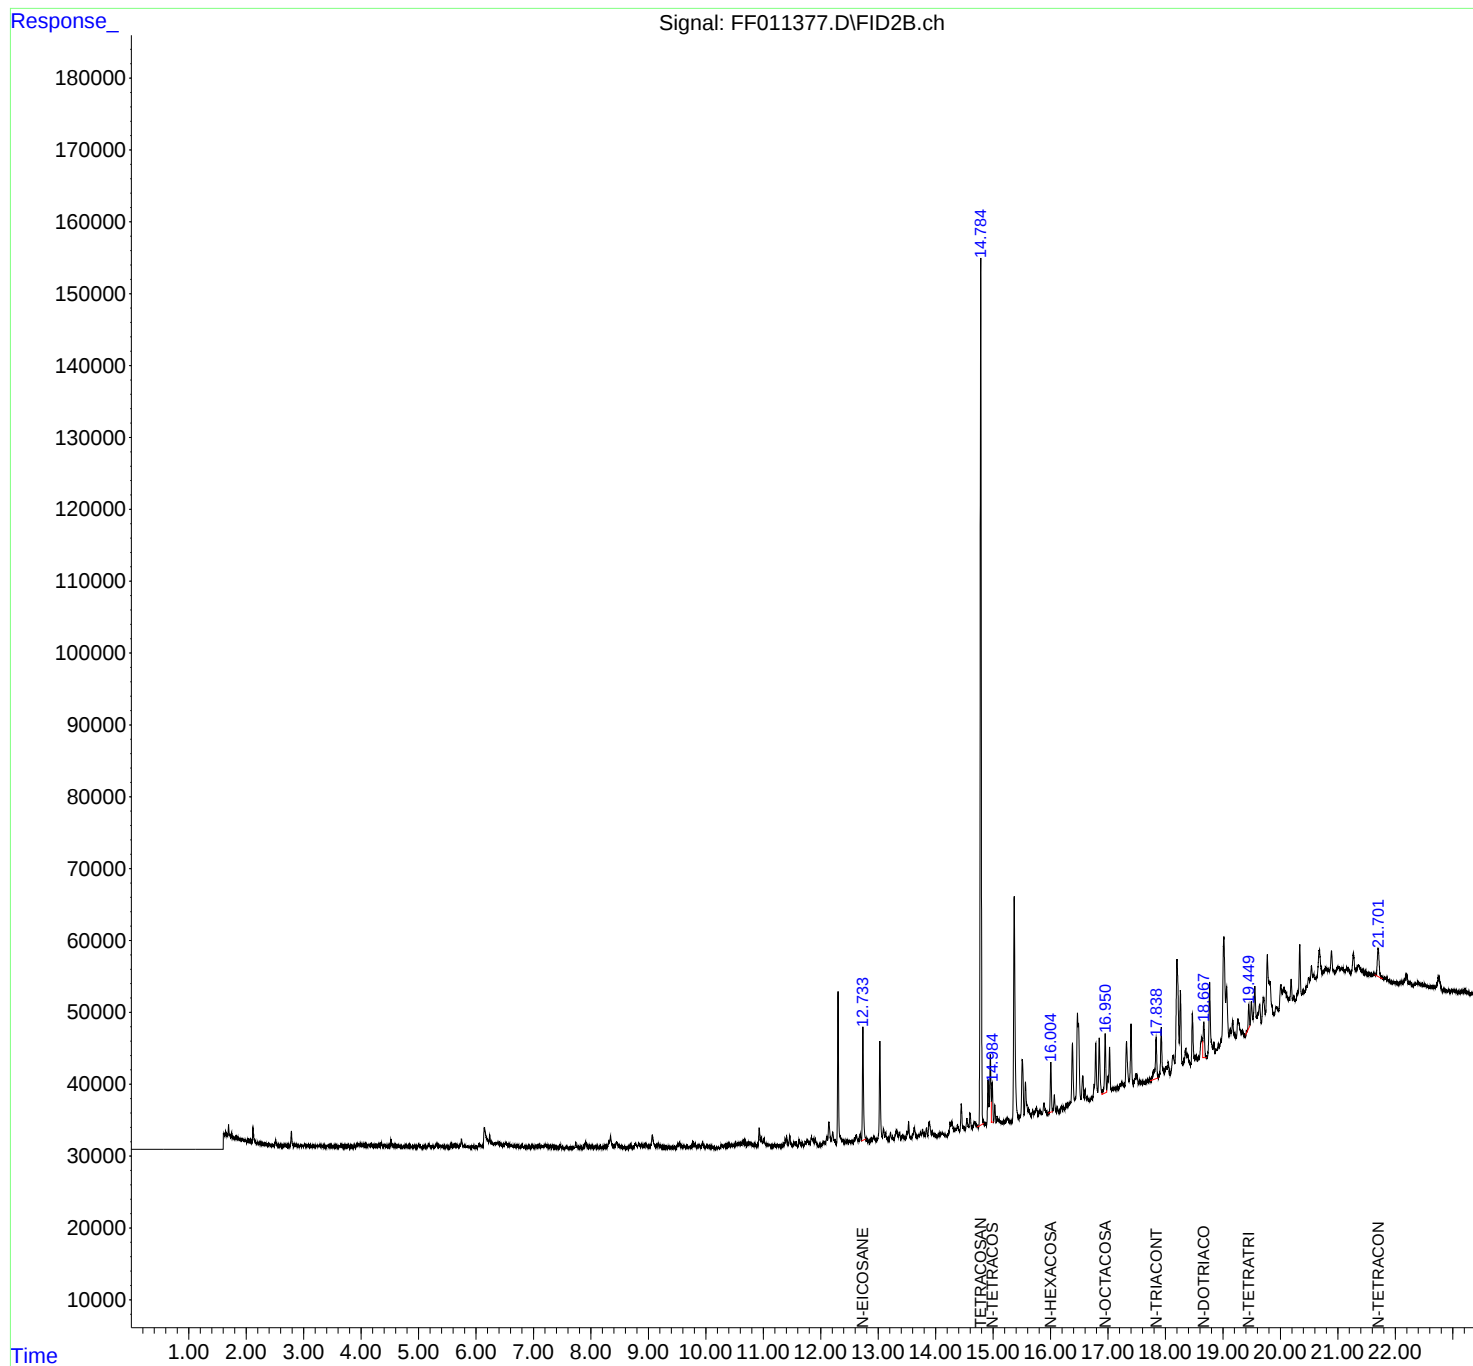


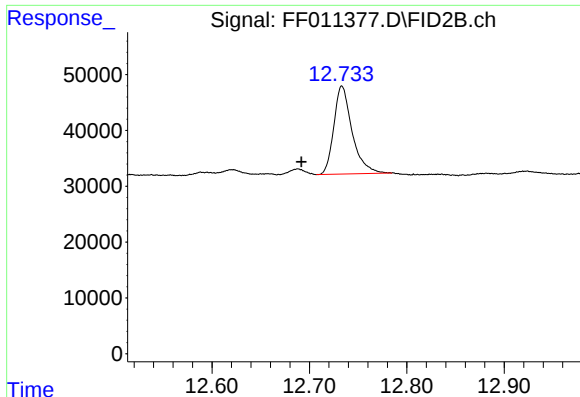

#7 N-EICOSANE


R.T.: 12.733 min
Delta R.T.: 0.041 min
Response: 205476
Conc: 1.56 ug/ml

Instrument :
FID_F
ClientSampleId :

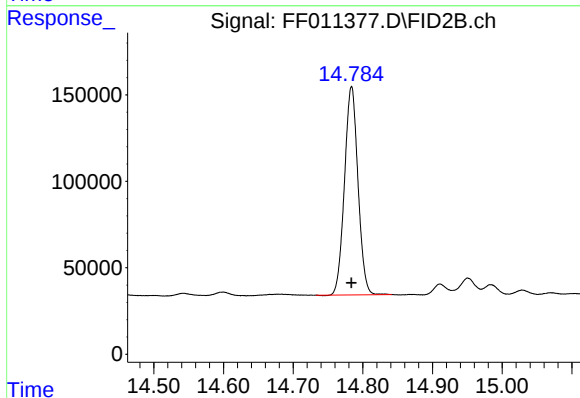


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 1620901
Conc: 14.46 ug/ml

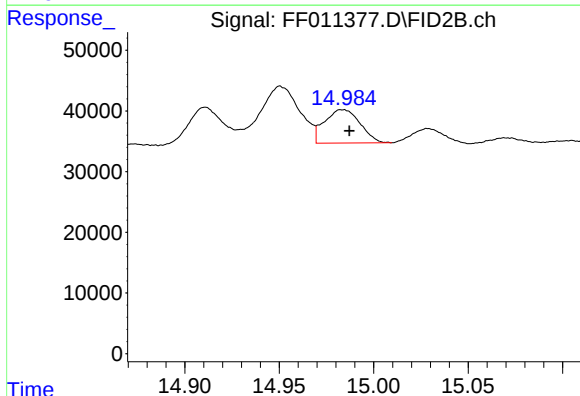


#10 N-TETRACOSANE

R.T.: 14.983 min
Delta R.T.: -0.004 min
Response: 72296
Conc: 0.57 ug/ml

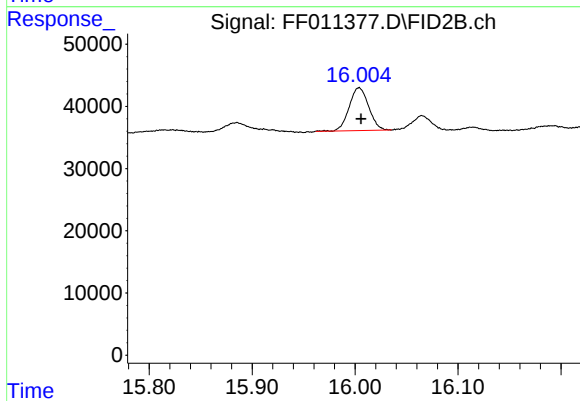

#11 N-HEXACOSANE


R.T.: 16.004 min
Delta R.T.: -0.002 min
Response: 90368
Conc: 0.72 ug/ml

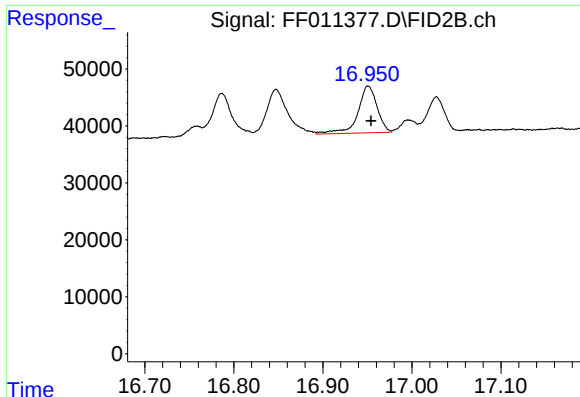

#12 N-OCTACOSANE


R.T.: 16.951 min
Delta R.T.: -0.003 min
Response: 123129
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :

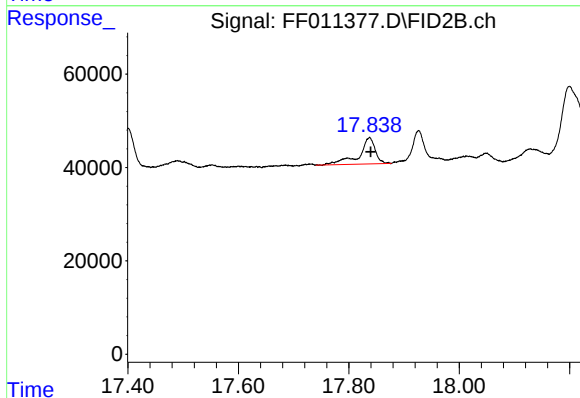


#13 N-TRIACONTANE

R.T.: 17.838 min
Delta R.T.: -0.002 min
Response: 115536
Conc: 0.96 ug/ml

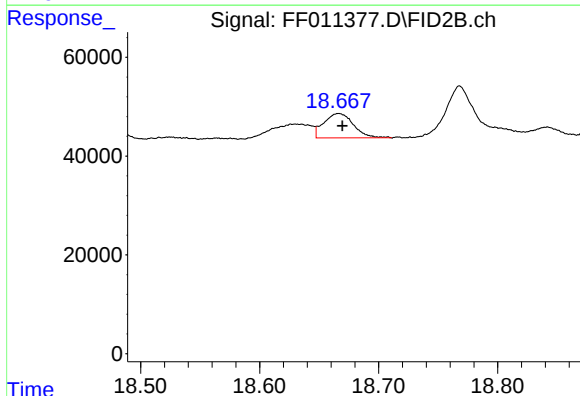


#14 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: -0.003 min
Response: 85397
Conc: 0.72 ug/ml

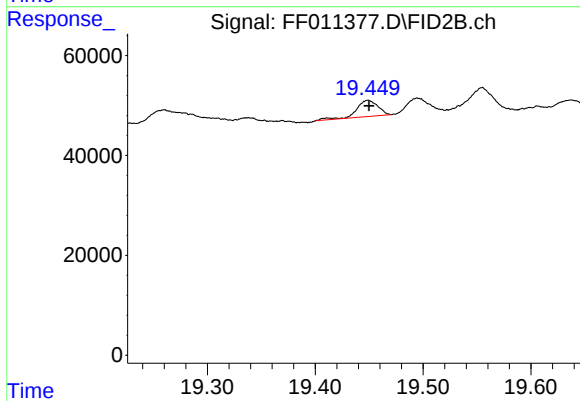

#15 N-TETRATRIACONTANE

R.T.: 19.449 min
Delta R.T.: -0.001 min
Response: 44627
Conc: 0.39 ug/ml

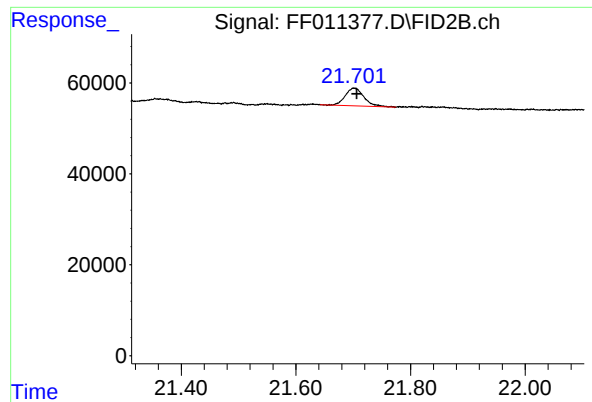

#18 N-TETRACONTANE

R.T.: 21.701 min
Delta R.T.: -0.005 min
Response: 87959
Conc: 0.83 ug/ml

Instrument :

FID_F

ClientSampleId :