

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
 Data File : FF011378.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2022 17:13
 Operator : YP\AJ
 Sample : N4500-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 03:22:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	1730849	15.442 ug/ml
Target Compounds			
6) N-OCTADECANE	11.404	123952	0.932 ug/ml
7) N-EICOSANE	12.684	91599	0.696 ug/ml
8) N-DOCOSANE	13.892	354857	2.776 ug/ml
10) N-TETRACOSANE	14.945	1473879	11.575 ug/ml
11) N-HEXACOSANE	16.007	157324	1.260 ug/ml
12) N-OCTACOSANE	16.944	573177	4.679 ug/ml
13) N-TRIACONTANE	17.838	162208	1.344 ug/ml
14) N-DOTRIACONTANE	18.663	182948	1.547 ug/ml
15) N-TETRATRIACONTANE	19.456	38547	0.338 ug/ml
16) N-HEXATRIACONTANE	20.142	139992	1.315 ug/ml
18) N-TETRACONTANE	21.722	126265	1.197 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011378.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 17:13
Operator : YP\AJ
Sample : N4500-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:22:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

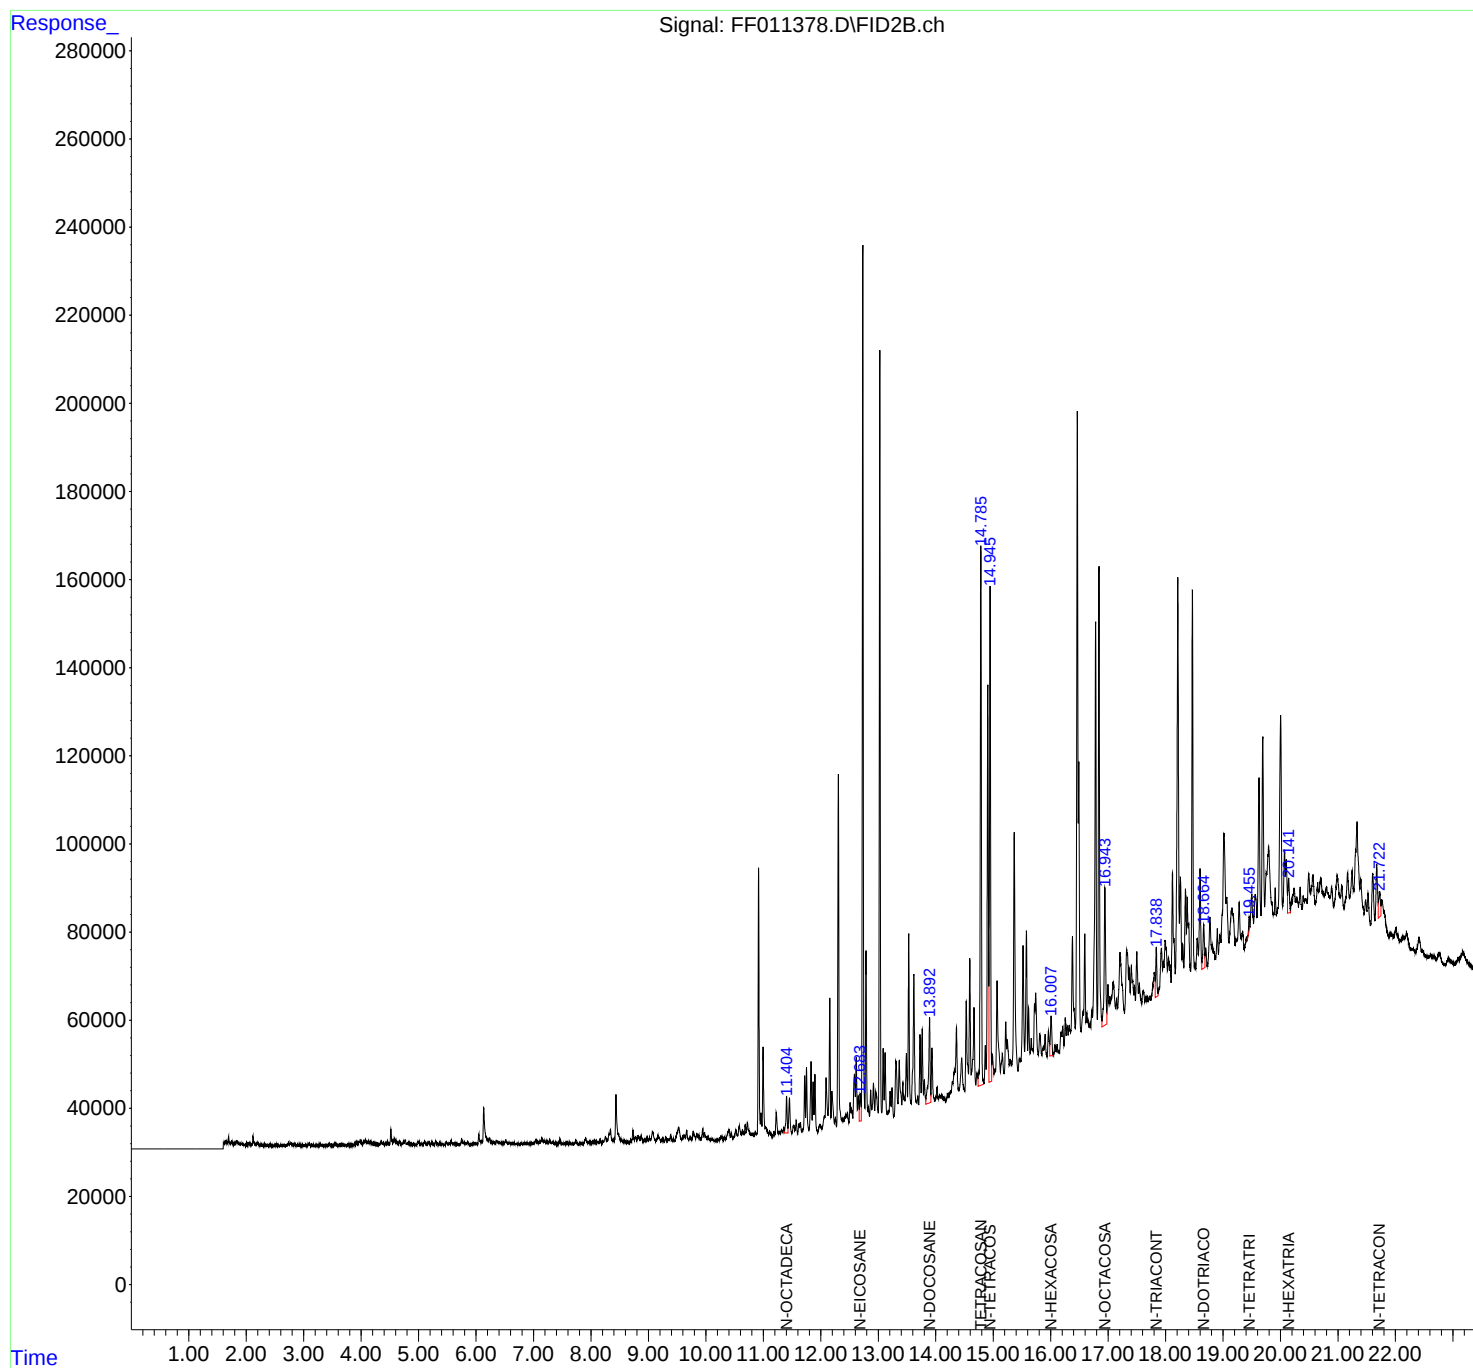


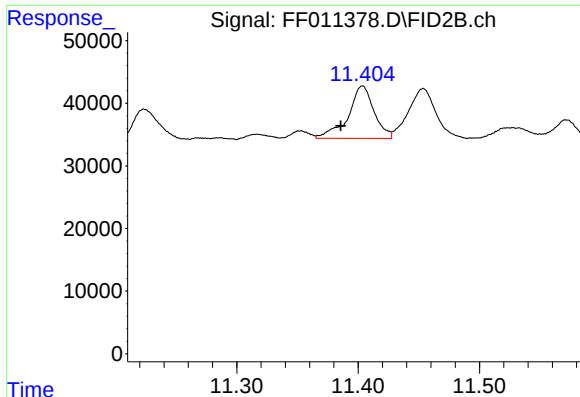

#6 N-OCTADECANE


R.T.: 11.404 min
Delta R.T.: 0.018 min
Response: 123952
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :

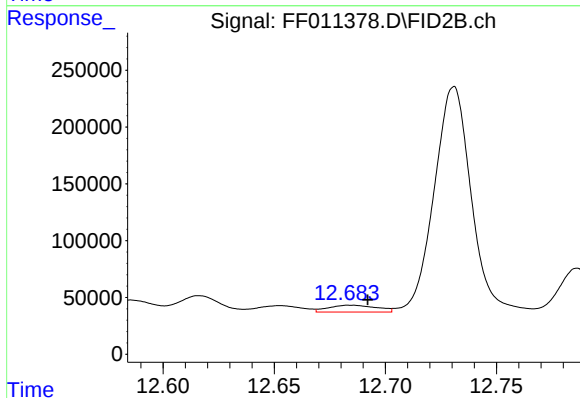


#7 N-EICOSANE

R.T.: 12.684 min
Delta R.T.: -0.008 min
Response: 91599
Conc: 0.70 ug/ml

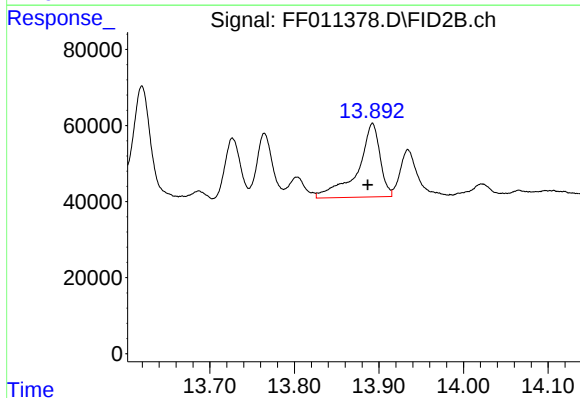


#8 N-DOCOSANE

R.T.: 13.892 min
Delta R.T.: 0.006 min
Response: 354857
Conc: 2.78 ug/ml

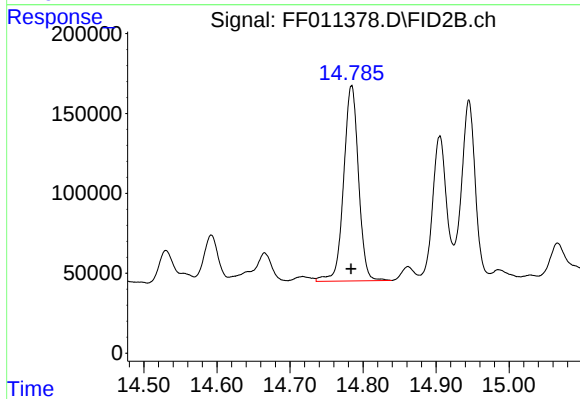

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 1730849
Conc: 15.44 ug/ml

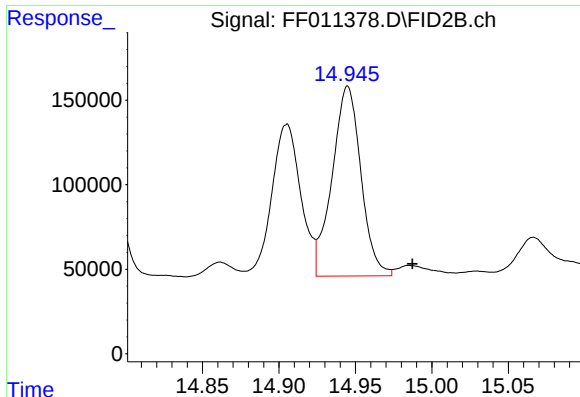

#10 N-TETRACOSANE


R.T.: 14.945 min
Delta R.T.: -0.042 min
Response: 1473879
Conc: 11.58 ug/ml

Instrument :
FID_F
ClientSampleId :

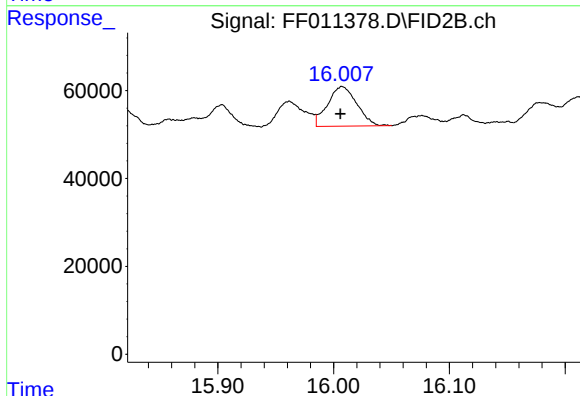


#11 N-HEXACOSANE

R.T.: 16.007 min
Delta R.T.: 0.002 min
Response: 157324
Conc: 1.26 ug/ml

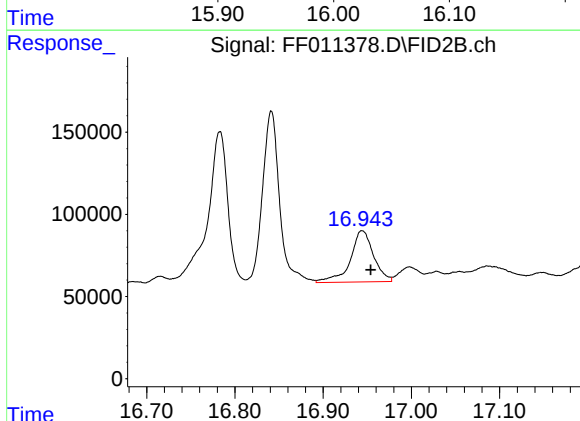


#12 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: -0.010 min
Response: 573177
Conc: 4.68 ug/ml

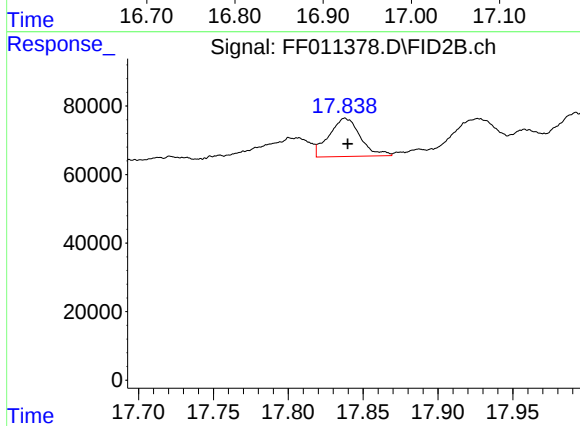

#13 N-TRIACONTANE


R.T.: 17.838 min
Delta R.T.: -0.002 min
Response: 162208
Conc: 1.34 ug/ml

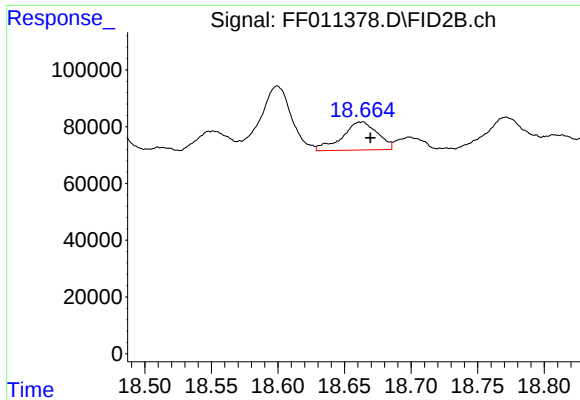

#14 N-DOTRIACONTANE


R.T.: 18.663 min
Delta R.T.: -0.006 min
Response: 182948
Conc: 1.55 ug/ml

Instrument :
FID_F
ClientSampleId :

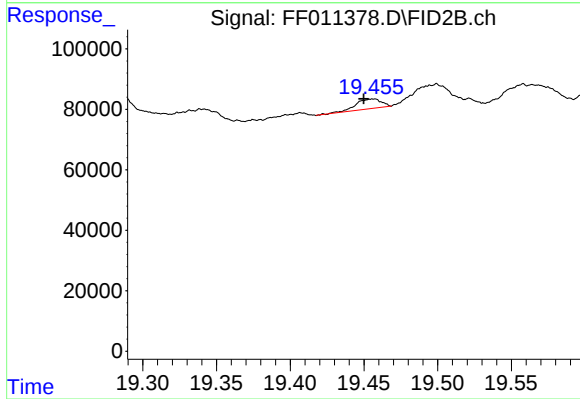


#15 N-TETRATRIACONTANE

R.T.: 19.456 min
Delta R.T.: 0.006 min
Response: 38547
Conc: 0.34 ug/ml

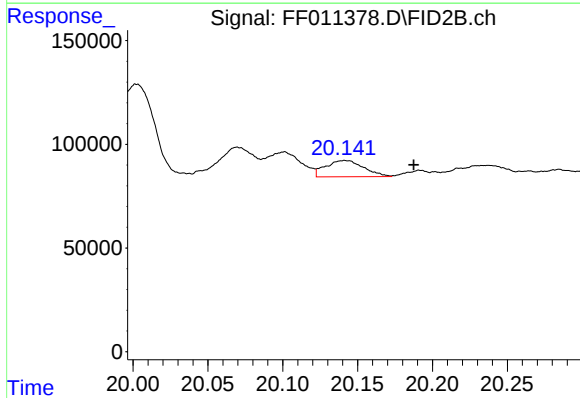

#16 N-HEXATRIACONTANE

R.T.: 20.142 min
Delta R.T.: -0.046 min
Response: 139992
Conc: 1.32 ug/ml

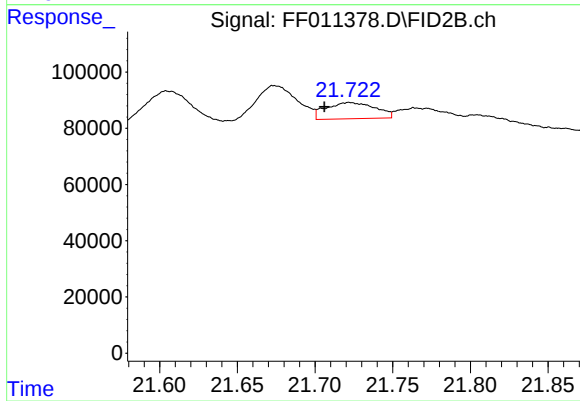

#18 N-TETRACONTANE

R.T.: 21.722 min
Delta R.T.: 0.016 min
Response: 126265
Conc: 1.20 ug/ml