

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
 Data File : FF011380.D
 Signal(s) : FID2B.ch
 Acq On : 06 Sep 2022 18:12
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 07 03:22:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
 Quant Title :
 QLast Update : Mon Aug 29 01:24:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	2348768	20.954 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.954	67274	0.549 ug/ml
13) N-TRIACONTANE	17.838	187728	1.556 ug/ml
14) N-DOTRIACONTANE	18.668	245662	2.077 ug/ml
15) N-TETRATRIACONTANE	19.449	188790	1.654 ug/ml
16) N-HEXATRIACONTANE	20.187	135427	1.272 ug/ml
17) N-OCTATRIACONTANE	20.889	102021	0.981 ug/ml
18) N-TETRACONTANE	21.705	149092	1.413 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011380.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 18:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:22:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

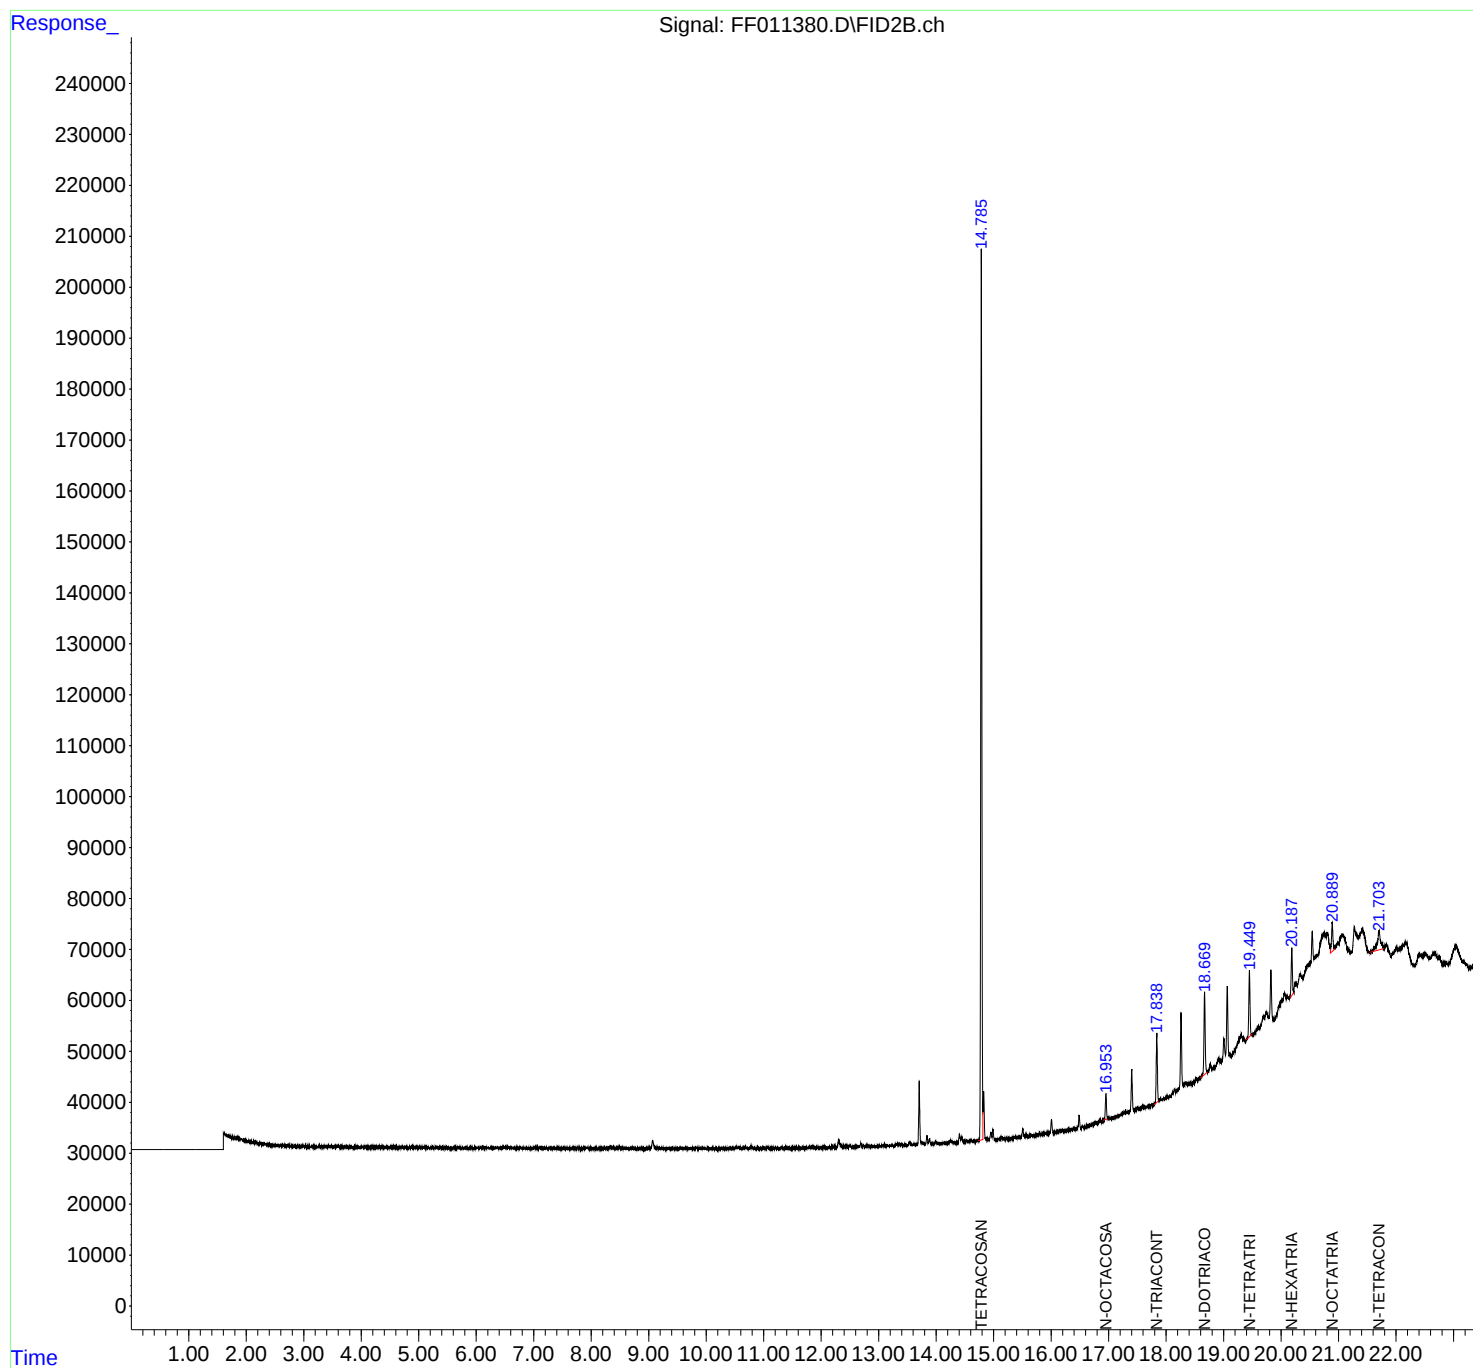


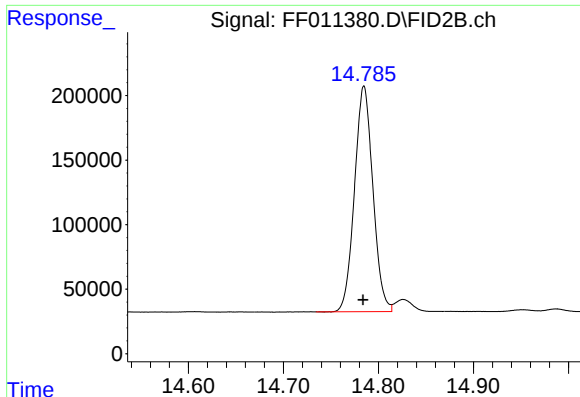

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: 0.001 min
Response: 2348768
Conc: 20.95 ug/ml

Instrument :
FID_F
ClientSampleId :

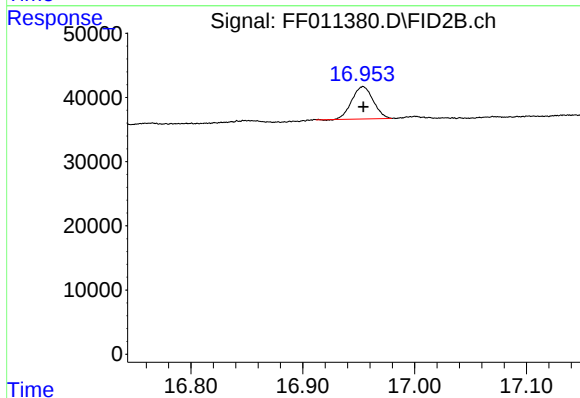


#12 N-OCTACOSANE

R.T.: 16.954 min
Delta R.T.: 0.000 min
Response: 67274
Conc: 0.55 ug/ml

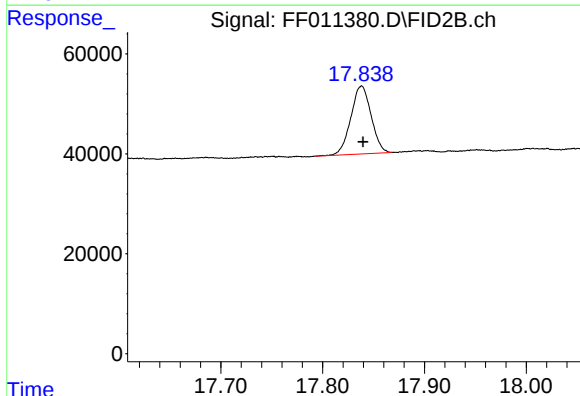


#13 N-TRIACONTANE

R.T.: 17.838 min
Delta R.T.: -0.002 min
Response: 187728
Conc: 1.56 ug/ml

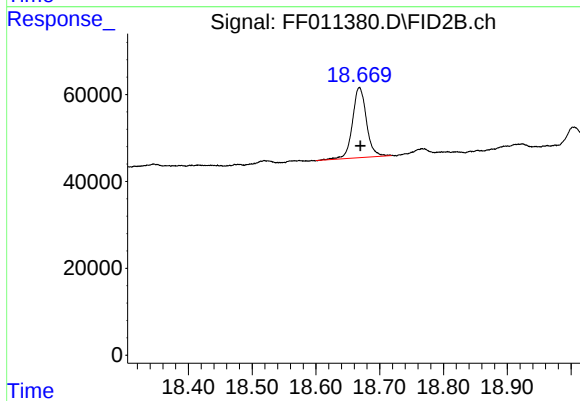

#14 N-DOTRIACONTANE


R.T.: 18.668 min
Delta R.T.: -0.001 min
Response: 245662
Conc: 2.08 ug/ml

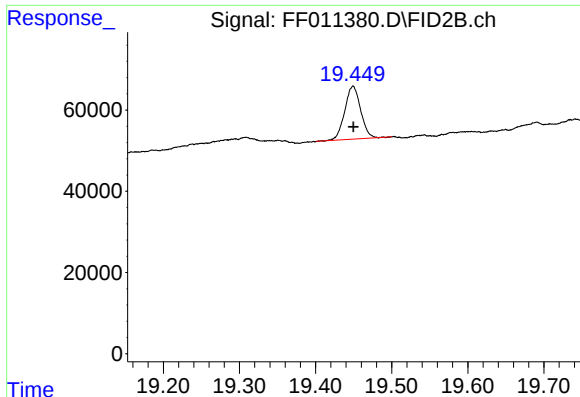

#15 N-TETRATRIACONTANE


R.T.: 19.449 min
Delta R.T.: 0.000 min
Response: 188790
Conc: 1.65 ug/ml

Instrument :
FID_F
ClientSampleId :

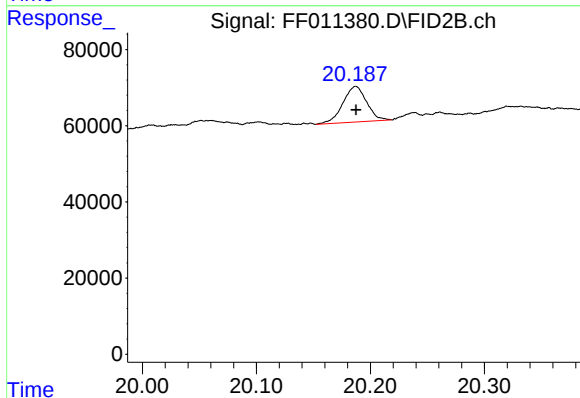


#16 N-HEXATRIACONTANE

R.T.: 20.187 min
Delta R.T.: 0.000 min
Response: 135427
Conc: 1.27 ug/ml

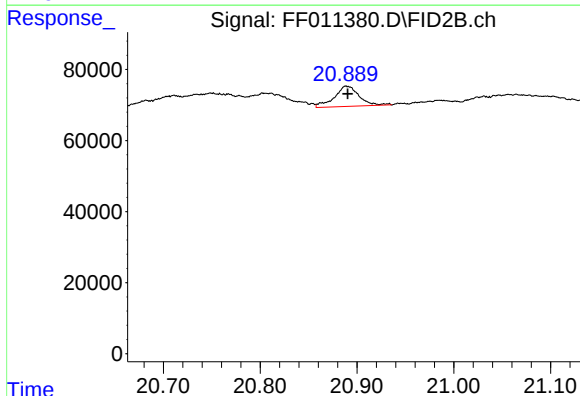

#17 N-OCTATRIACONTANE

R.T.: 20.889 min
Delta R.T.: -0.001 min
Response: 102021
Conc: 0.98 ug/ml

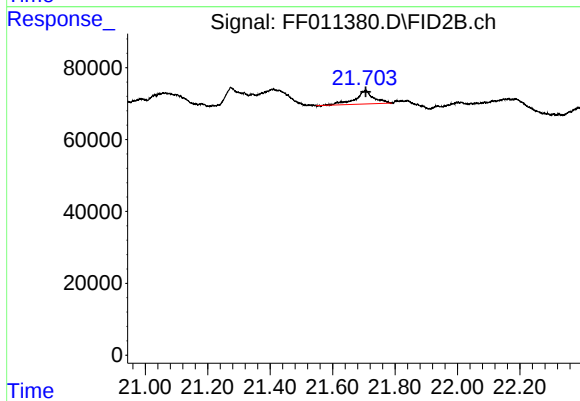

#18 N-TETRACONTANE

R.T.: 21.705 min
Delta R.T.: -0.001 min
Response: 149092
Conc: 1.41 ug/ml