

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011386.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 22:12
Operator : YP\AJ
Sample : N4501-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:23:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	1524040	13.597 ug/ml
Target Compounds			
7) N-EICOSANE	12.733	195492	1.486 ug/ml
10) N-TETRACOSANE	14.985	59079	0.464 ug/ml
11) N-HEXACOSANE	16.004	60099	0.481 ug/ml
12) N-OCTACOSANE	16.952	53489	0.437 ug/ml
14) N-DOTRIACONTANE	18.661	90257	0.763 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011386.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 22:12
Operator : YP\AJ
Sample : N4501-14
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:23:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

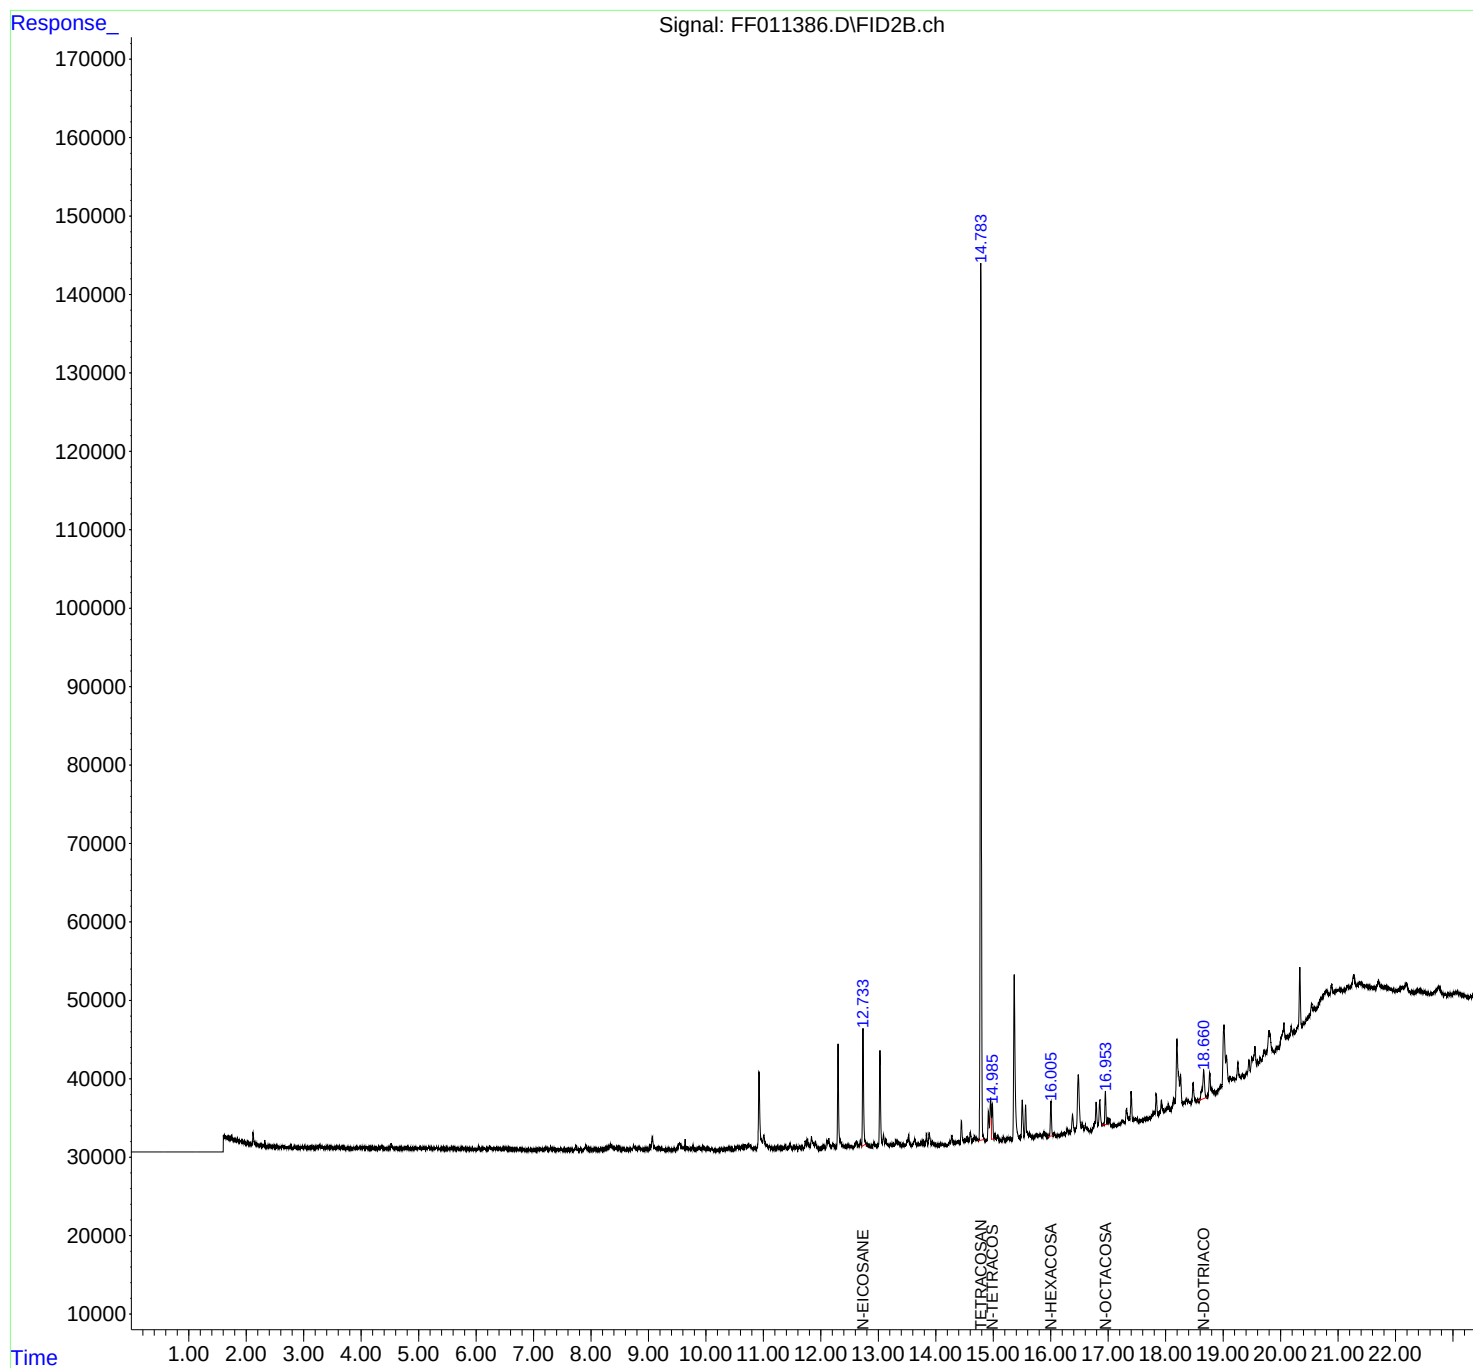


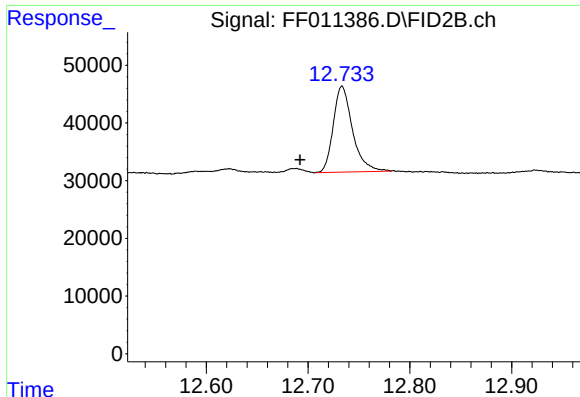

#7 N-EICOSANE


R.T.: 12.733 min
Delta R.T.: 0.041 min
Response: 195492
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

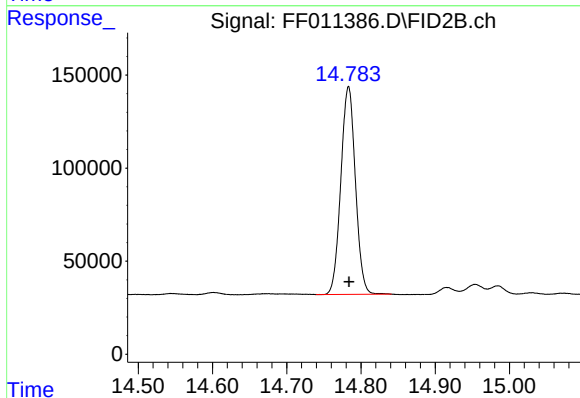


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 1524040
Conc: 13.60 ug/ml

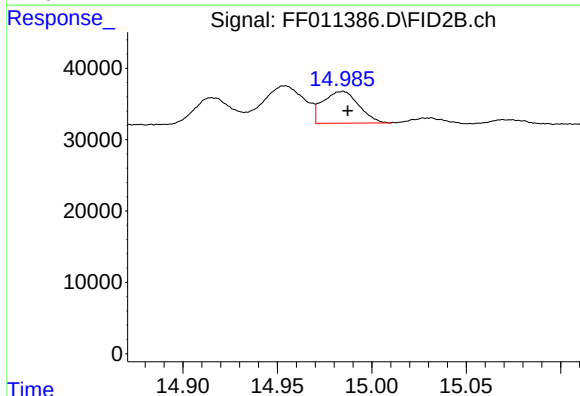


#10 N-TETRACOSANE

R.T.: 14.985 min
Delta R.T.: -0.003 min
Response: 59079
Conc: 0.46 ug/ml

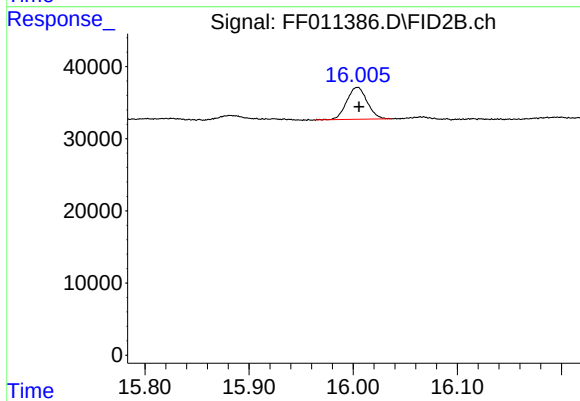

#11 N-HEXACOSANE


R.T.: 16.004 min
Delta R.T.: -0.002 min
Response: 60099
Conc: 0.48 ug/ml

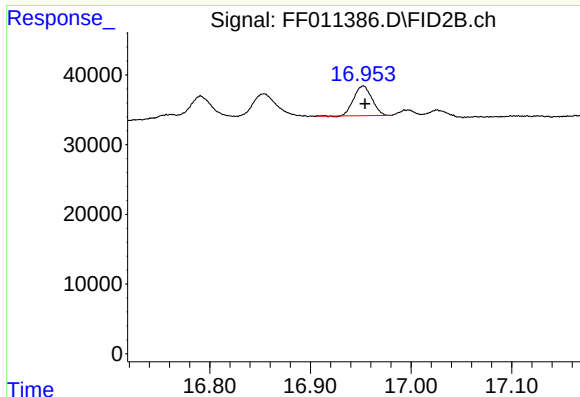

#12 N-OCTACOSANE

R.T.: 16.952 min
Delta R.T.: -0.002 min
Response: 53489
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

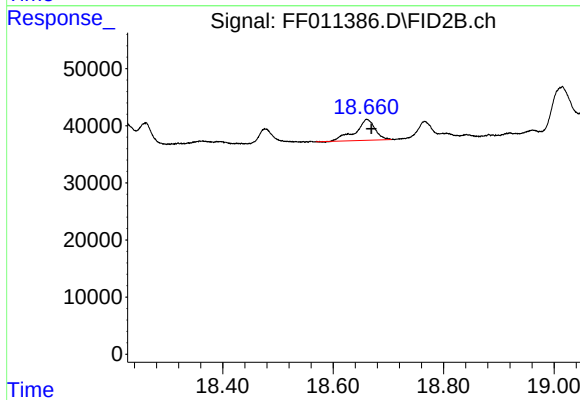

#14 N-DOTRIACONTANE

R.T.: 18.661 min
Delta R.T.: -0.009 min
Response: 90257
Conc: 0.76 ug/ml