

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011387.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 22:42
Operator : YP\AJ
Sample : N4501-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:23:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.782	1073686	9.579 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.984	92581	0.727 ug/ml
11) N-HEXACOSANE	16.003	64495	0.516 ug/ml
12) N-OCTACOSANE	16.951	48455	0.396 ug/ml
14) N-DOTRIACONTANE	18.662	99078	0.838 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090622\
Data File : FF011387.D
Signal(s) : FID2B.ch
Acq On : 06 Sep 2022 22:42
Operator : YP\AJ
Sample : N4501-16
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 07 03:23:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

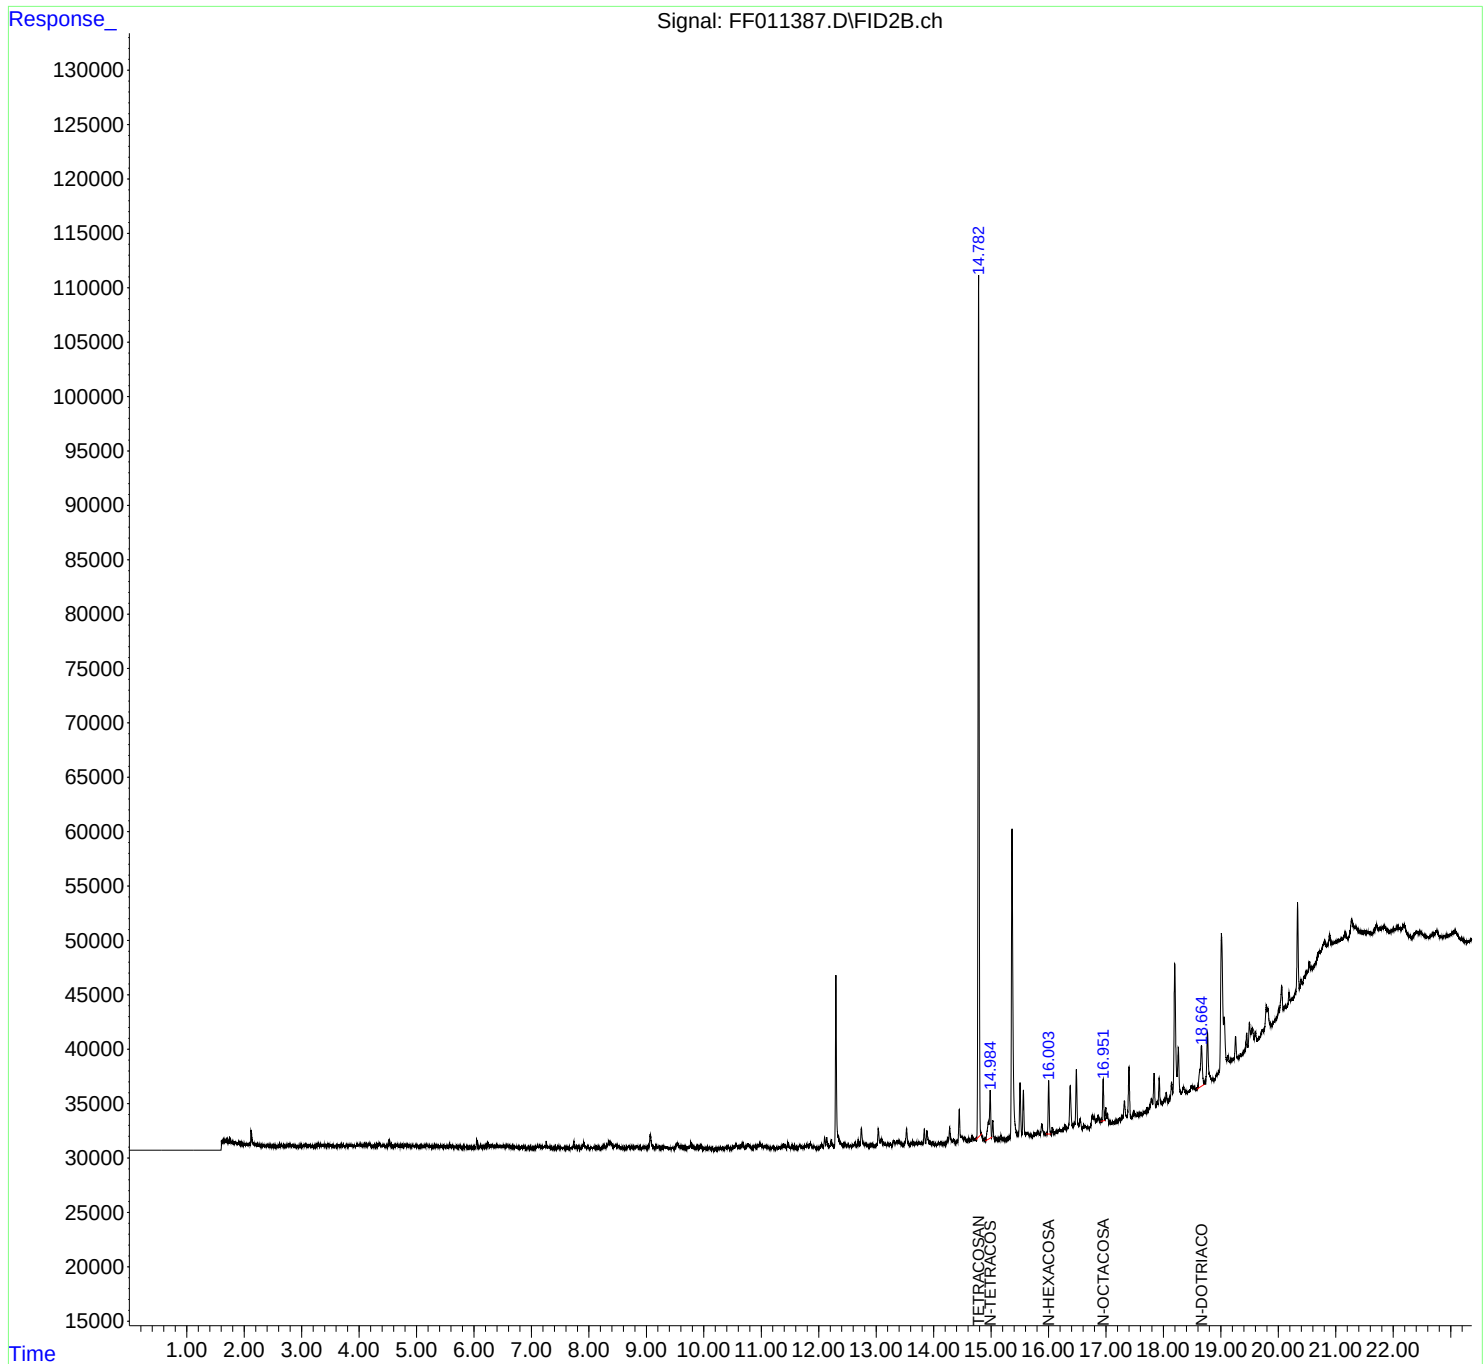


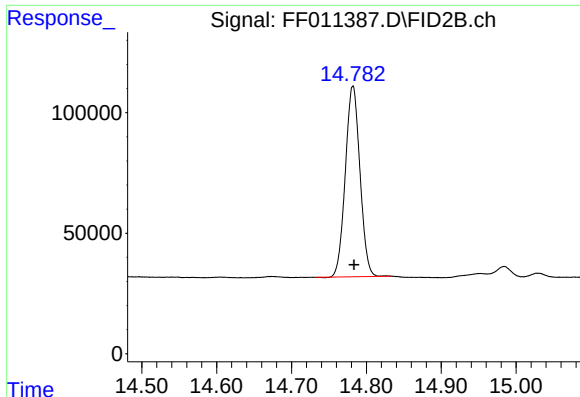

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.782 min
Delta R.T.: -0.002 min
Response: 1073686
Conc: 9.58 ug/ml

Instrument :
FID_F
ClientSampleId :

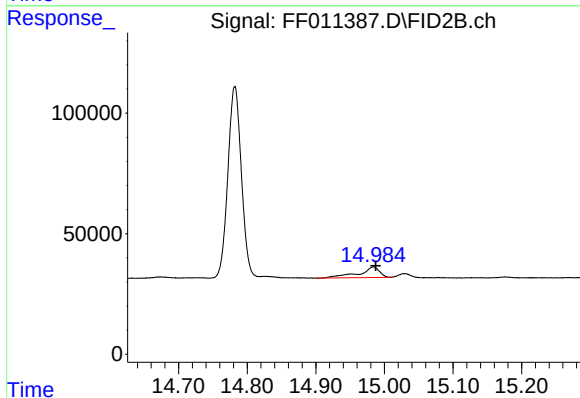


#10 N-TETRACOSANE

R.T.: 14.984 min
Delta R.T.: -0.003 min
Response: 92581
Conc: 0.73 ug/ml

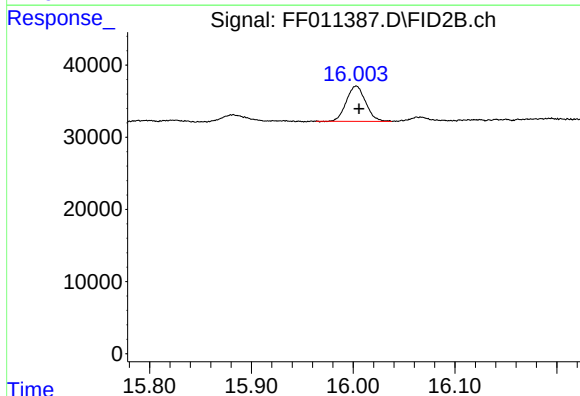


#11 N-HEXACOSANE

R.T.: 16.003 min
Delta R.T.: -0.003 min
Response: 64495
Conc: 0.52 ug/ml

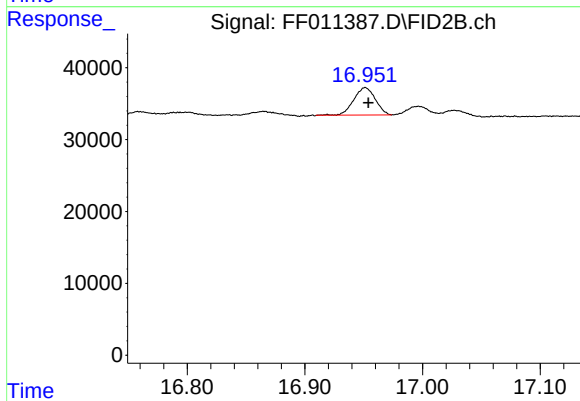

#12 N-OCTACOSANE

R.T.: 16.951 min
Delta R.T.: -0.003 min
Response: 48455
Conc: 0.40 ug/ml

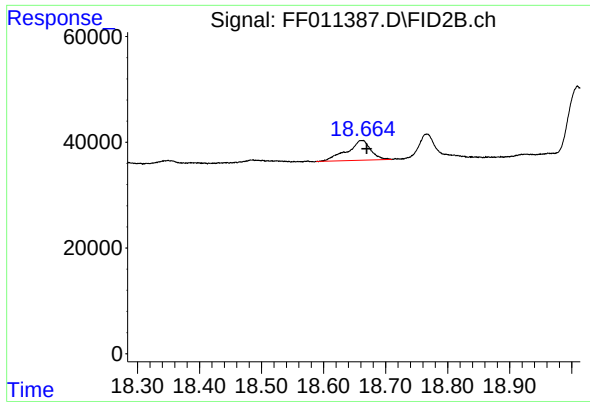

#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.008 min
Response: 99078
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :