

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
 Data File : FF002032.D
 Signal(s) : FID2B.ch
 Acq On : 07 Sep 2018 16:04
 Operator : AJ\SJ
 Sample : J4825-06
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 08 02:09:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.276	1618522	12.913 ug/ml
Target Compounds			
2) N-DECANE	4.073	246585	2.128 ug/ml
8) N-DOCOSANE	13.337	98551	0.692 ug/ml
10) N-TETRACOSANE	14.479	507957	3.579 ug/ml
11) N-HEXACOSANE	15.495	359744	2.529 ug/ml
12) N-OCTACOSANE	16.441	566178	3.946 ug/ml
13) N-TRIACONTANE	17.328	488105	3.366 ug/ml
14) N-DOTRIACONTANE	18.155	576756	4.091 ug/ml
15) N-TETRATRIACONTANE	18.939	160449	1.193 ug/ml
16) N-HEXATRIACONTANE	19.689	109276	0.877 ug/ml
17) N-OCTATRIACONTANE	20.381	334890	3.058 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
Data File : FF002032.D
Signal(s) : FID2B.ch
Acq On : 07 Sep 2018 16:04
Operator : AJ\SJ
Sample : J4825-06
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 08 02:09:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

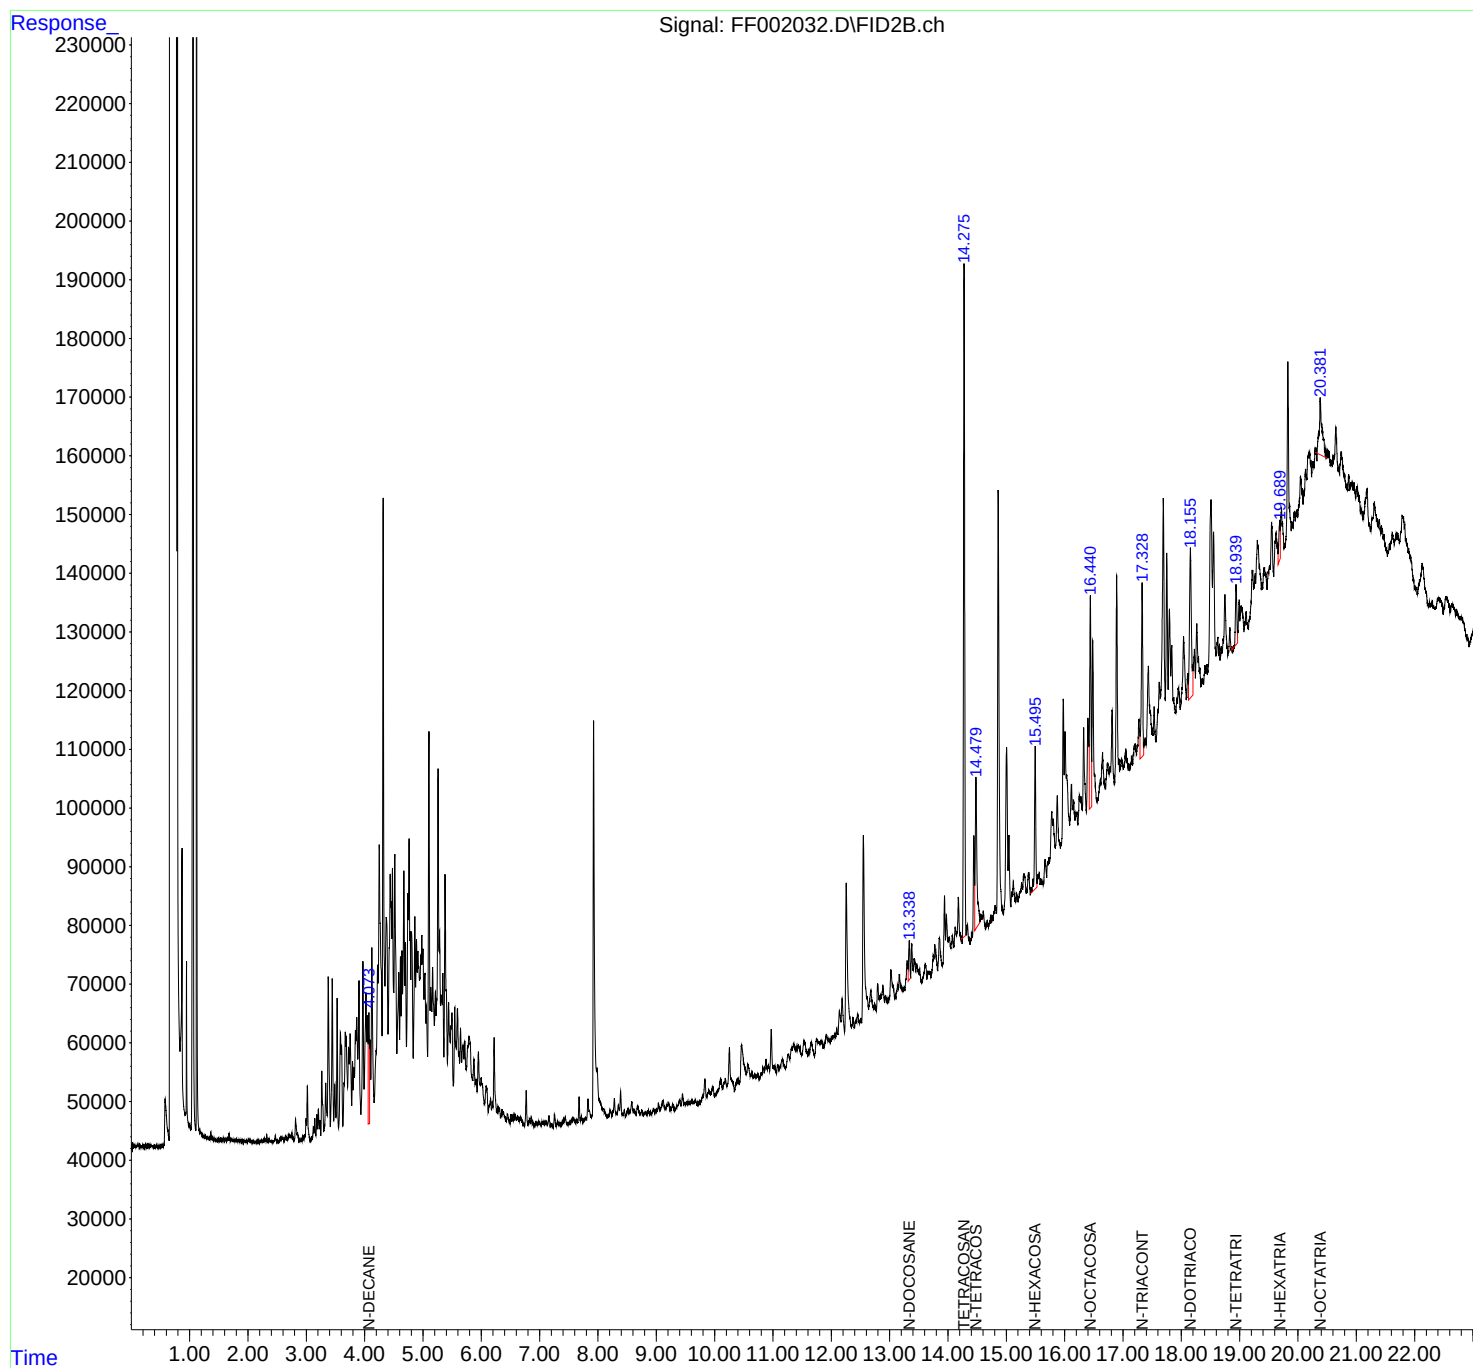

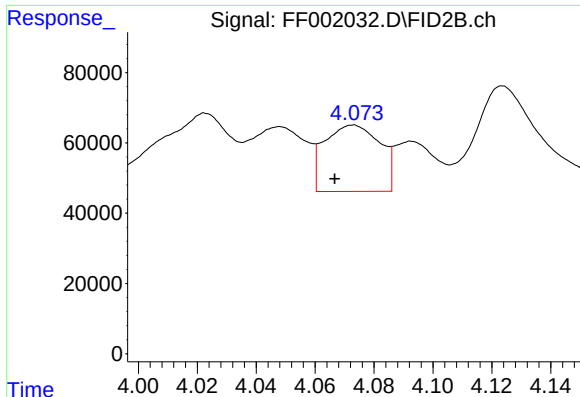


#2 N-DECANE

R.T.: 4.073 min
Delta R.T.: 0.006 min
Response: 246585
Conc: 2.13 ug/ml

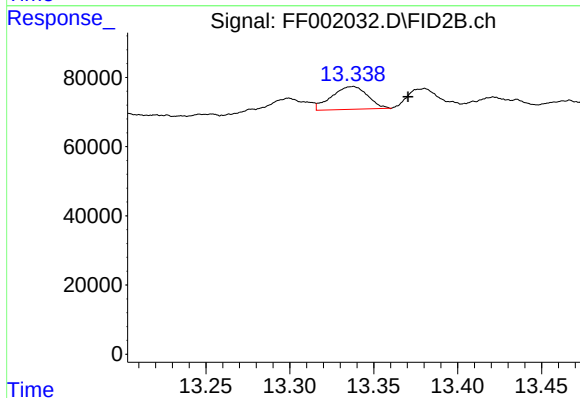


#8 N-DOCOSANE

R.T.: 13.337 min
Delta R.T.: -0.034 min
Response: 98551
Conc: 0.69 ug/ml

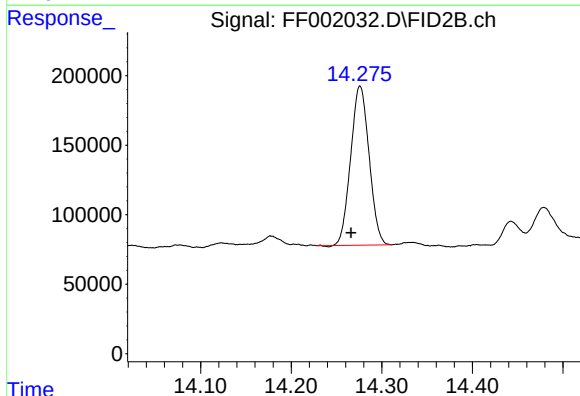


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.276 min
Delta R.T.: 0.010 min
Response: 1618522
Conc: 12.91 ug/ml

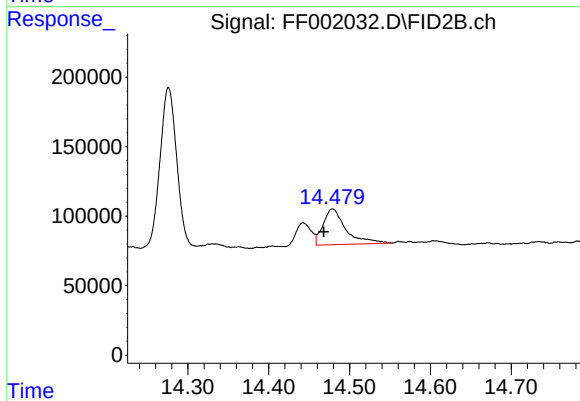


#10 N-TETRACOSANE

R.T.: 14.479 min
Delta R.T.: 0.011 min
Response: 507957
Conc: 3.58 ug/ml

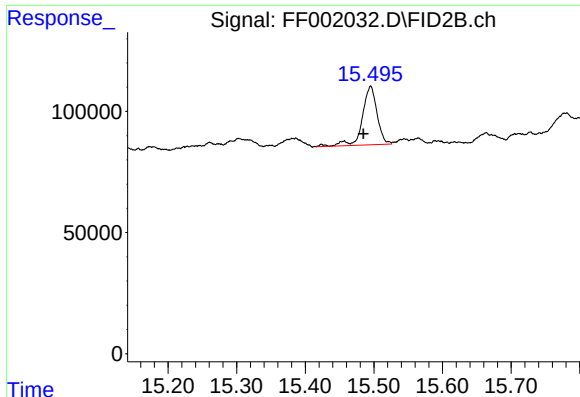


#11 N-HEXACOSANE

R.T.: 15.495 min
Delta R.T.: 0.010 min
Response: 359744
Conc: 2.53 ug/ml

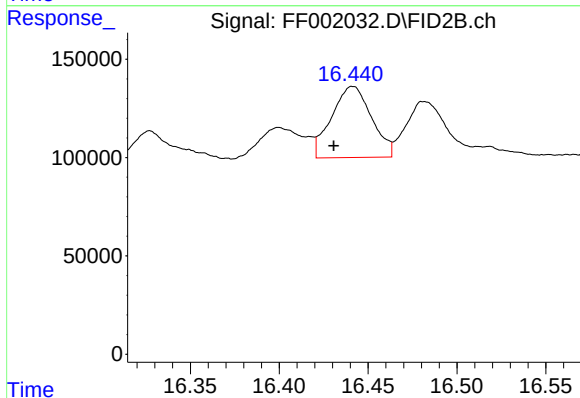


#12 N-OCTACOSANE

R.T.: 16.441 min
Delta R.T.: 0.010 min
Response: 566178
Conc: 3.95 ug/ml

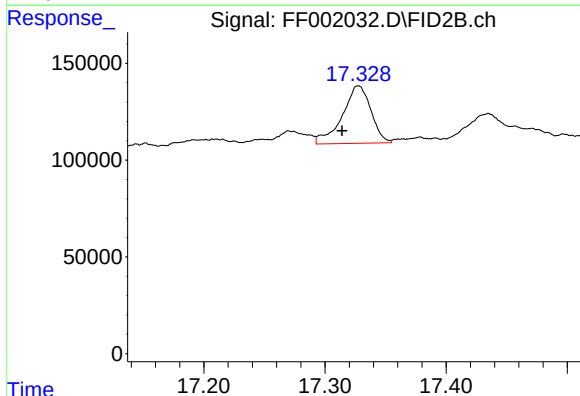


#13 N-TRIACONTANE

R.T.: 17.328 min
Delta R.T.: 0.014 min
Response: 488105
Conc: 3.37 ug/ml

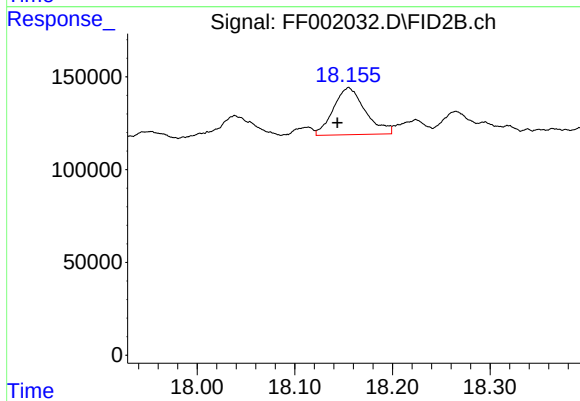

#14 N-DOTRIACONTANE

R.T.: 18.155 min
Delta R.T.: 0.011 min
Response: 576756
Conc: 4.09 ug/ml

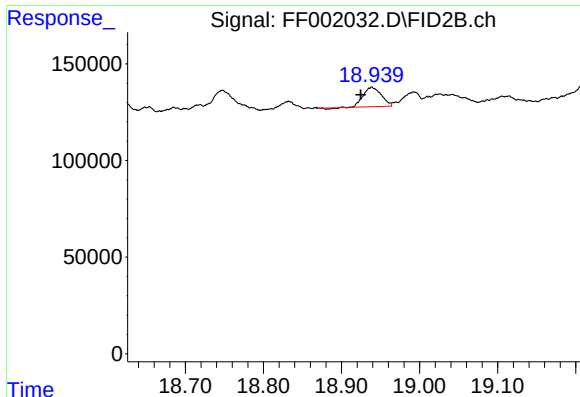


#15 N-TETRATRIACONTANE

R.T.: 18.939 min

Delta R.T.: 0.014 min

Response: 160449

Conc: 1.19 ug/ml

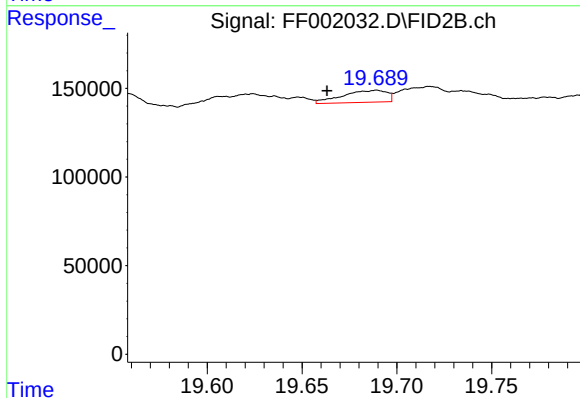


#16 N-HEXATRIACONTANE

R.T.: 19.689 min

Delta R.T.: 0.025 min

Response: 109276

Conc: 0.88 ug/ml

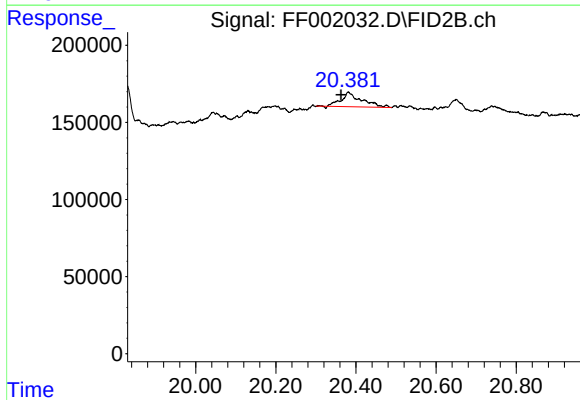

#17 N-OCTATRIACONTANE

R.T.: 20.381 min

Delta R.T.: 0.019 min

Response: 334890

Conc: 3.06 ug/ml