

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
Data File : FF002048.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2018 00:06
Operator : AJ\SJ
Sample : J4825-01 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 08 02:15:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.276	157579	1.257 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.327	117589	0.811 ug/ml
14)	N-DOTRIACONTANE	18.157	96168	0.682 ug/ml
15)	N-TETRATRIACONTANE	18.940	36357	0.270 ug/ml
16)	N-HEXATRIACONTANE	19.681	13131	0.105 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
Data File : FF002048.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2018 00:06
Operator : AJ\SJ
Sample : J4825-01 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 08 02:15:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

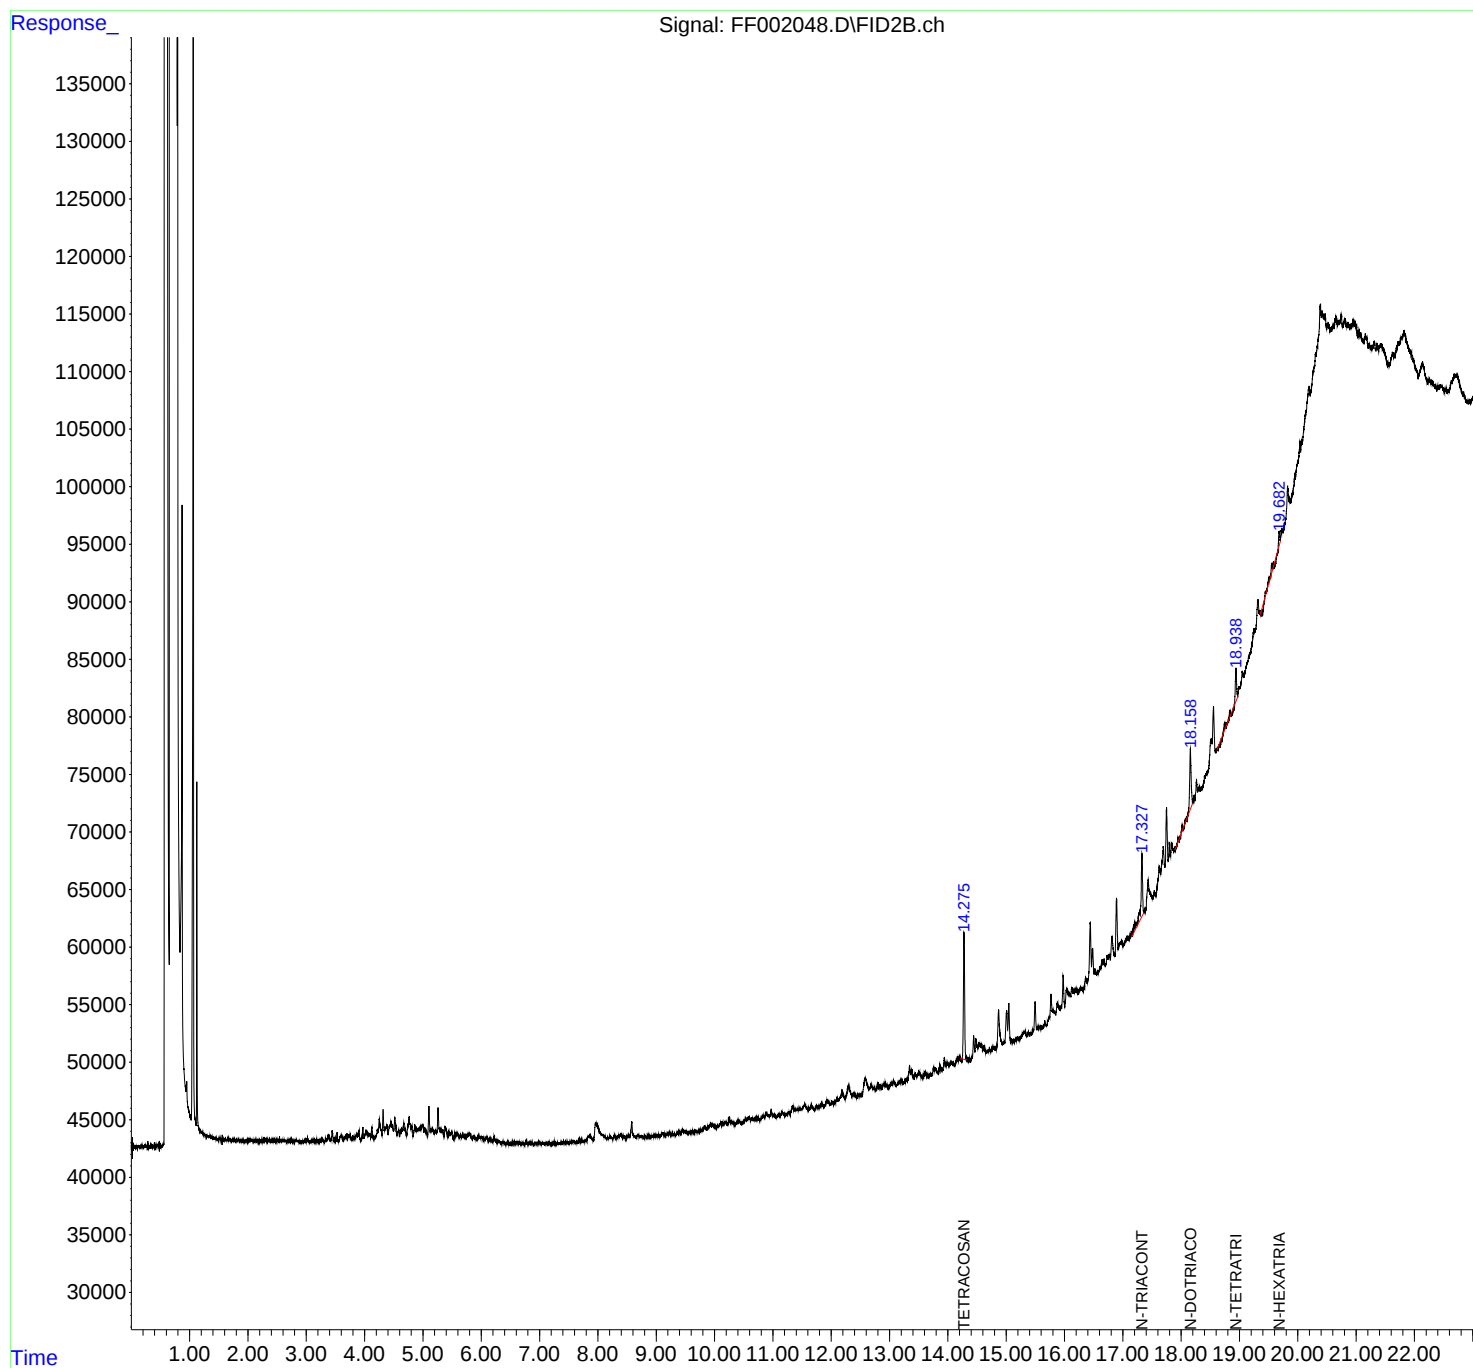

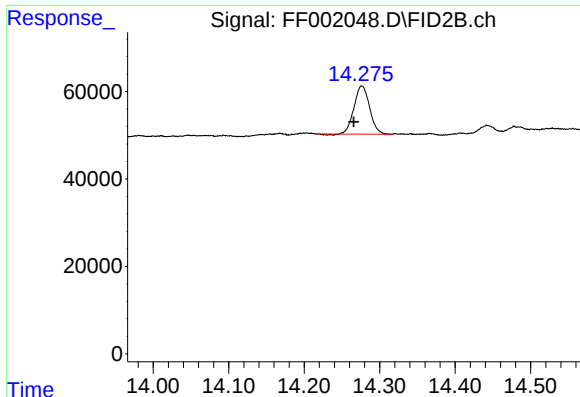


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.276 min
Delta R.T.: 0.011 min
Response: 157579
Conc: 1.26 ug/ml

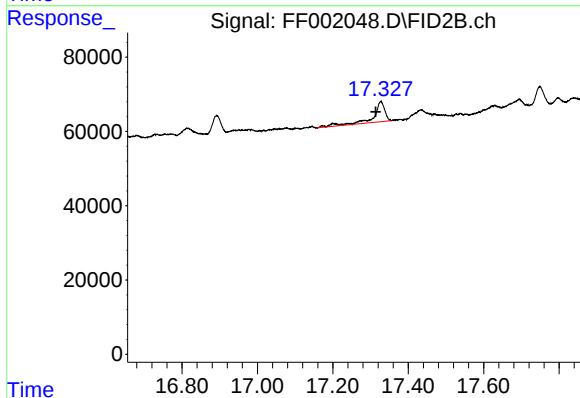


#13 N-TRIACONTANE

R.T.: 17.327 min
Delta R.T.: 0.013 min
Response: 117589
Conc: 0.81 ug/ml

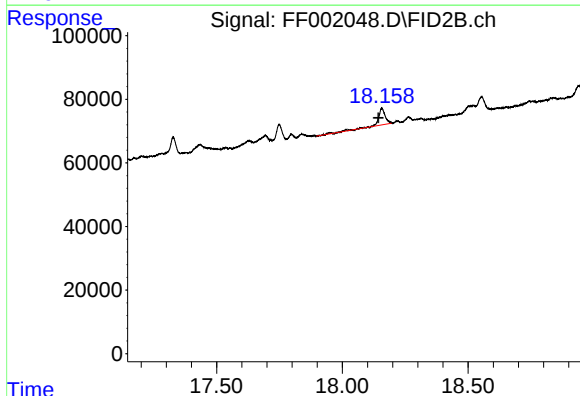


#14 N-DOTRIACONTANE

R.T.: 18.157 min
Delta R.T.: 0.014 min
Response: 96168
Conc: 0.68 ug/ml

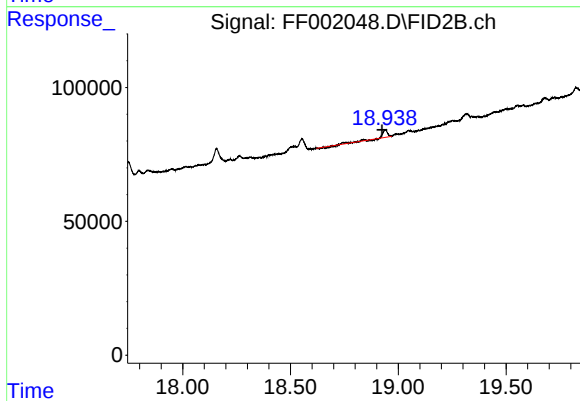

#15 N-TETRATRIACONTANE

R.T.: 18.940 min
Delta R.T.: 0.015 min
Response: 36357
Conc: 0.27 ug/ml

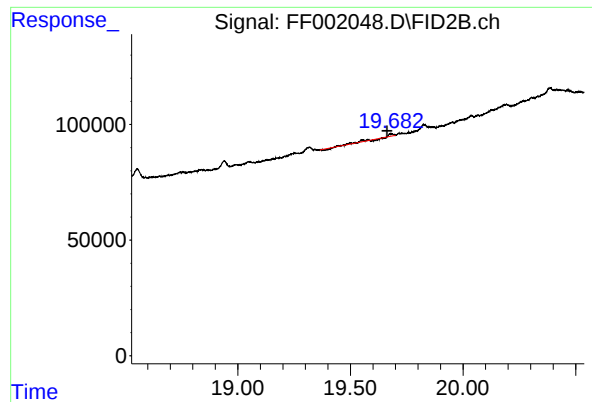

#16 N-HEXATRIACONTANE

R.T.: 19.681 min
Delta R.T.: 0.018 min
Response: 13131
Conc: 0.11 ug/ml