

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
 Data File : FF002060.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2018 06:09
 Operator : AJ\SJ
 Sample : J4825-15 2X
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 10 01:54:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.275	854580	6.818 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.484	681986	4.806 ug/ml
11)	N-HEXACOSANE	15.494	139917	0.984 ug/ml
12)	N-OCTACOSANE	16.440	555319	3.871 ug/ml
13)	N-TRIACONTANE	17.328	1636700	11.287 ug/ml
14)	N-DOTRIACONTANE	18.160	3186893	22.605 ug/ml
15)	N-TETRATRIACONTANE	18.941	1958569	14.564 ug/ml
16)	N-HEXATRIACONTANE	19.678	733989	5.894 ug/ml
17)	N-OCTATRIACONTANE	20.379	284824	2.601 ug/ml
18)	N-TETRACONTANE	21.178	518581	4.898 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
Data File : FF002060.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2018 06:09
Operator : AJ\SJ
Sample : J4825-15 2X
Misc :
ALS Vial : 85 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 10 01:54:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

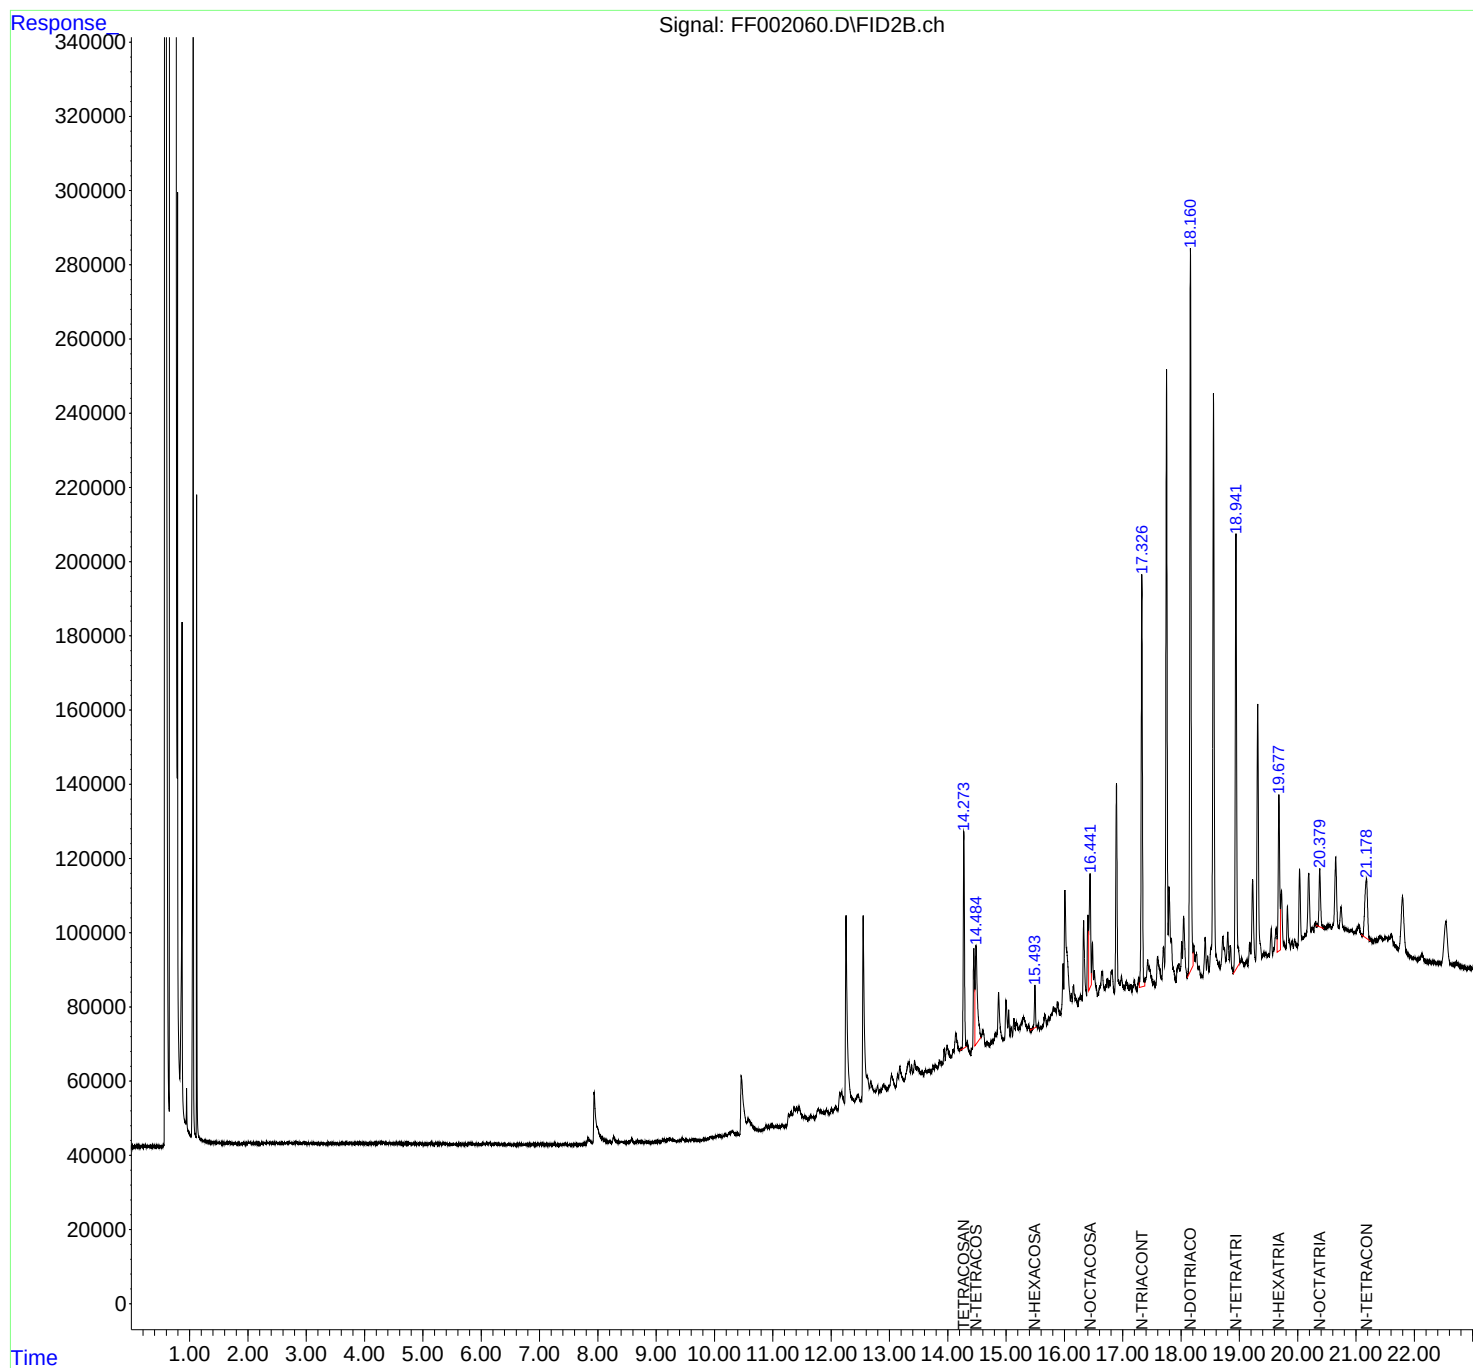

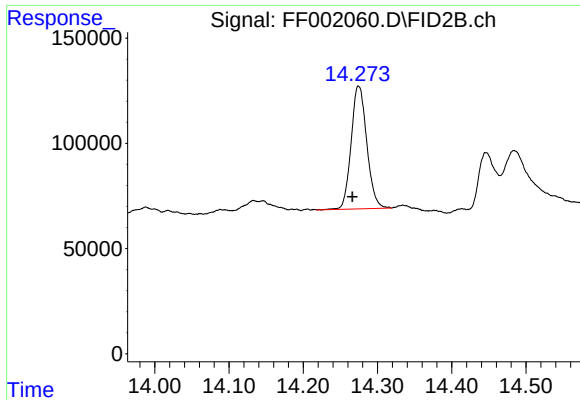


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.275 min
Delta R.T.: 0.009 min
Response: 854580
Conc: 6.82 ug/ml

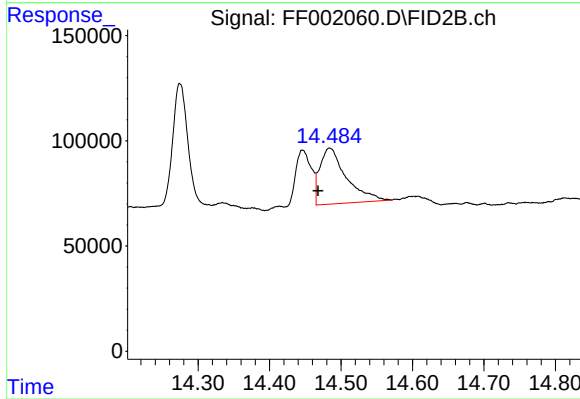


#10 N-TETRACOSANE

R.T.: 14.484 min
Delta R.T.: 0.016 min
Response: 681986
Conc: 4.81 ug/ml

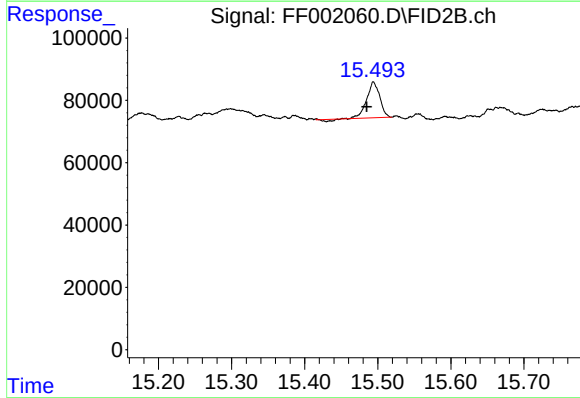


#11 N-HEXACOSANE

R.T.: 15.494 min
Delta R.T.: 0.009 min
Response: 139917
Conc: 0.98 ug/ml

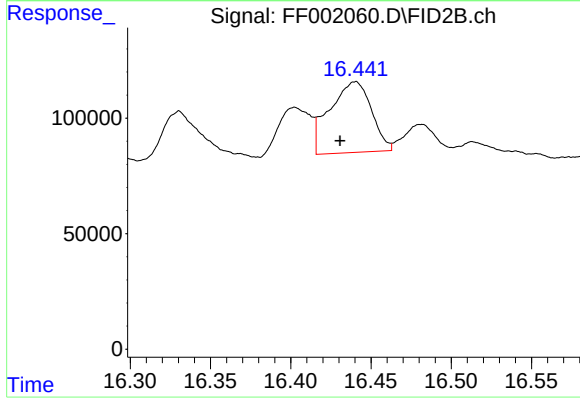


#12 N-OCTACOSANE

R.T.: 16.440 min
Delta R.T.: 0.009 min
Response: 555319
Conc: 3.87 ug/ml

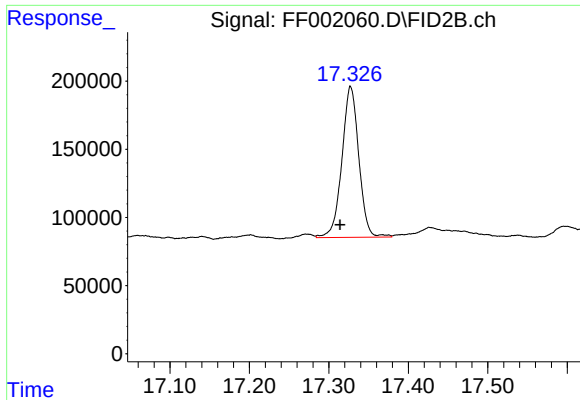


#13 N-TRIACONTANE

R.T.: 17.328 min
Delta R.T.: 0.013 min
Response: 1636700
Conc: 11.29 ug/ml

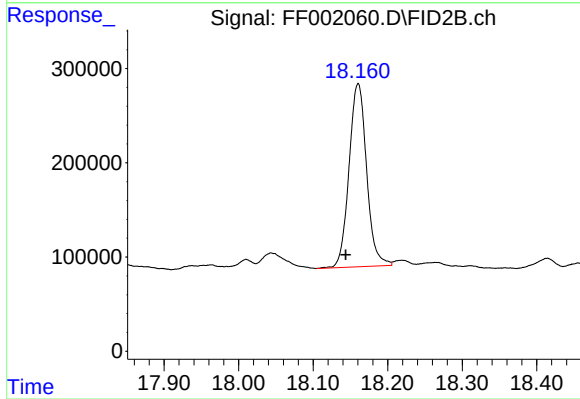


#14 N-DOTRIACONTANE

R.T.: 18.160 min
Delta R.T.: 0.017 min
Response: 3186893
Conc: 22.60 ug/ml

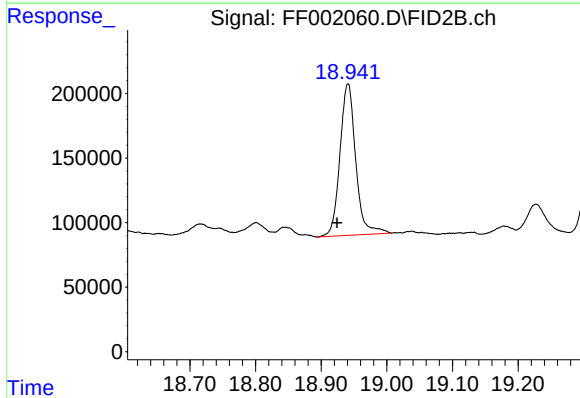


#15 N-TETRATRIACONTANE

R.T.: 18.941 min
Delta R.T.: 0.016 min
Response: 1958569
Conc: 14.56 ug/ml

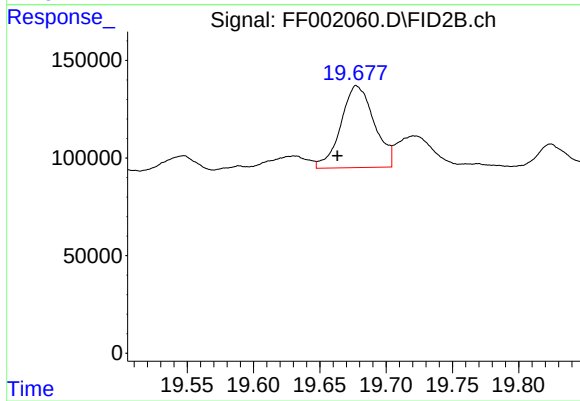


#16 N-HEXATRIACONTANE

R.T.: 19.678 min
Delta R.T.: 0.015 min
Response: 733989
Conc: 5.89 ug/ml

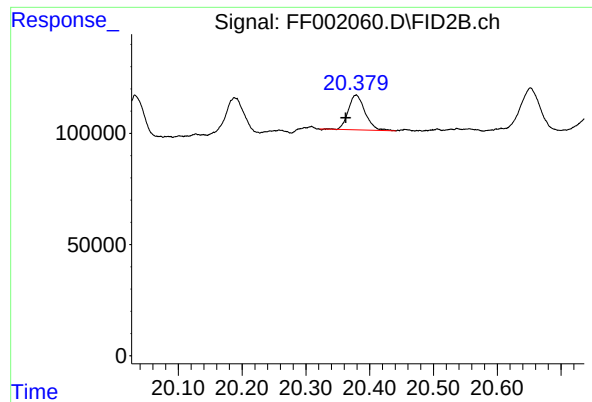

#17 N-OCTATRIACONTANE

R.T.: 20.379 min
Delta R.T.: 0.016 min
Response: 284824
Conc: 2.60 ug/ml

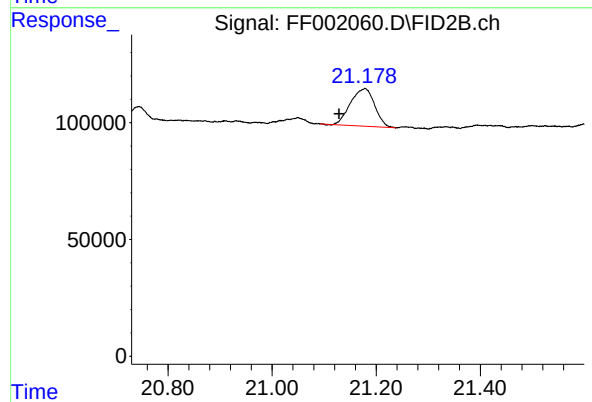

#18 N-TETRACONTANE

R.T.: 21.178 min
Delta R.T.: 0.049 min
Response: 518581
Conc: 4.90 ug/ml