

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
 Data File : FF002063.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2018 07:40
 Operator : AJ\SJ
 Sample : J4825-09 2X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 10 01:55:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:20:53 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.275	880377	7.024 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.449	304096	2.143 ug/ml
11)	N-HEXACOSANE	15.494	106993	0.752 ug/ml
12)	N-OCTACOSANE	16.439	288757	2.013 ug/ml
13)	N-TRIACONTANE	17.327	330242	2.277 ug/ml
14)	N-DOTRIACONTANE	18.158	597027	4.235 ug/ml
15)	N-TETRATRIACONTANE	18.940	805929	5.993 ug/ml
16)	N-HEXATRIACONTANE	19.679	652901	5.242 ug/ml
17)	N-OCTATRIACONTANE	20.379	1179214	10.769 ug/ml
18)	N-TETRACONTANE	21.179	449121	4.242 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090718\
Data File : FF002063.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2018 07:40
Operator : AJ\SJ
Sample : J4825-09 2X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 10 01:55:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

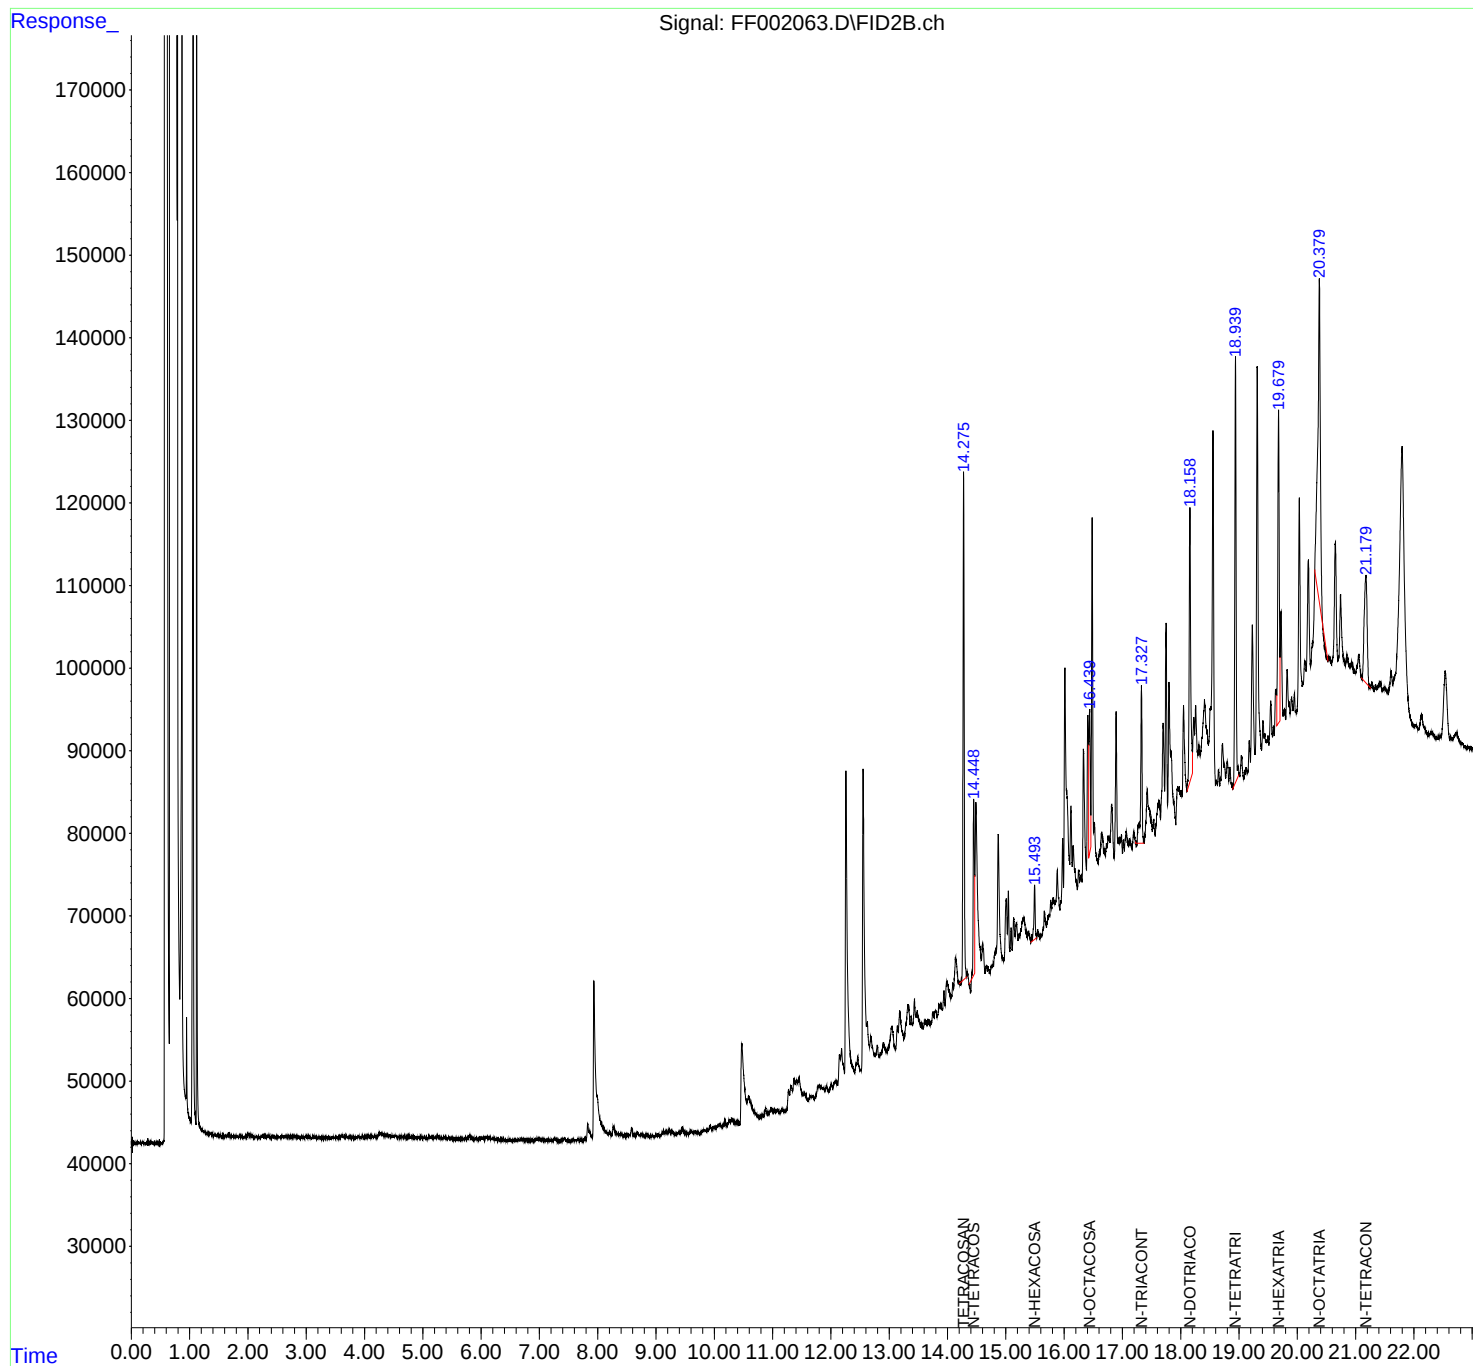

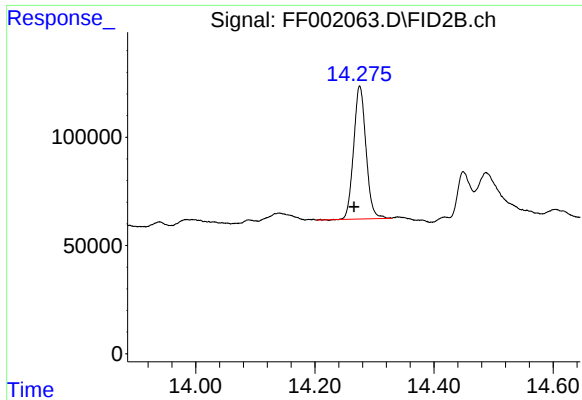


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.275 min
Delta R.T.: 0.009 min
Response: 880377
Conc: 7.02 ug/ml

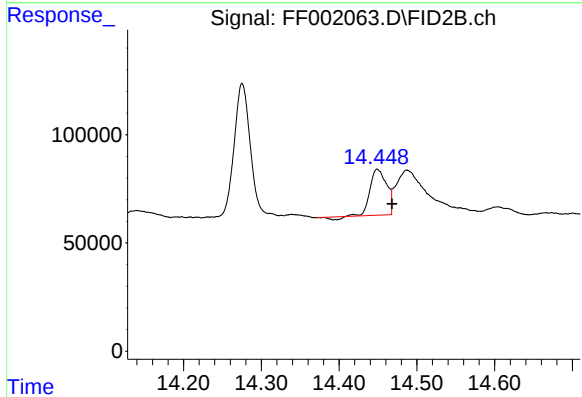


#10 N-TETRACOSANE

R.T.: 14.449 min
Delta R.T.: -0.019 min
Response: 304096
Conc: 2.14 ug/ml

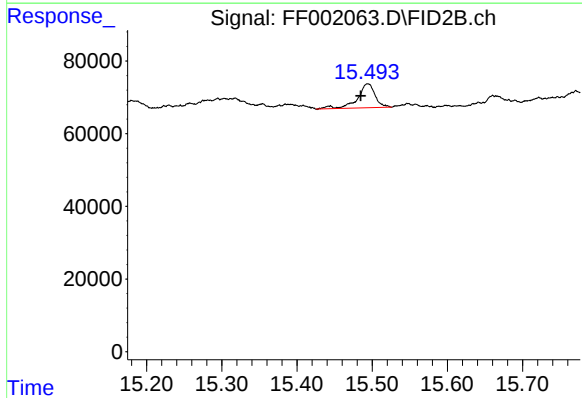


#11 N-HEXACOSANE

R.T.: 15.494 min
Delta R.T.: 0.009 min
Response: 106993
Conc: 0.75 ug/ml

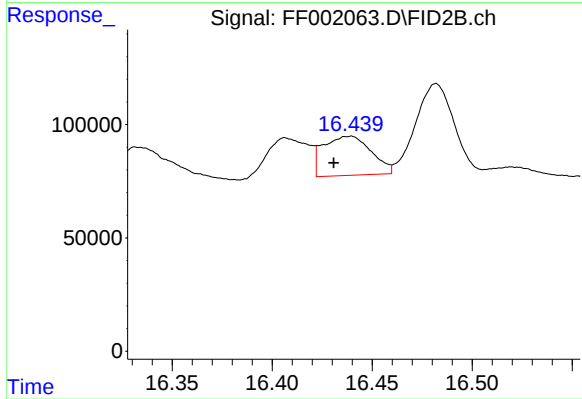


#12 N-OCTACOSANE

R.T.: 16.439 min
Delta R.T.: 0.008 min
Response: 288757
Conc: 2.01 ug/ml

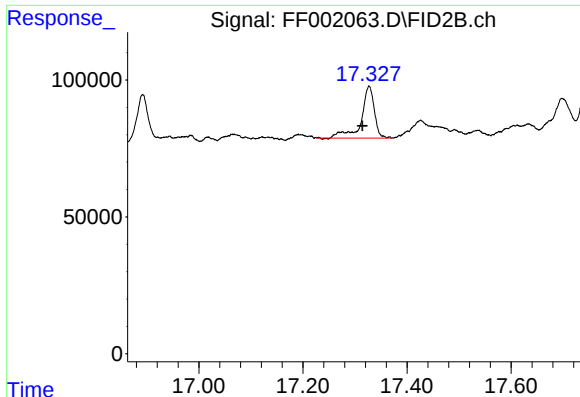


#13 N-TRIACONTANE

R.T.: 17.327 min
Delta R.T.: 0.013 min
Response: 330242
Conc: 2.28 ug/ml

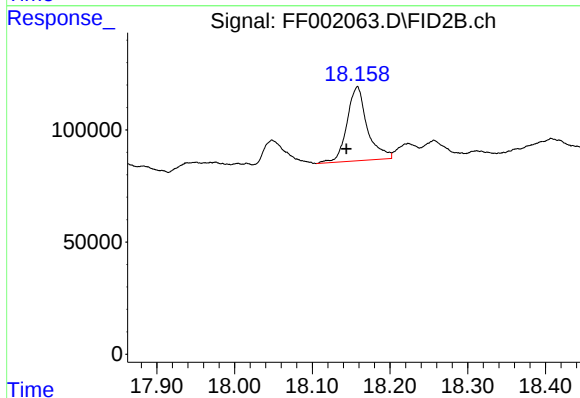


#14 N-DOTRIACONTANE

R.T.: 18.158 min
Delta R.T.: 0.014 min
Response: 597027
Conc: 4.23 ug/ml

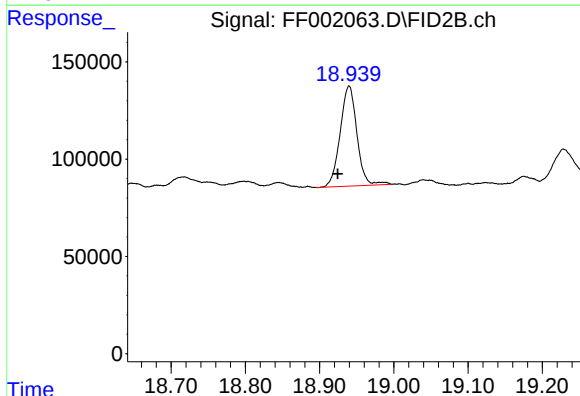


#15 N-TETRATRIACONTANE

R.T.: 18.940 min
Delta R.T.: 0.015 min
Response: 805929
Conc: 5.99 ug/ml

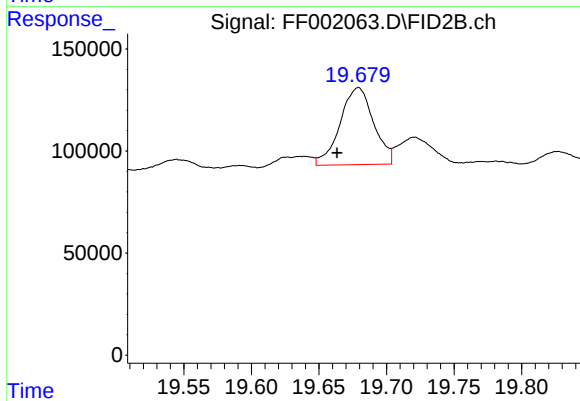


#16 N-HEXATRIACONTANE

R.T.: 19.679 min
Delta R.T.: 0.016 min
Response: 652901
Conc: 5.24 ug/ml

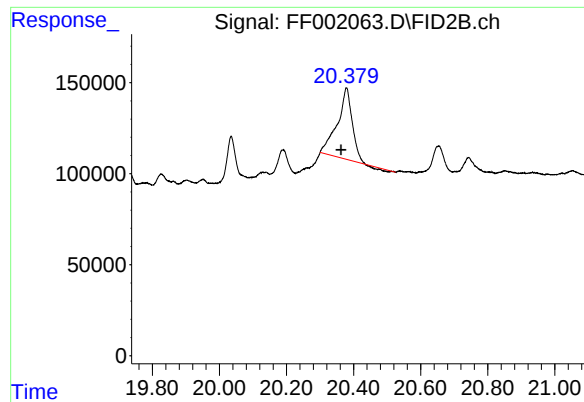

#17 N-OCTATRIACONTANE

R.T.: 20.379 min
Delta R.T.: 0.016 min
Response: 1179214
Conc: 10.77 ug/ml

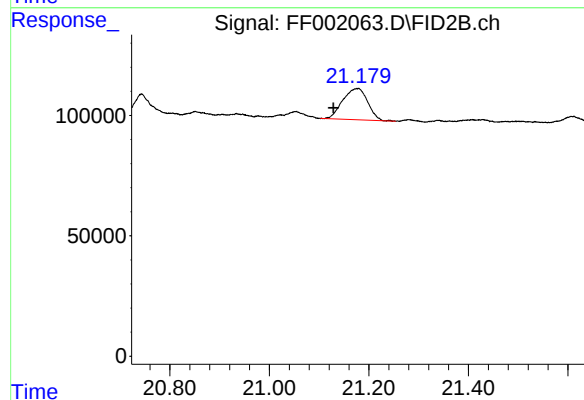

#18 N-TETRACONTANE

R.T.: 21.179 min
Delta R.T.: 0.050 min
Response: 449121
Conc: 4.24 ug/ml