

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090722\
Data File : FF011393.D
Signal(s) : FID2B.ch
Acq On : 07 Sep 2022 12:22
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 08 02:19:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.511	1966146	15.014 ug/ml
12)	N-OCTACOSANE	16.952	1888641	15.419 ug/ml
13)	N-TRIACONTANE	17.837	237590	1.969 ug/ml
14)	N-DOTRIACONTANE	18.667	340657	2.880 ug/ml
15)	N-TETRATRIACONTANE	19.448	308674	2.704 ug/ml
16)	N-HEXATRIACONTANE	20.185	214748	2.018 ug/ml
17)	N-OCTATRIACONTANE	20.889	143252	1.377 ug/ml
18)	N-TETRACONTANE	21.704	99967	0.947 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090722\
Data File : FF011393.D
Signal(s) : FID2B.ch
Acq On : 07 Sep 2022 12:22
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 08 02:19:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

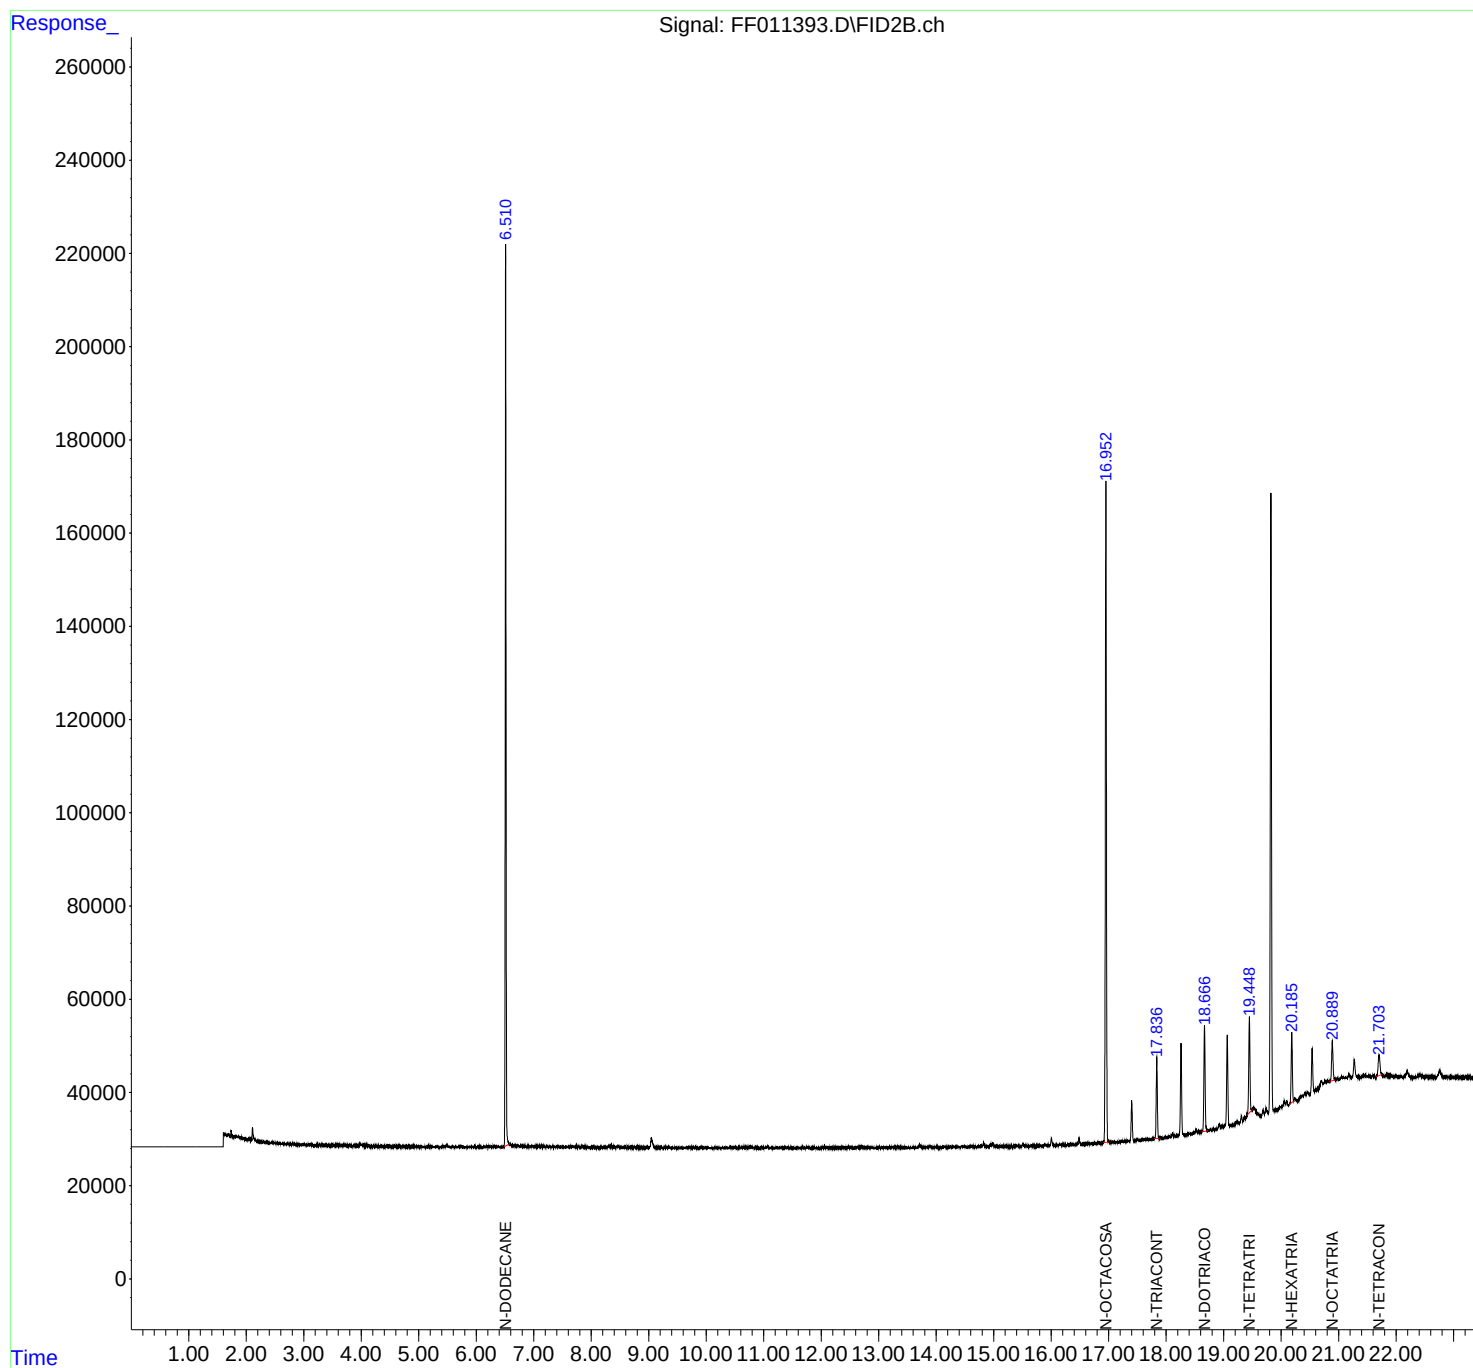


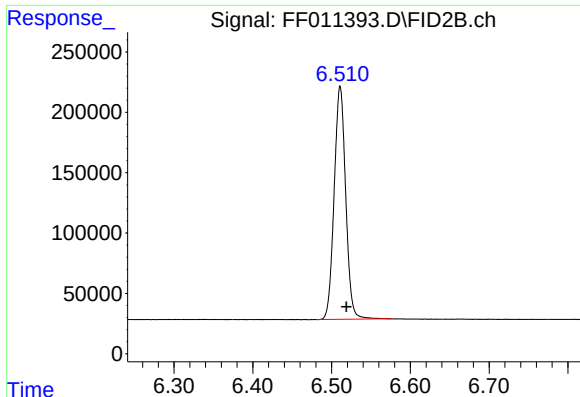

#3 N-DODECANE


R.T.: 6.511 min
Delta R.T.: -0.008 min
Response: 1966146
Conc: 15.01 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

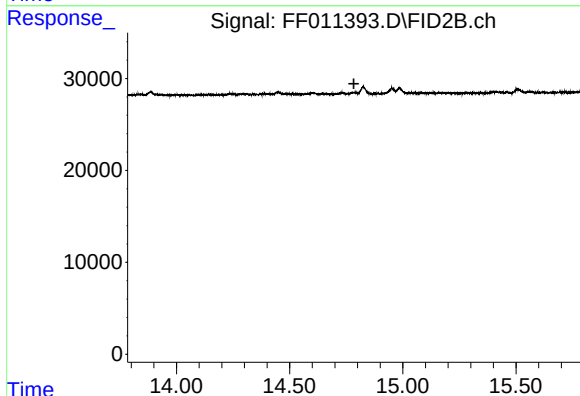


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

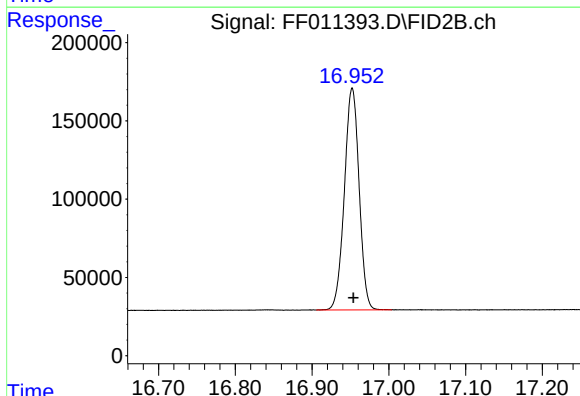


#12 N-OCTACOSANE

R.T.: 16.952 min
Delta R.T.: -0.002 min
Response: 1888641
Conc: 15.42 ug/ml

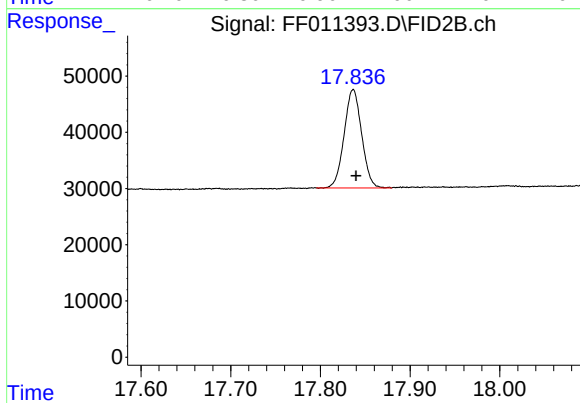

#13 N-TRIACONTANE


R.T.: 17.837 min
Delta R.T.: -0.003 min
Response: 237590
Conc: 1.97 ug/ml

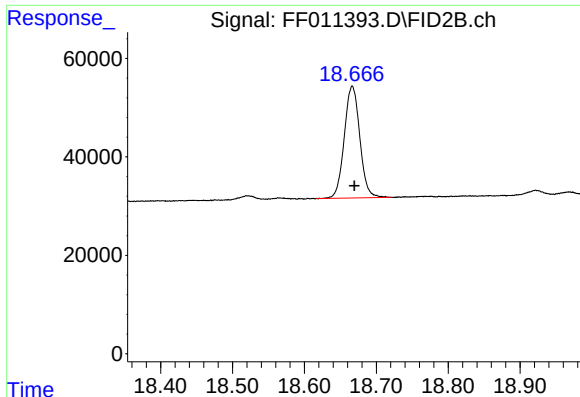

#14 N-DOTRIACONTANE


R.T.: 18.667 min
Delta R.T.: -0.003 min
Response: 340657
Conc: 2.88 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

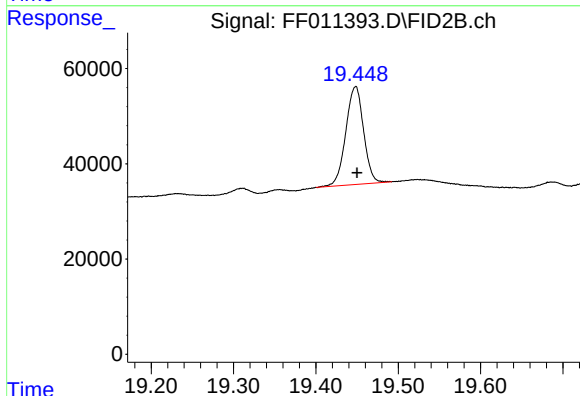


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.002 min
Response: 308674
Conc: 2.70 ug/ml

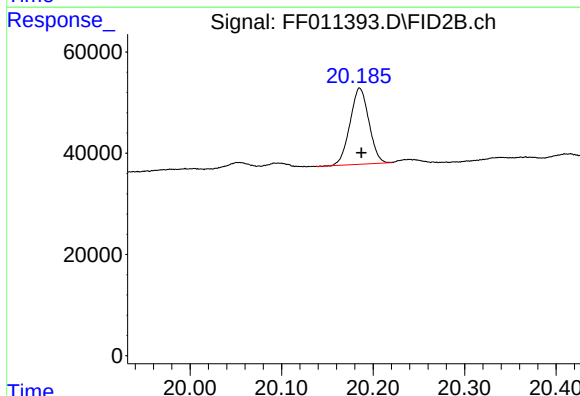


#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: -0.002 min
Response: 214748
Conc: 2.02 ug/ml

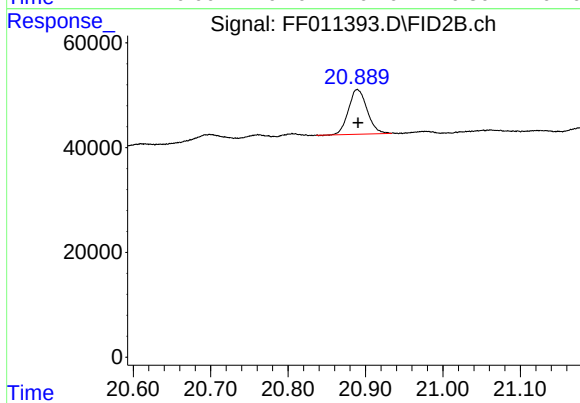

#17 N-OCTATRIACONTANE

R.T.: 20.889 min
Delta R.T.: -0.001 min
Response: 143252
Conc: 1.38 ug/ml

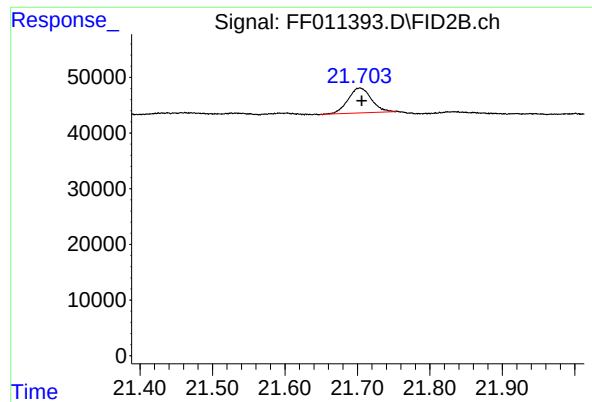

#18 N-TETRACONTANE

R.T.: 21.704 min
Delta R.T.: -0.002 min
Response: 99967
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER