

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090722\
Data File : FF011394.D
Signal(s) : FID2B.ch
Acq On : 07 Sep 2022 13:29
Operator : YP\AJ
Sample : PB147504BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB147504BL

Integration File: autoint1.e
Quant Time: Sep 08 02:20:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.782	2013911	17.967 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.668	55214	0.467 ug/ml
15)	N-TETRATRIACONTANE	19.448	62522	0.548 ug/ml
16)	N-HEXATRIACONTANE	20.186	75248	0.707 ug/ml
17)	N-OCTATRIACONTANE	20.890	91806	0.883 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090722\
Data File : FF011394.D
Signal(s) : FID2B.ch
Acq On : 07 Sep 2022 13:29
Operator : YP\AJ
Sample : PB147504BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB147504BL

Integration File: autoint1.e
Quant Time: Sep 08 02:20:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

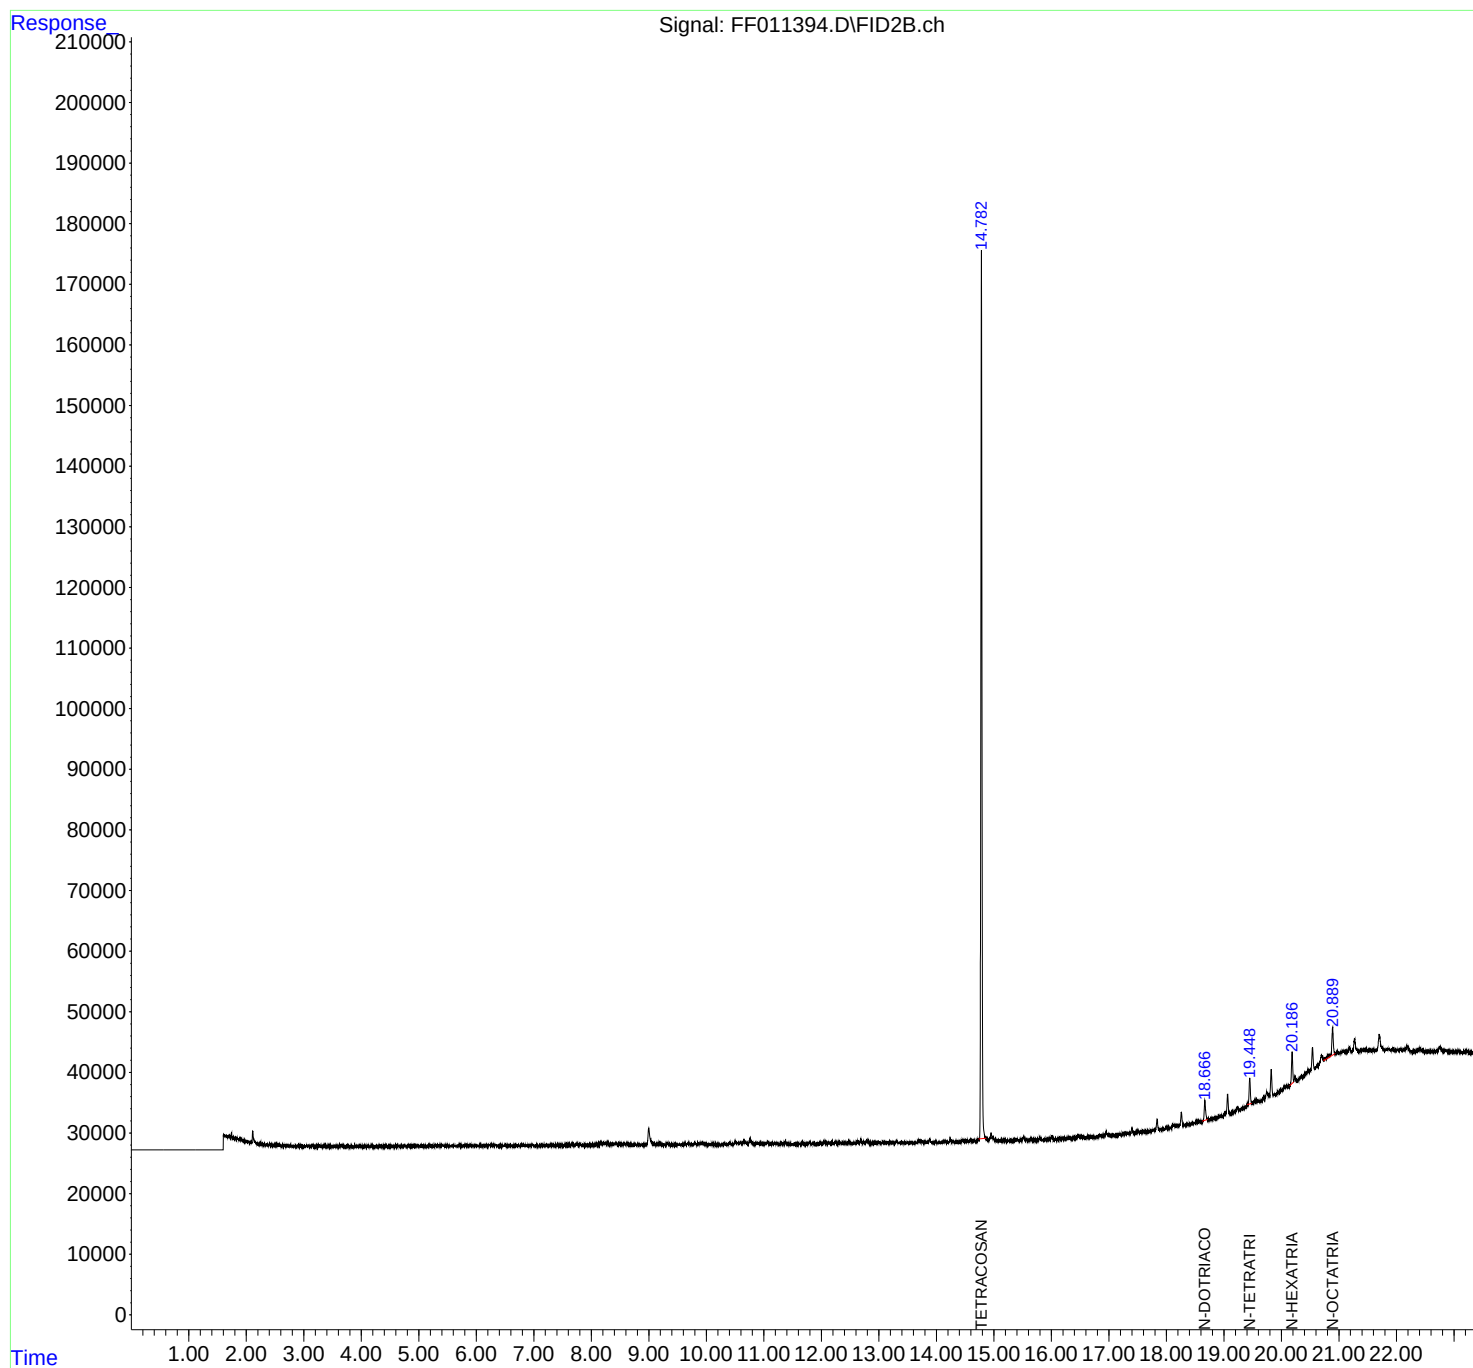


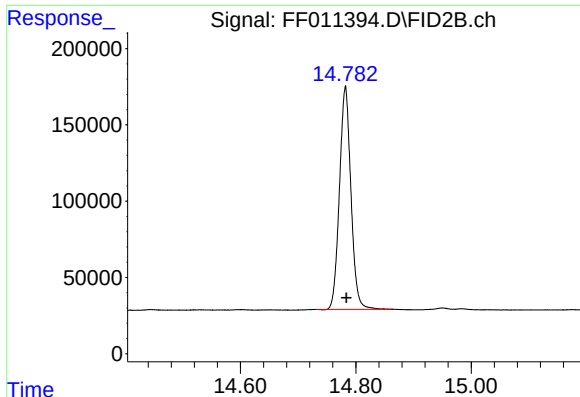

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.782 min
Delta R.T.: -0.002 min
Response: 2013911
Conc: 17.97 ug/ml

Instrument :
FID_F
ClientSampleId :
PB147504BL

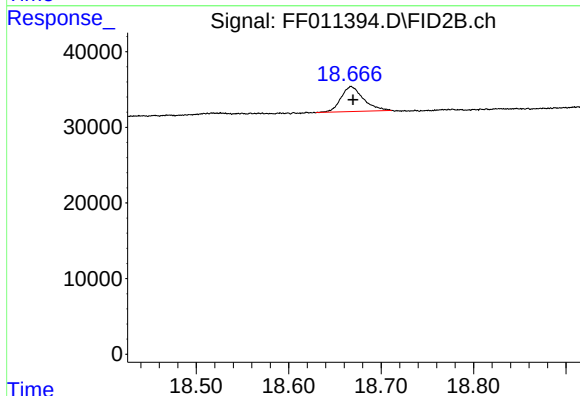


#14 N-DOTRIACONTANE

R.T.: 18.668 min
Delta R.T.: -0.002 min
Response: 55214
Conc: 0.47 ug/ml

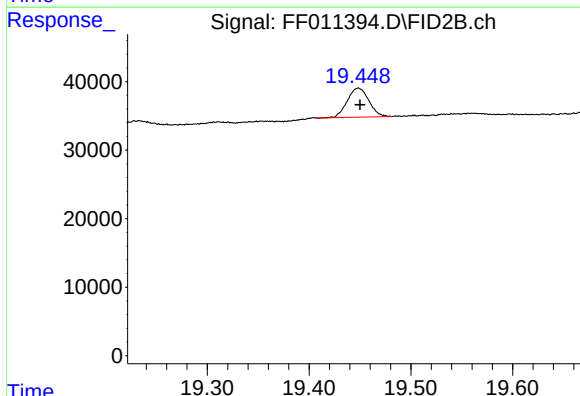


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.002 min
Response: 62522
Conc: 0.55 ug/ml

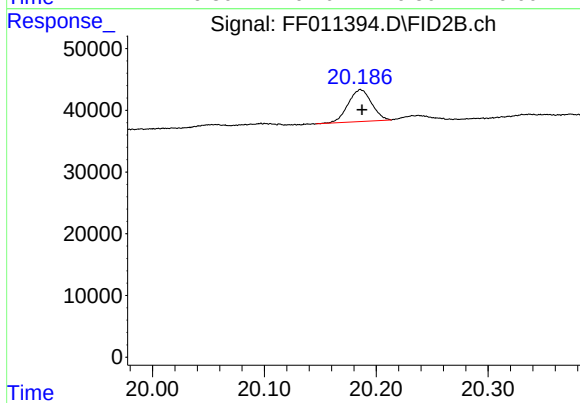

#16 N-HEXATRIACONTANE

R.T.: 20.186 min
Delta R.T.: -0.001 min
Response: 75248
Conc: 0.71 ug/ml

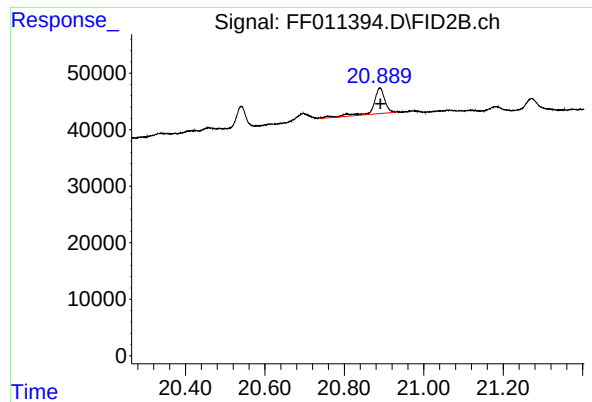

#17 N-OCTATRIACONTANE

R.T.: 20.890 min
Delta R.T.: 0.000 min
Response: 91806
Conc: 0.88 ug/ml

Instrument :

FID_F

ClientSampleId :

PB147504BL