

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
 Data File : FF007475.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2020 13:19
 Operator : DD\AJ
 Sample : L3808-05
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 09 01:22:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	2353632	16.003 ug/ml
Target Compounds			
4) N-TETRADECANE	8.329	501359	3.047 ug/ml
6) N-OCTADECANE	11.316	106335	0.624 ug/ml
7) N-EICOSANE	12.629	160015	0.952 ug/ml
8) N-DOCOSANE	13.831	57815	0.351 ug/ml
10) N-TETRACOSANE	14.919	400484	2.455 ug/ml
11) N-HEXACOSANE	15.961	957688	6.058 ug/ml
12) N-OCTACOSANE	16.916	1584104	10.322 ug/ml
13) N-TRIACONTANE	17.807	496407	3.359 ug/ml
14) N-DOTRIACONTANE	18.642	245272	1.768 ug/ml
18) N-TETRACONTANE	21.924	242124	2.182 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007475.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 13:19
Operator : DD\AJ
Sample : L3808-05
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:22:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

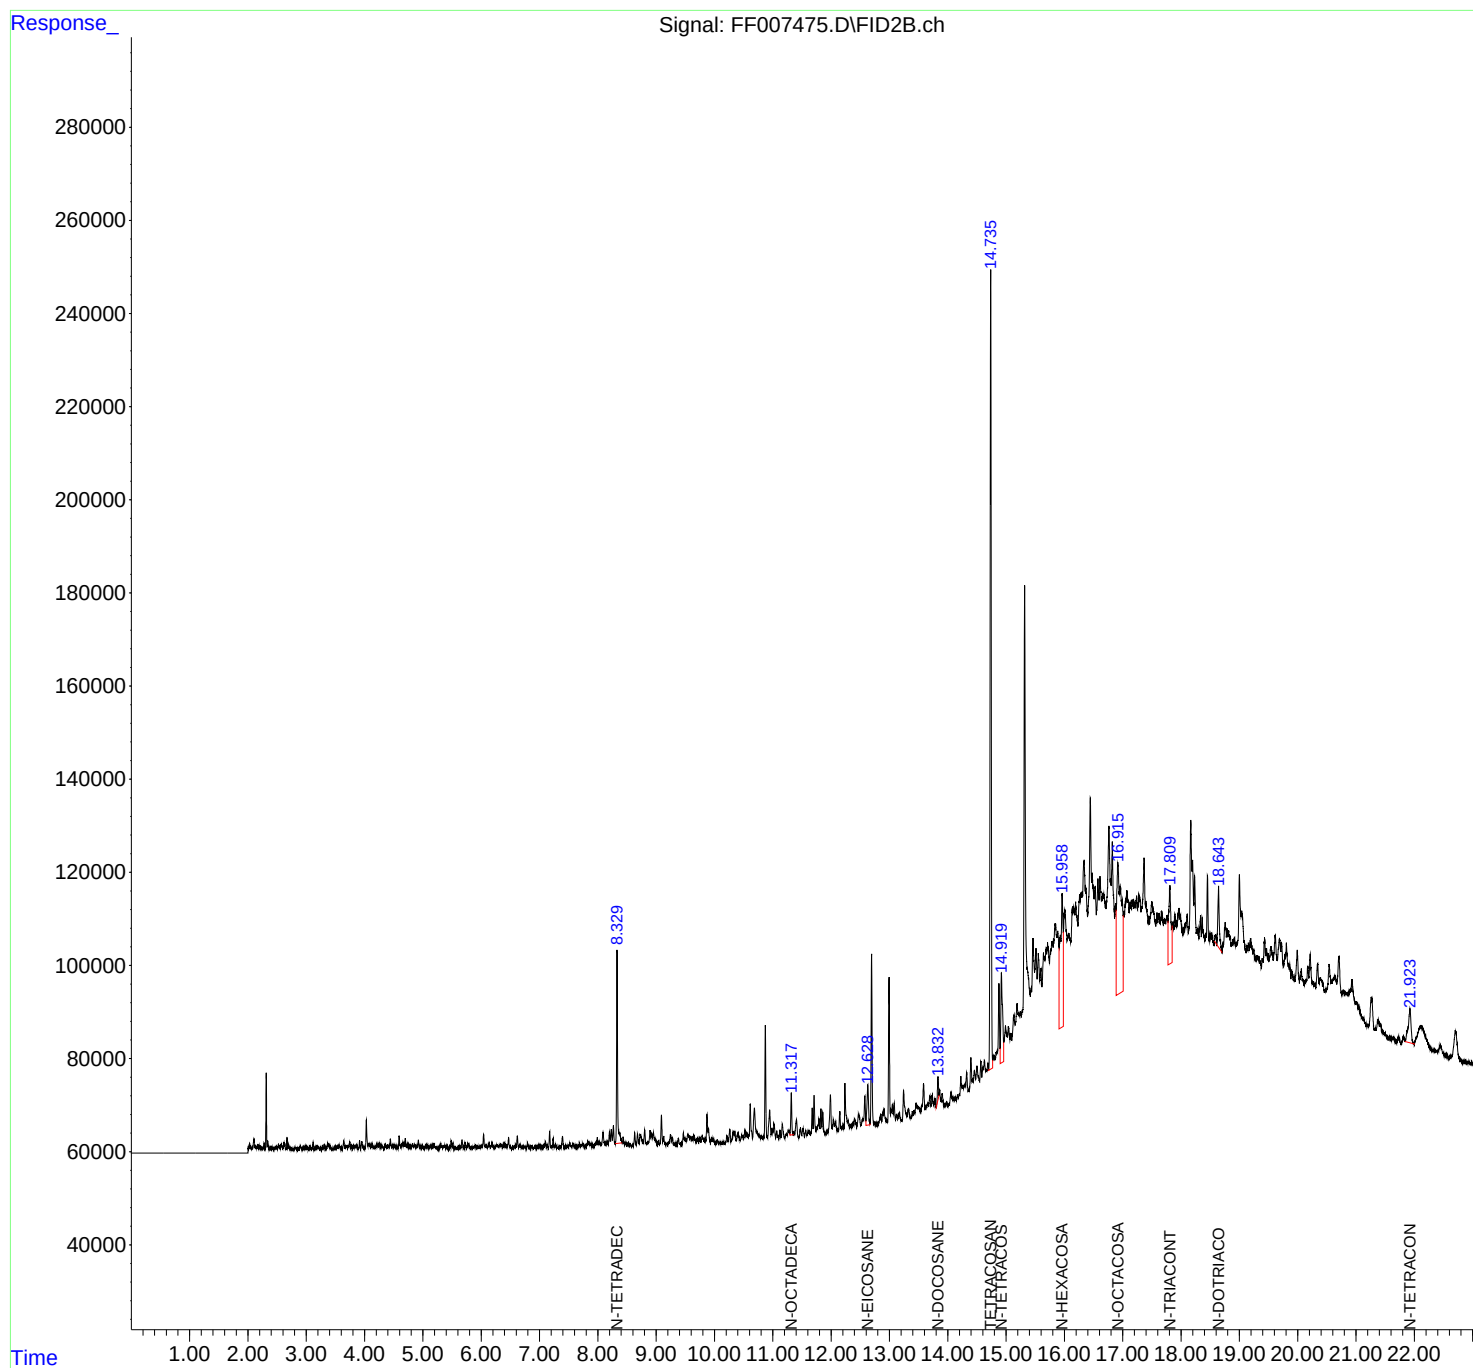

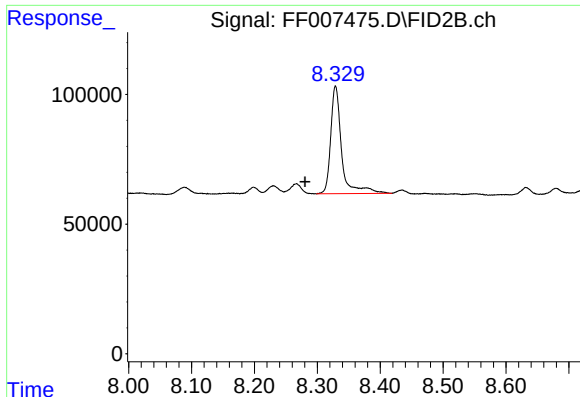


#4 N-TETRADECANE

R.T.: 8.329 min
Delta R.T.: 0.048 min
Response: 501359
Conc: 3.05 ug/ml

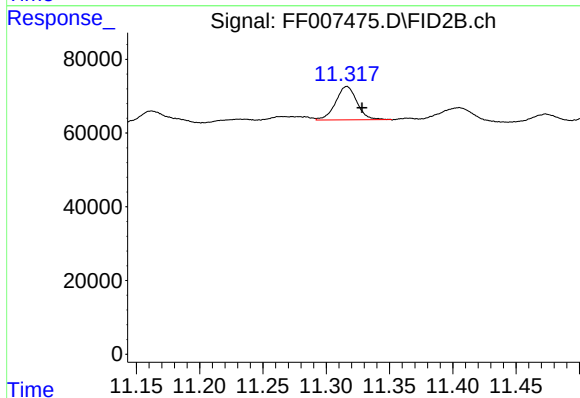


#6 N-OCTADECANE

R.T.: 11.316 min
Delta R.T.: -0.012 min
Response: 106335
Conc: 0.62 ug/ml

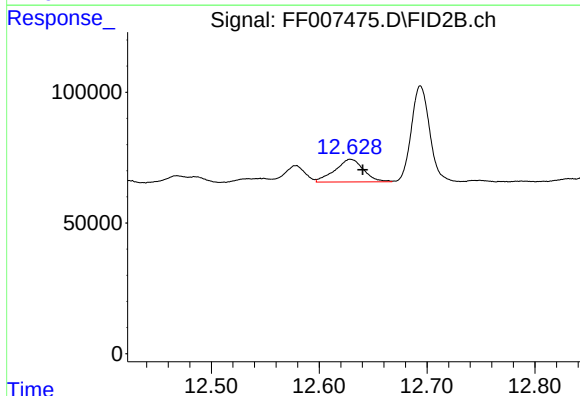


#7 N-EICOSANE

R.T.: 12.629 min
Delta R.T.: -0.011 min
Response: 160015
Conc: 0.95 ug/ml

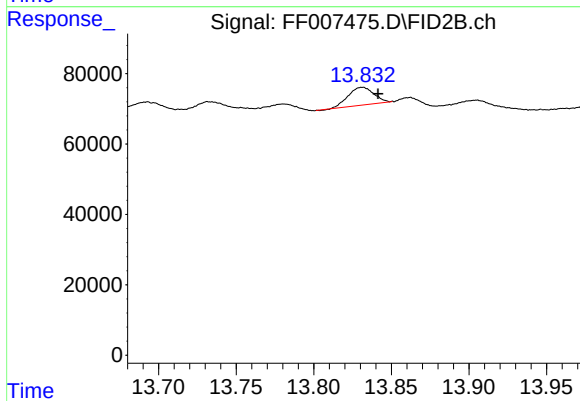


#8 N-DOCOSANE

R.T.: 13.831 min
Delta R.T.: -0.010 min
Response: 57815
Conc: 0.35 ug/ml

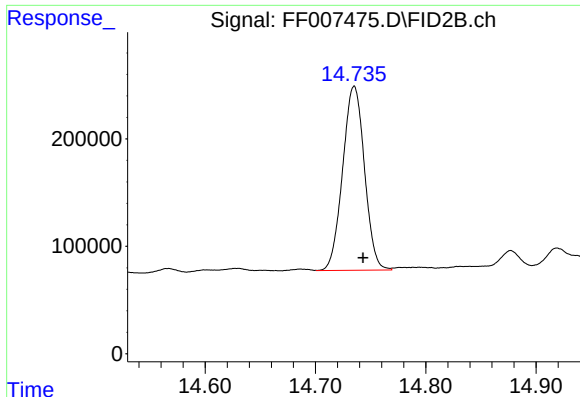


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.008 min
Response: 2353632
Conc: 16.00 ug/ml

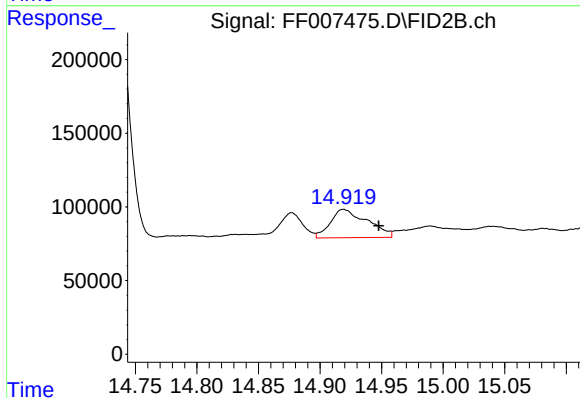


#10 N-TETRACOSANE

R.T.: 14.919 min
Delta R.T.: -0.028 min
Response: 400484
Conc: 2.46 ug/ml

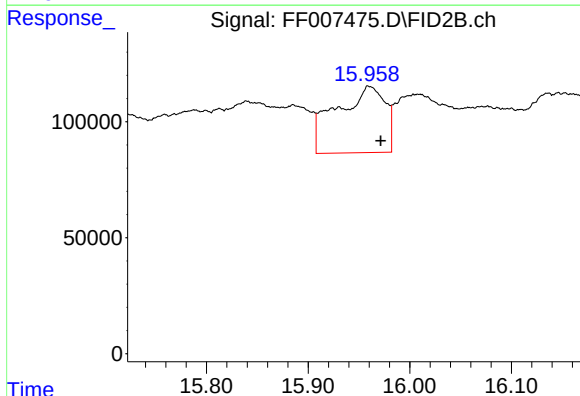


#11 N-HEXACOSANE

R.T.: 15.961 min
Delta R.T.: -0.011 min
Response: 957688
Conc: 6.06 ug/ml

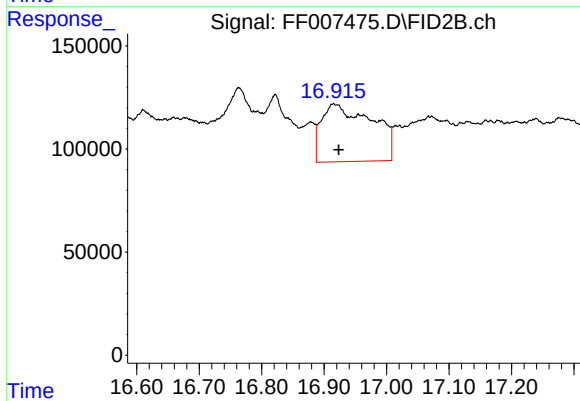


#12 N-OCTACOSANE

R.T.: 16.916 min
Delta R.T.: -0.008 min
Response: 1584104
Conc: 10.32 ug/ml

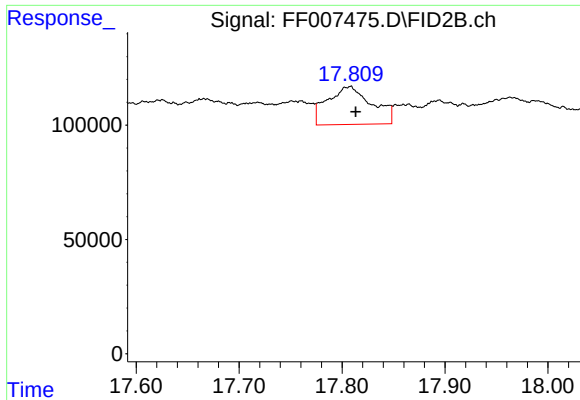


#13 N-TRIACONTANE

R.T.: 17.807 min
Delta R.T.: -0.007 min
Response: 496407
Conc: 3.36 ug/ml

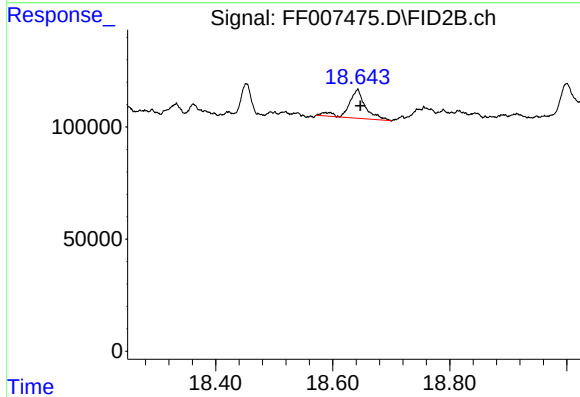

#14 N-DOTRIACONTANE

R.T.: 18.642 min
Delta R.T.: -0.005 min
Response: 245272
Conc: 1.77 ug/ml

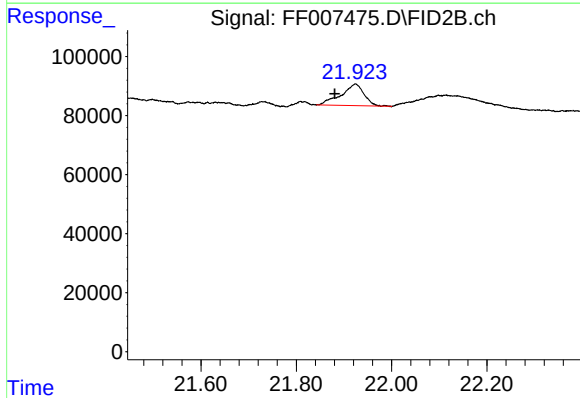

#18 N-TETRACONTANE

R.T.: 21.924 min
Delta R.T.: 0.043 min
Response: 242124
Conc: 2.18 ug/ml