

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
 Data File : FF007476.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2020 13:49
 Operator : DD\AJ
 Sample : L3808-07
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 09 01:22:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.736	3678216	25.009 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.238	74324	0.452 ug/ml
6)	N-OCTADECANE	11.318	105523	0.619 ug/ml
7)	N-EICOSANE	12.696f	217494	1.294 ug/ml
10)	N-TETRACOSANE	14.940	1127107	6.911 ug/ml
11)	N-HEXACOSANE	15.965	3412309	21.586 ug/ml
12)	N-OCTACOSANE	16.914	3773931	24.591 ug/ml
13)	N-TRIACONTANE	17.812	3220669	21.791 ug/ml
14)	N-DOTRIACONTANE	18.638	4198267	30.256 ug/ml
15)	N-TETRATRIACONTANE	19.427	2560738	20.291 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007476.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 13:49
Operator : DD\AJ
Sample : L3808-07
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:22:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

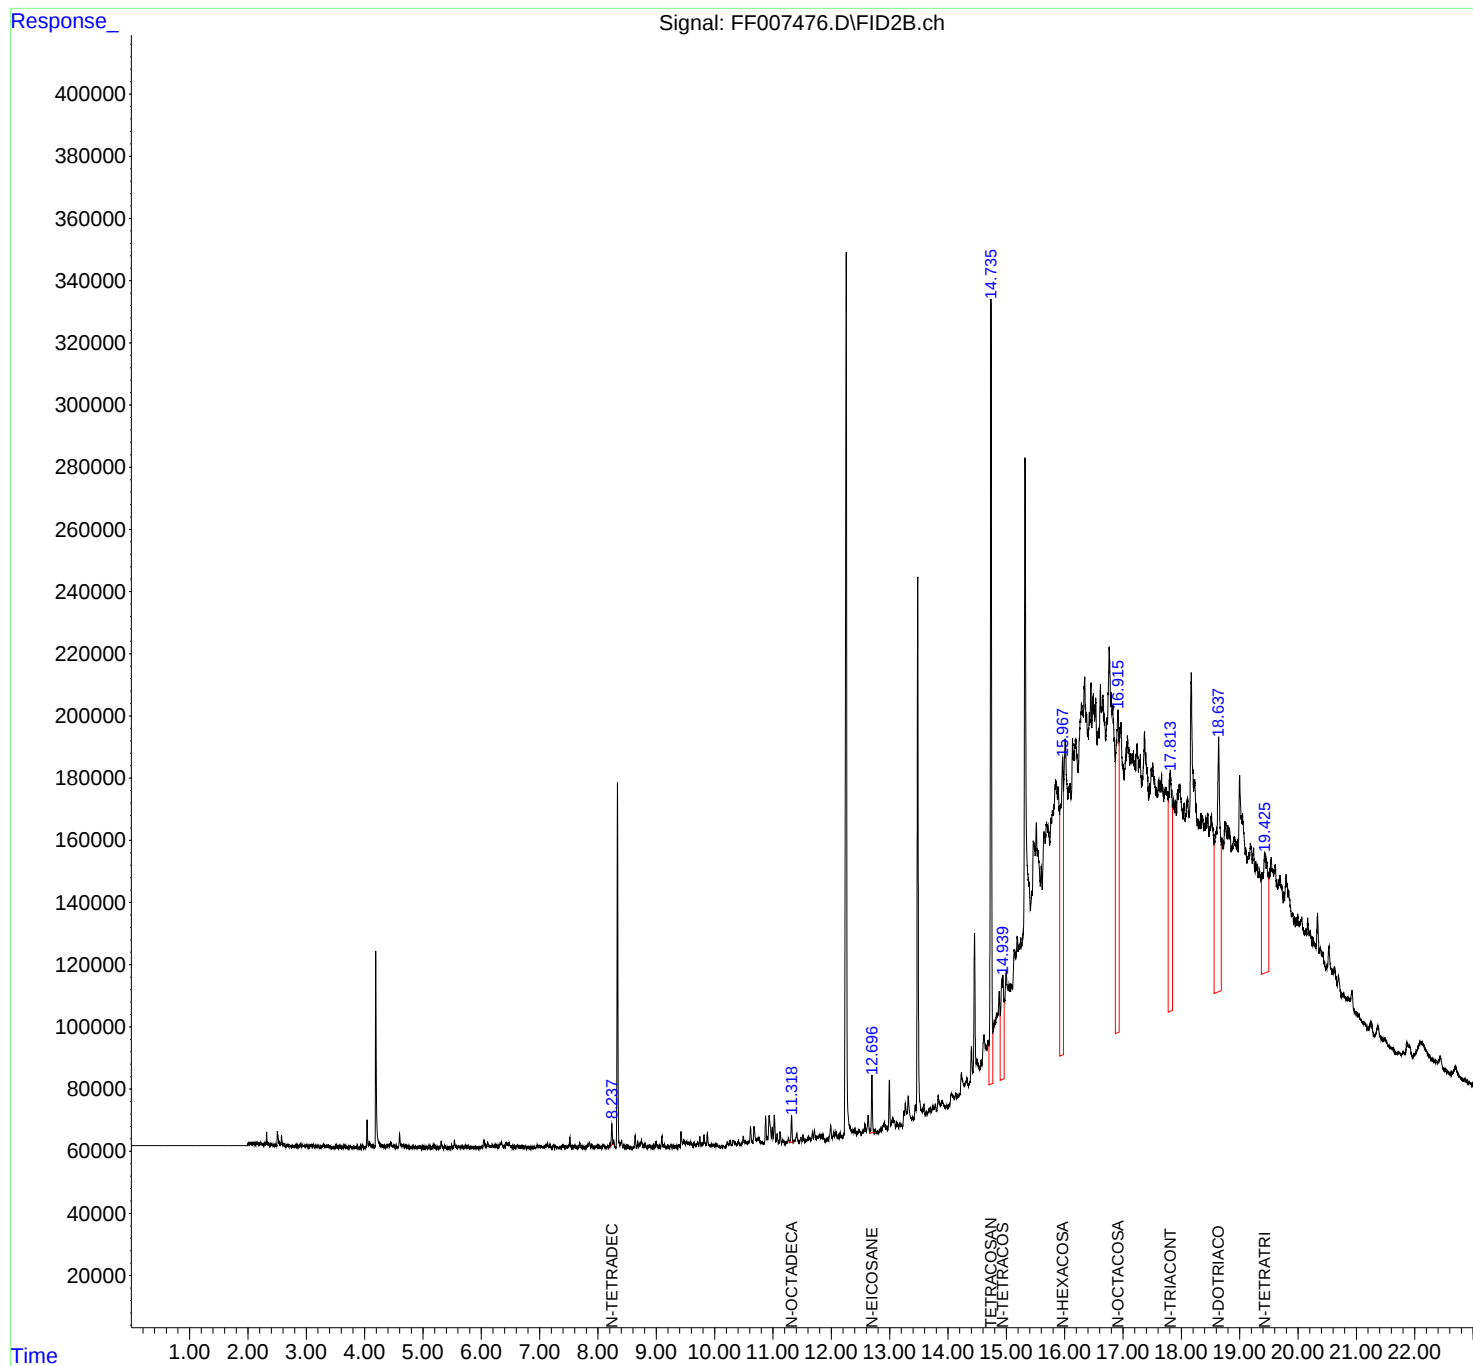

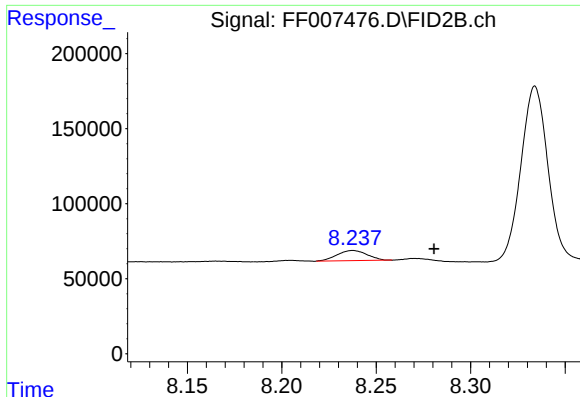


#4 N-TETRADECANE

R.T.: 8.238 min
Delta R.T.: -0.043 min
Response: 74324
Conc: 0.45 ug/ml

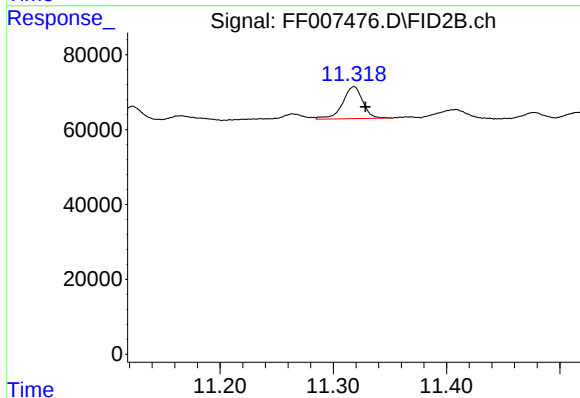


#6 N-OCTADECANE

R.T.: 11.318 min
Delta R.T.: -0.010 min
Response: 105523
Conc: 0.62 ug/ml

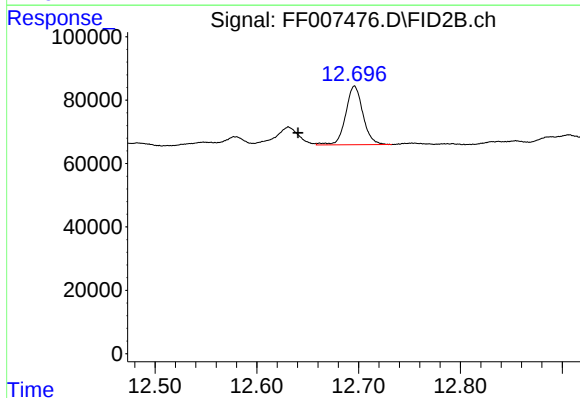


#7 N-EICOSANE

R.T.: 12.696 min
Delta R.T.: 0.055 min
Response: 217494
Conc: 1.29 ug/ml

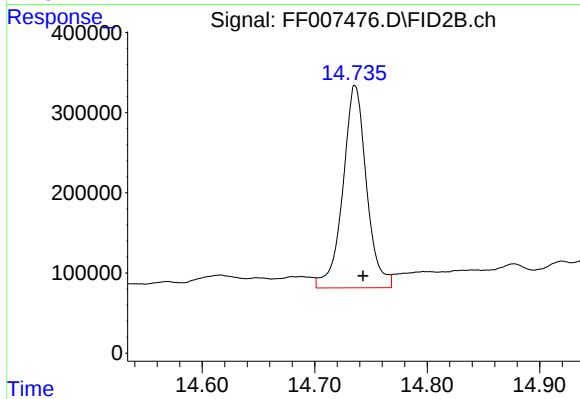


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 3678216
Conc: 25.01 ug/ml

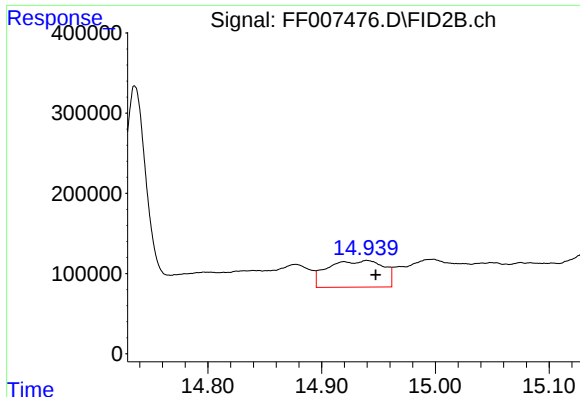


#10 N-TETRACOSANE

R.T.: 14.940 min
Delta R.T.: -0.007 min
Response: 1127107
Conc: 6.91 ug/ml

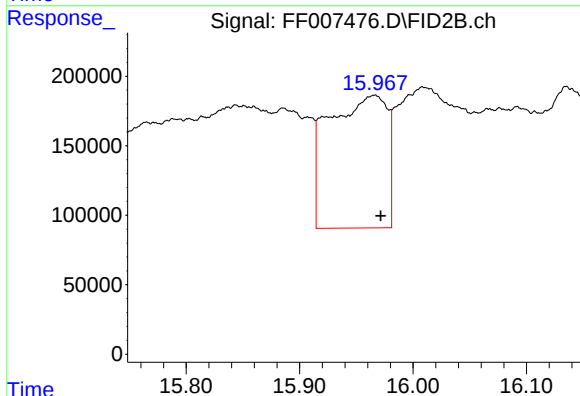


#11 N-HEXACOSANE

R.T.: 15.965 min
Delta R.T.: -0.006 min
Response: 3412309
Conc: 21.59 ug/ml

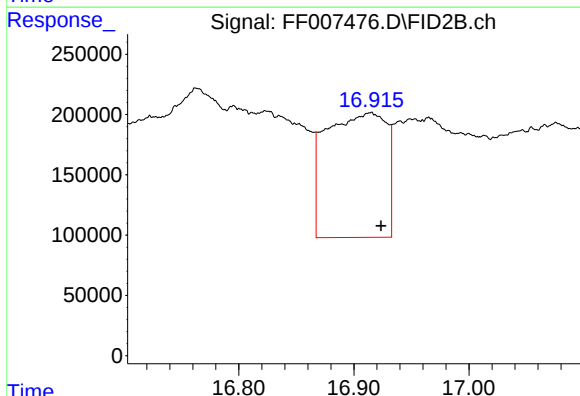


#12 N-OCTACOSANE

R.T.: 16.914 min
Delta R.T.: -0.009 min
Response: 3773931
Conc: 24.59 ug/ml

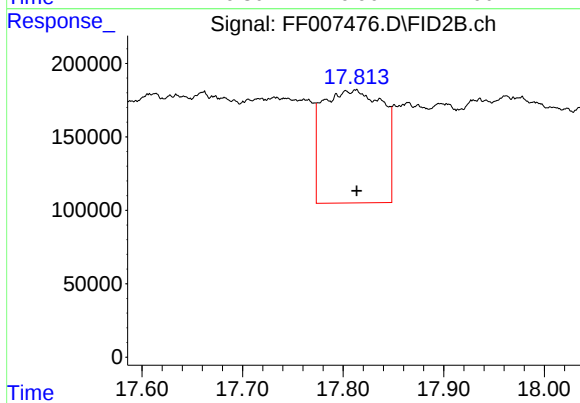


#13 N-TRIACONTANE

R.T.: 17.812 min
Delta R.T.: -0.001 min
Response: 3220669
Conc: 21.79 ug/ml

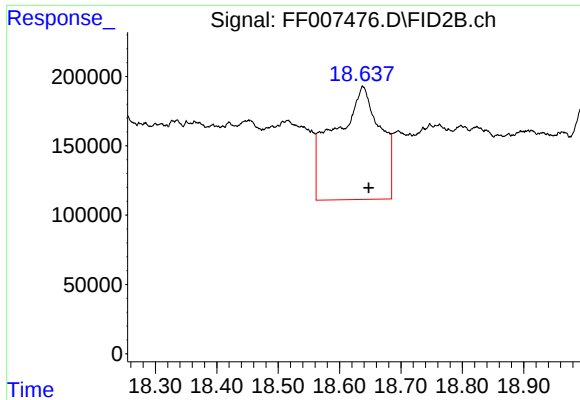

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 4198267
Conc: 30.26 ug/ml

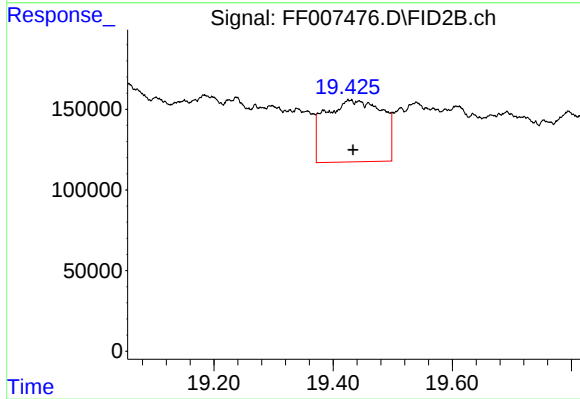

#15 N-TETRATRIACONTANE

R.T.: 19.427 min
Delta R.T.: -0.006 min
Response: 2560738
Conc: 20.29 ug/ml