

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
 Data File : FF007477.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2020 14:20
 Operator : DD\AJ
 Sample : L3808-09
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 09 01:23:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.737	2994841	20.363 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.335f	914479	5.557 ug/ml
6)	N-OCTADECANE	11.320	172266	1.011 ug/ml
7)	N-EICOSANE	12.632	145771	0.867 ug/ml
8)	N-DOCOSANE	13.833	89482	0.543 ug/ml
10)	N-TETRACOSANE	14.942	1096112	6.721 ug/ml
11)	N-HEXACOSANE	15.965	3288460	20.803 ug/ml
12)	N-OCTACOSANE	16.913	3879131	25.277 ug/ml
13)	N-TRIACONTANE	17.810	2169476	14.678 ug/ml
14)	N-DOTRIACONTANE	18.638	2043602	14.728 ug/ml
15)	N-TETRATRIACONTANE	19.432	49365	0.391 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007477.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 14:20
Operator : DD\AJ
Sample : L3808-09
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:23:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

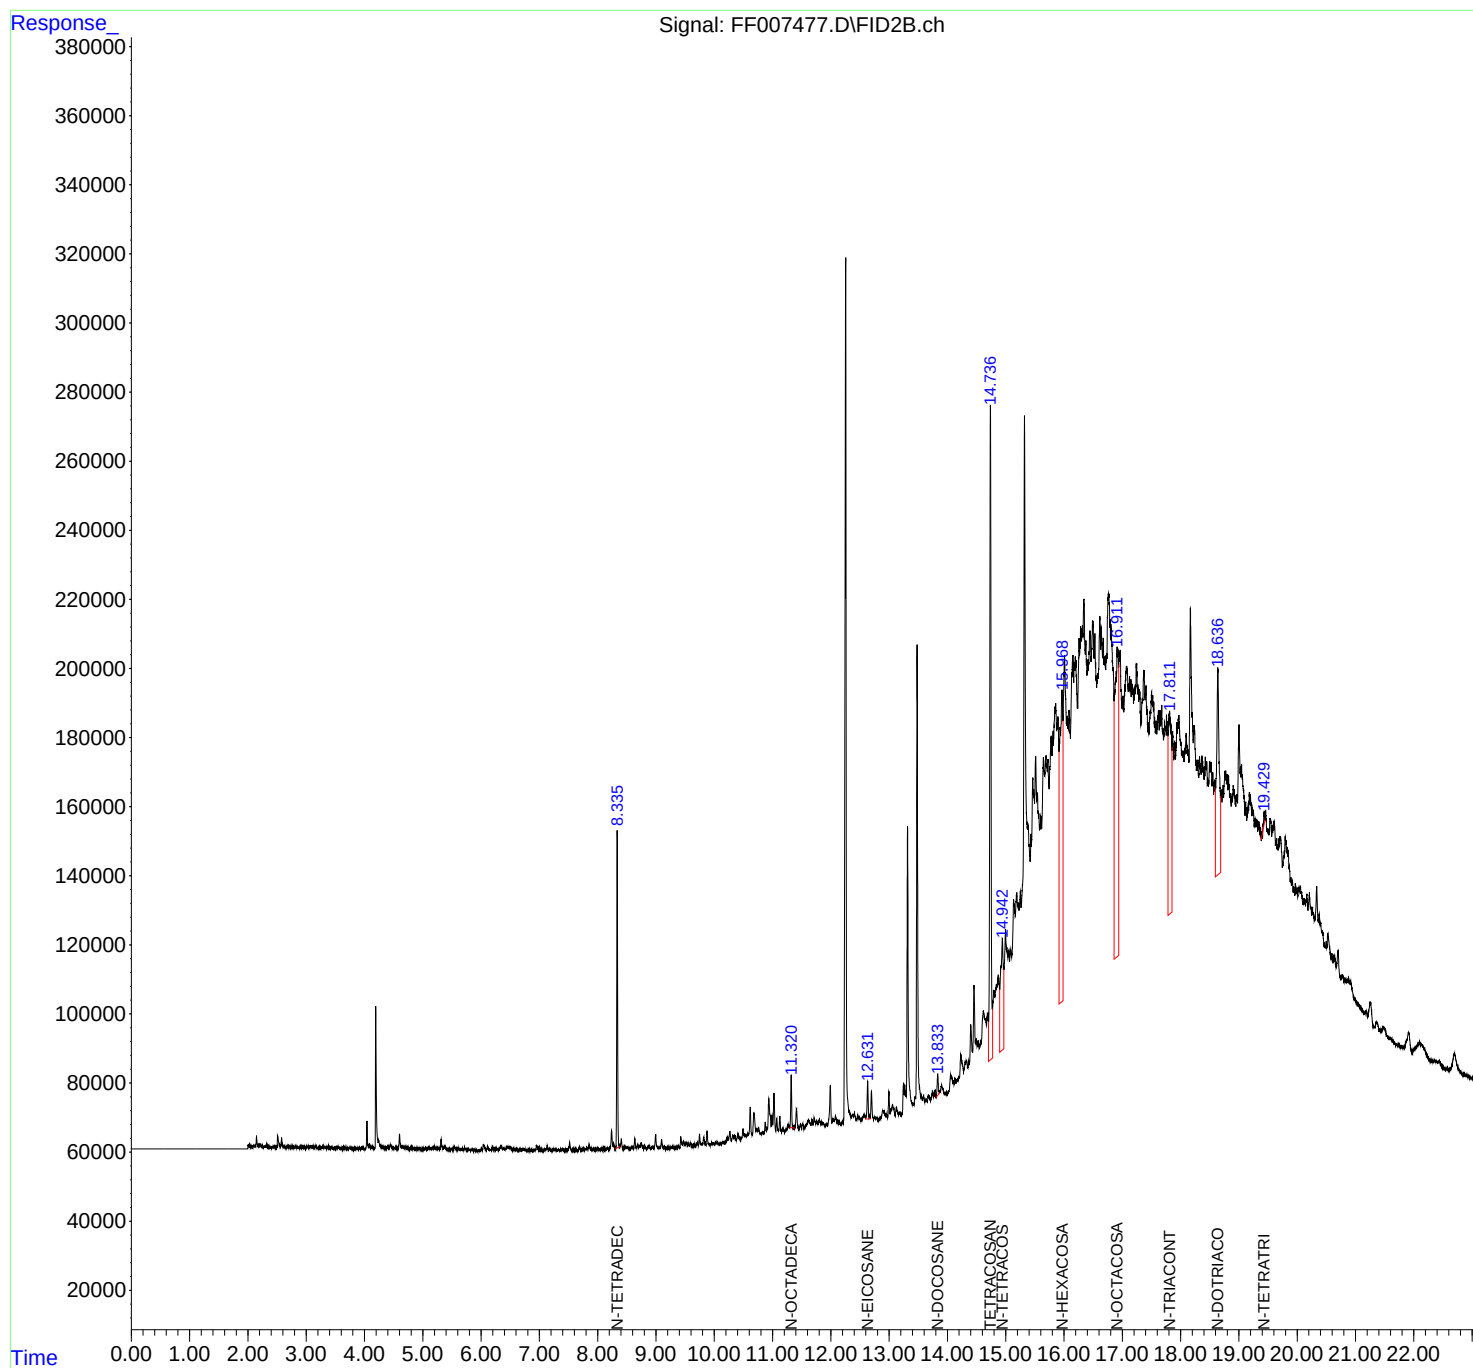

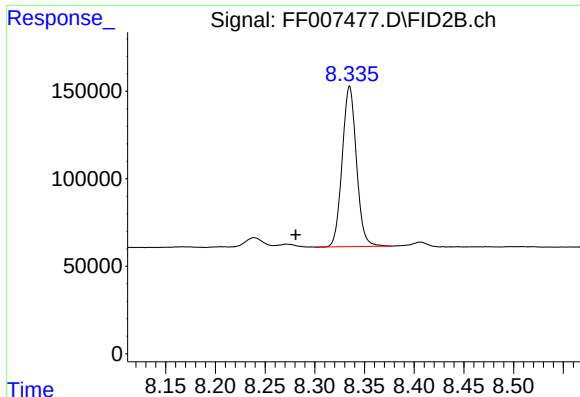


#4 N-TETRADECANE

R.T.: 8.335 min
Delta R.T.: 0.054 min
Response: 914479
Conc: 5.56 ug/ml

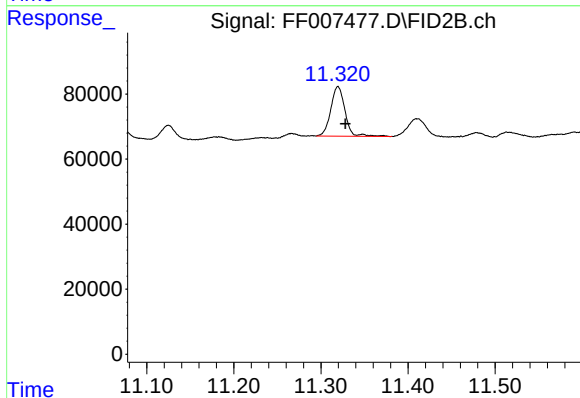


#6 N-OCTADECANE

R.T.: 11.320 min
Delta R.T.: -0.009 min
Response: 172266
Conc: 1.01 ug/ml

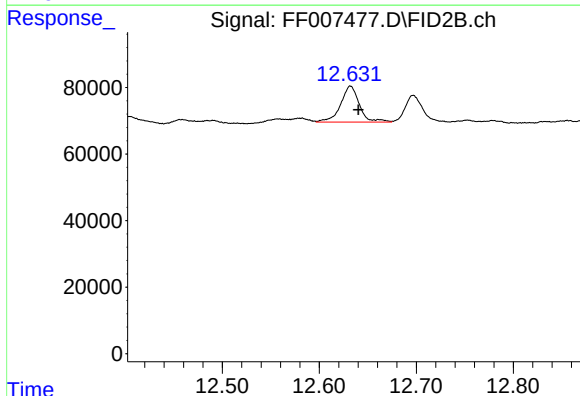


#7 N-EICOSANE

R.T.: 12.632 min
Delta R.T.: -0.008 min
Response: 145771
Conc: 0.87 ug/ml

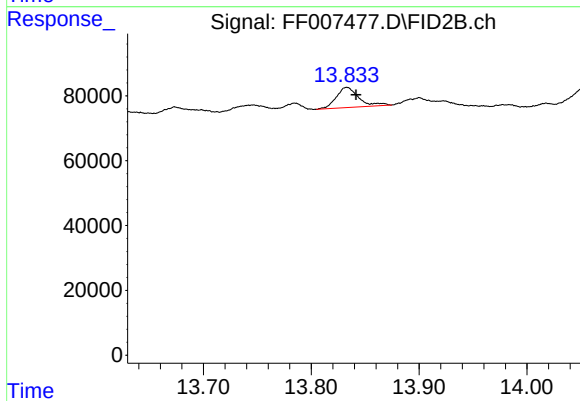


#8 N-DOCOSANE

R.T.: 13.833 min
Delta R.T.: -0.008 min
Response: 89482
Conc: 0.54 ug/ml

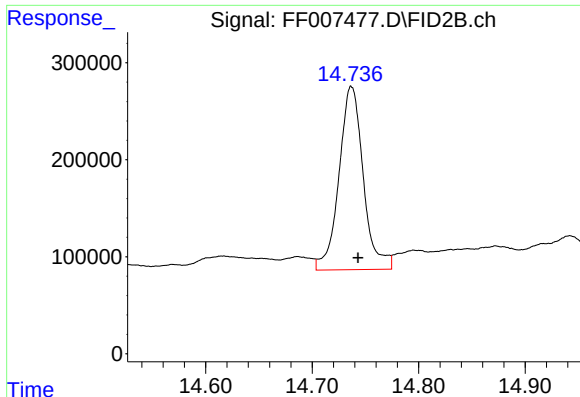


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.006 min
Response: 2994841
Conc: 20.36 ug/ml

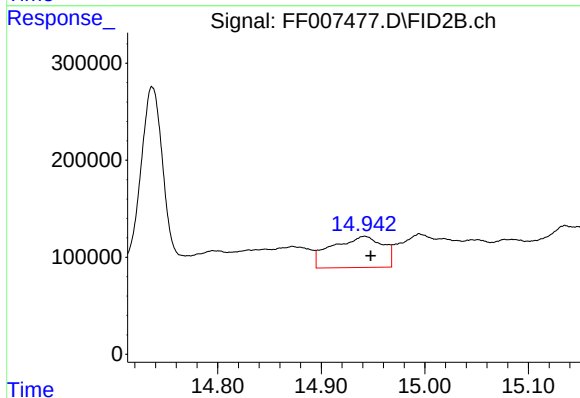


#10 N-TETRACOSANE

R.T.: 14.942 min
Delta R.T.: -0.006 min
Response: 1096112
Conc: 6.72 ug/ml

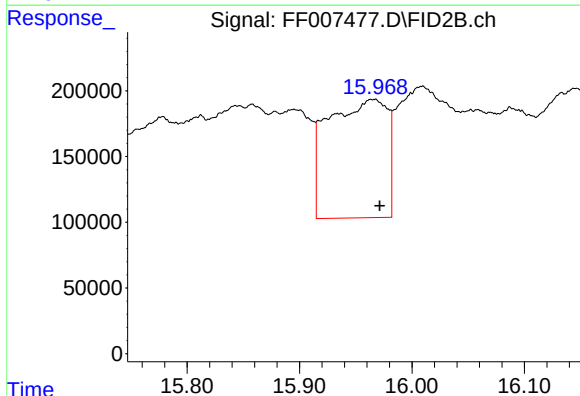


#11 N-HEXACOSANE

R.T.: 15.965 min
Delta R.T.: -0.006 min
Response: 3288460
Conc: 20.80 ug/ml

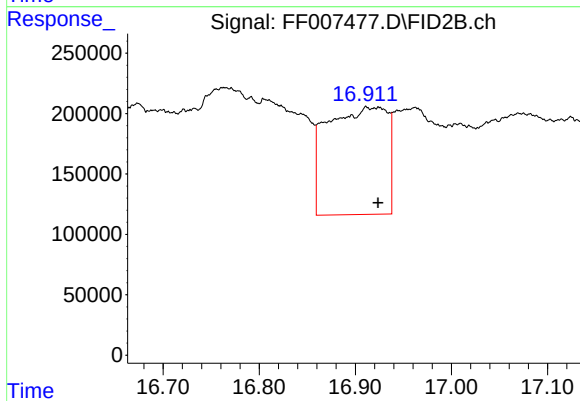


#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: -0.011 min
Response: 3879131
Conc: 25.28 ug/ml

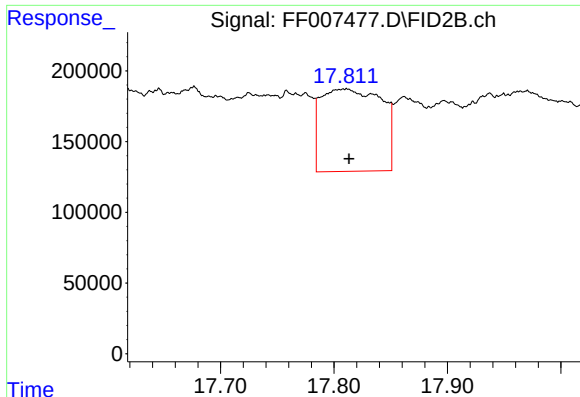


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: -0.004 min
Response: 2169476
Conc: 14.68 ug/ml

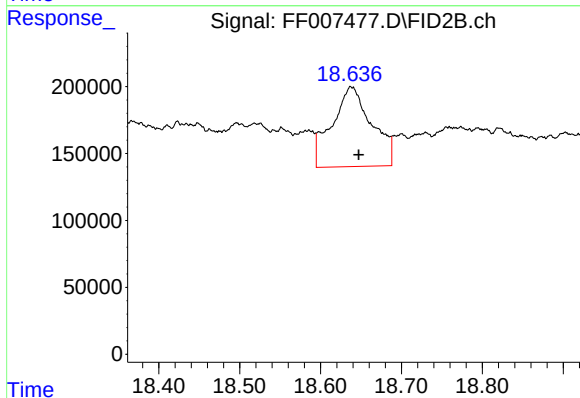

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 2043602
Conc: 14.73 ug/ml

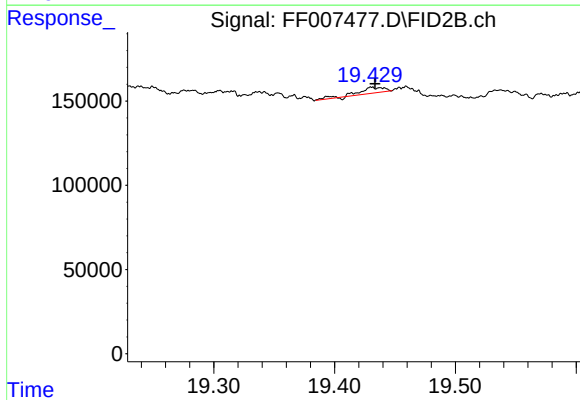

#15 N-TETRATRIACONTANE

R.T.: 19.432 min
Delta R.T.: -0.001 min
Response: 49365
Conc: 0.39 ug/ml