

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007483.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 17:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:24:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	2412688	16.404 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.805	142591	0.965 ug/ml
14) N-DOTRIACONTANE	18.639	175323	1.264 ug/ml
15) N-TETRATRIACONTANE	19.424	128944	1.022 ug/ml
16) N-HEXATRIACONTANE	20.167	145025	1.214 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007483.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 17:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:24:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

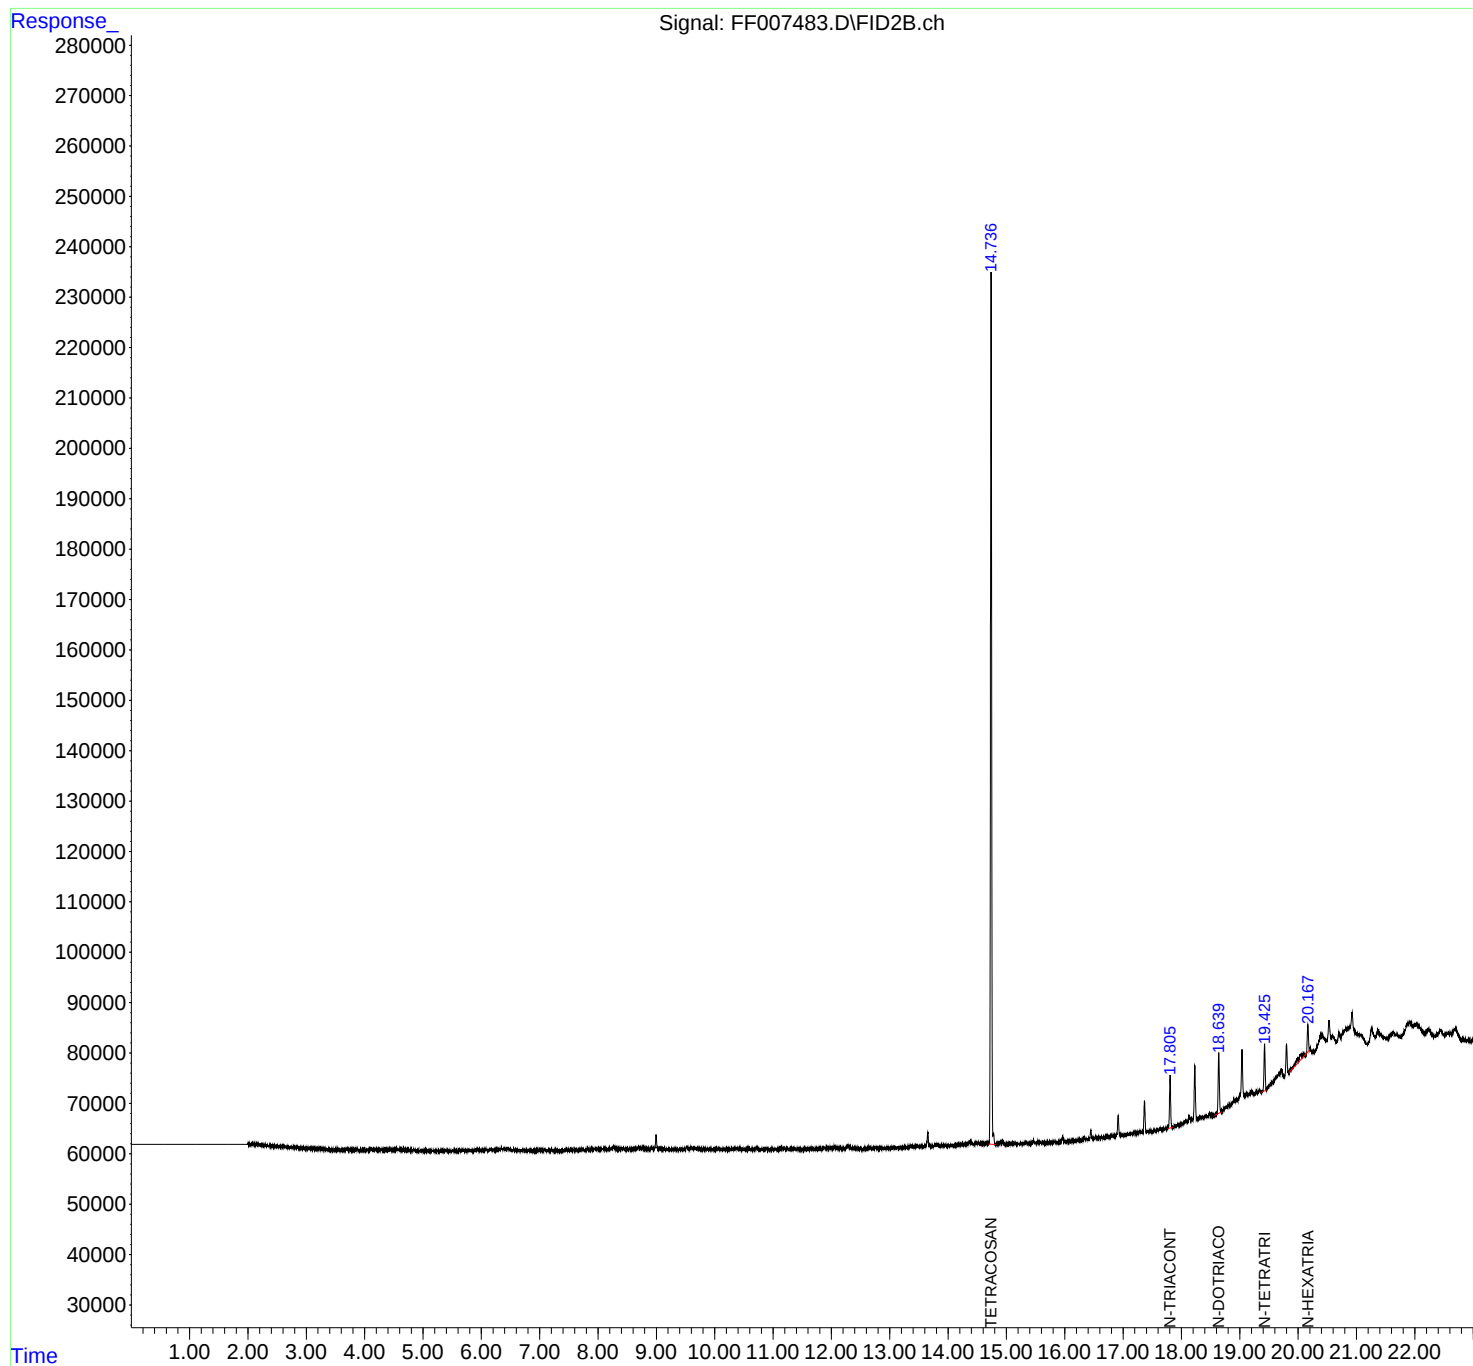

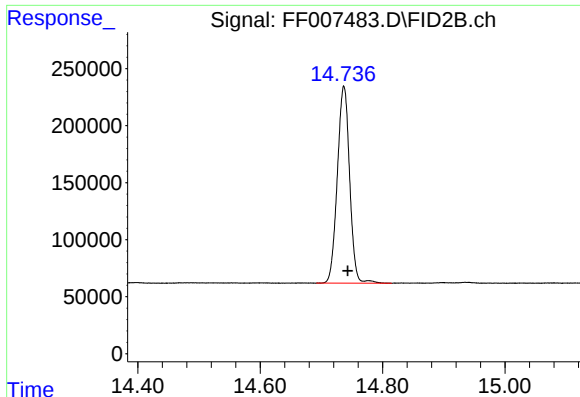


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.737 min
Delta R.T.: -0.006 min
Response: 2412688
Conc: 16.40 ug/ml

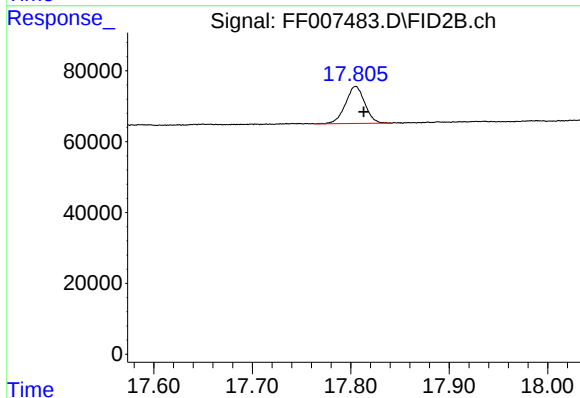


#13 N-TRIACONTANE

R.T.: 17.805 min
Delta R.T.: -0.008 min
Response: 142591
Conc: 0.96 ug/ml

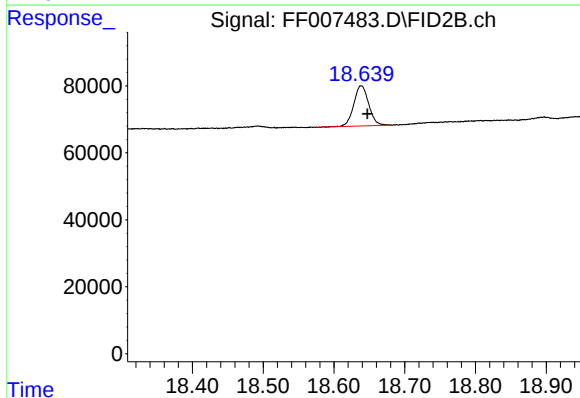


#14 N-DOTRIACONTANE

R.T.: 18.639 min
Delta R.T.: -0.009 min
Response: 175323
Conc: 1.26 ug/ml

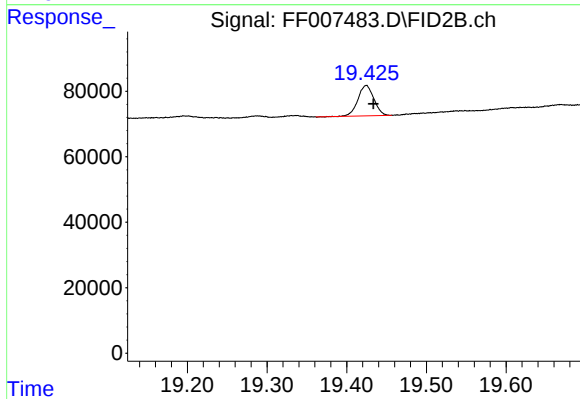

#15 N-TETRATRIACONTANE

R.T.: 19.424 min
Delta R.T.: -0.009 min
Response: 128944
Conc: 1.02 ug/ml

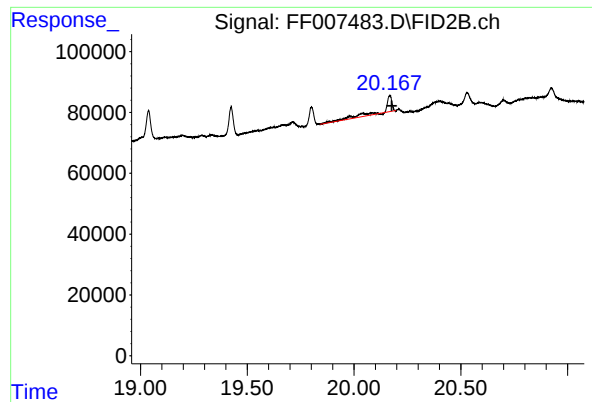

#16 N-HEXATRIACONTANE

R.T.: 20.167 min
Delta R.T.: -0.010 min
Response: 145025
Conc: 1.21 ug/ml