

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
 Data File : FF007486.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2020 19:00
 Operator : DD\AJ
 Sample : L3808-09 2X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 09 01:25:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	1090701	7.416 ug/ml
Target Compounds			
4) N-TETRADECANE	8.336f	401317	2.439 ug/ml
6) N-OCTADECANE	11.320	101713	0.597 ug/ml
10) N-TETRACOSANE	14.940	135010	0.828 ug/ml
11) N-HEXACOSANE	15.964	598892	3.789 ug/ml
12) N-OCTACOSANE	16.915	126396	0.824 ug/ml
13) N-TRIACONTANE	17.808	311875	2.110 ug/ml
14) N-DOTRIACONTANE	18.638	517705	3.731 ug/ml
15) N-TETRATRIACONTANE	19.425	254671	2.018 ug/ml
16) N-HEXATRIACONTANE	20.166	129512	1.084 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007486.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 19:00
Operator : DD\AJ
Sample : L3808-09 2X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:25:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

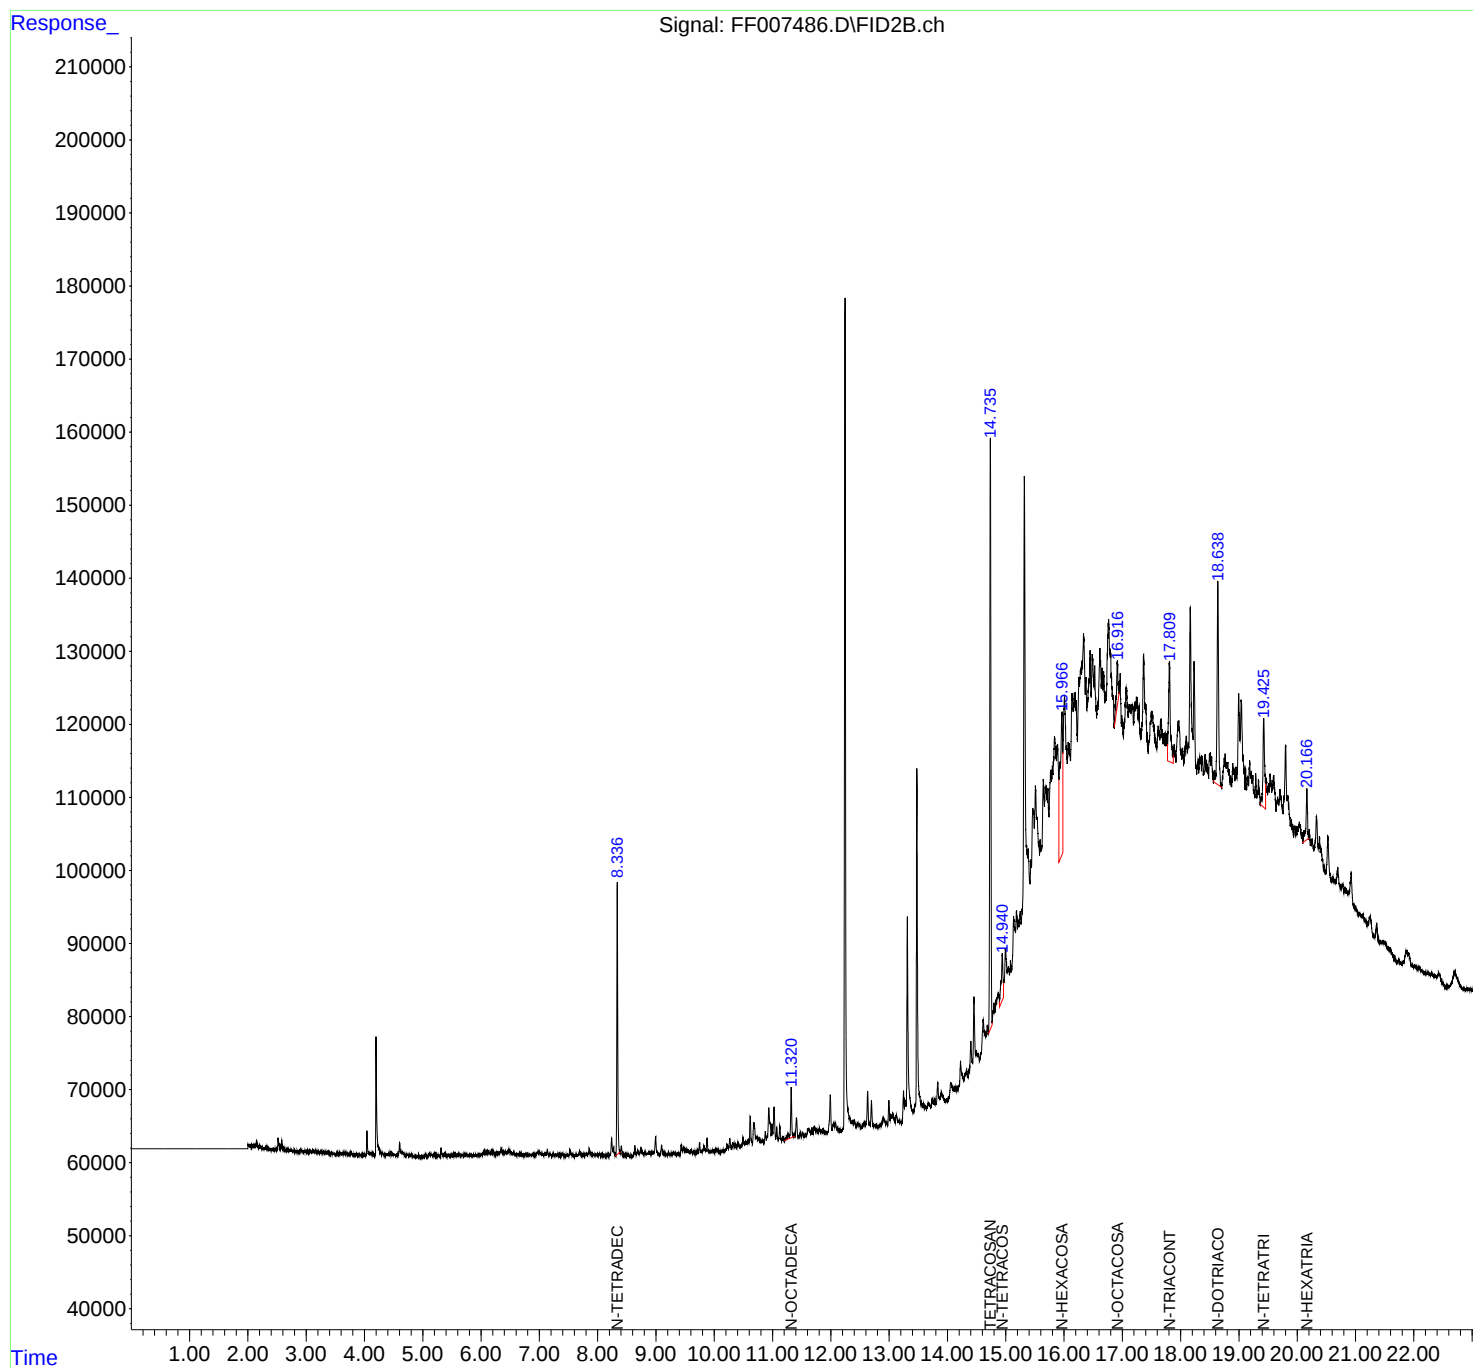

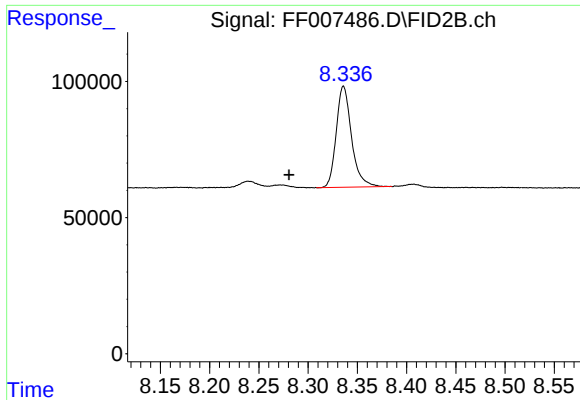


#4 N-TETRADECANE

R.T.: 8.336 min
Delta R.T.: 0.055 min
Response: 401317
Conc: 2.44 ug/ml

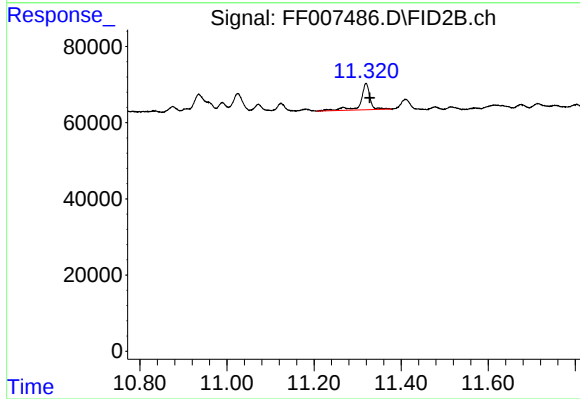


#6 N-OCTADECANE

R.T.: 11.320 min
Delta R.T.: -0.009 min
Response: 101713
Conc: 0.60 ug/ml

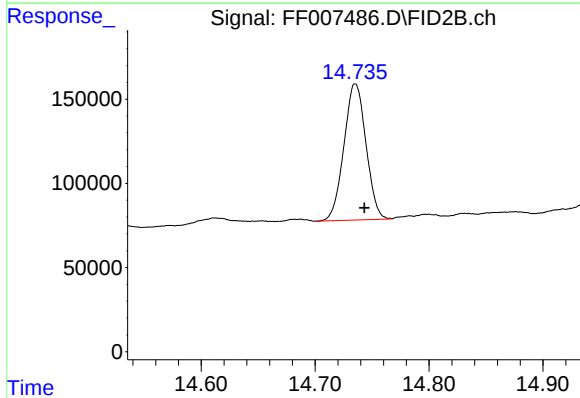


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: -0.008 min
Response: 1090701
Conc: 7.42 ug/ml

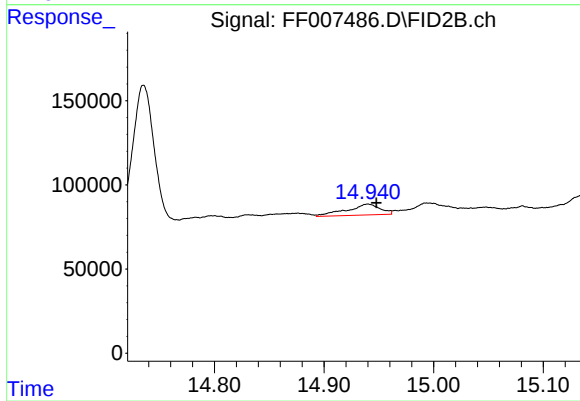


#10 N-TETRACOSANE

R.T.: 14.940 min
Delta R.T.: -0.008 min
Response: 135010
Conc: 0.83 ug/ml

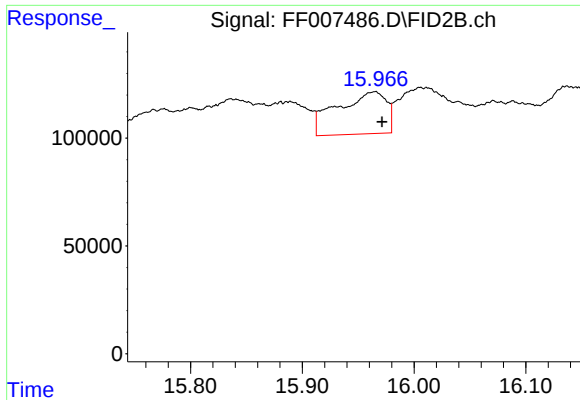


#11 N-HEXACOSANE

R.T.: 15.964 min
Delta R.T.: -0.007 min
Response: 598892
Conc: 3.79 ug/ml

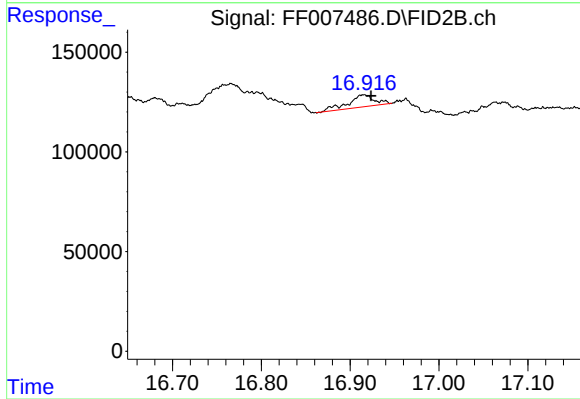


#12 N-OCTACOSANE

R.T.: 16.915 min
Delta R.T.: -0.008 min
Response: 126396
Conc: 0.82 ug/ml

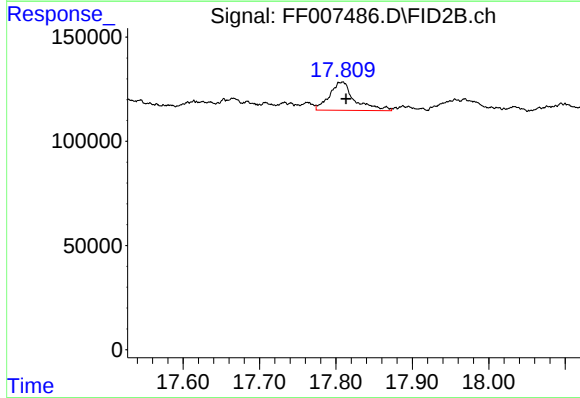


#13 N-TRIACONTANE

R.T.: 17.808 min
Delta R.T.: -0.006 min
Response: 311875
Conc: 2.11 ug/ml

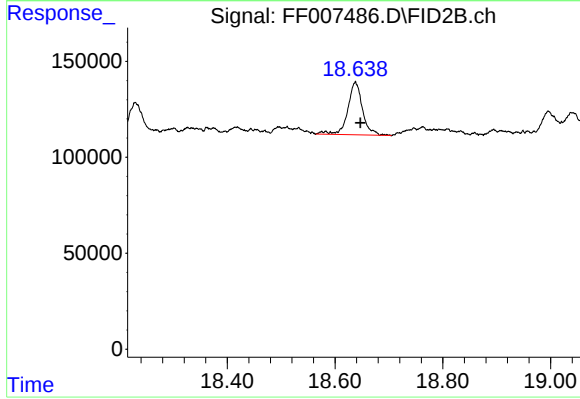


#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.009 min
Response: 517705
Conc: 3.73 ug/ml

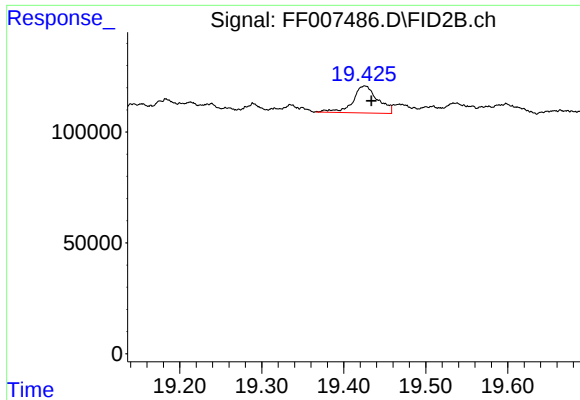

#15 N-TETRATRIACONTANE

R.T.: 19.425 min
Delta R.T.: -0.008 min
Response: 254671
Conc: 2.02 ug/ml

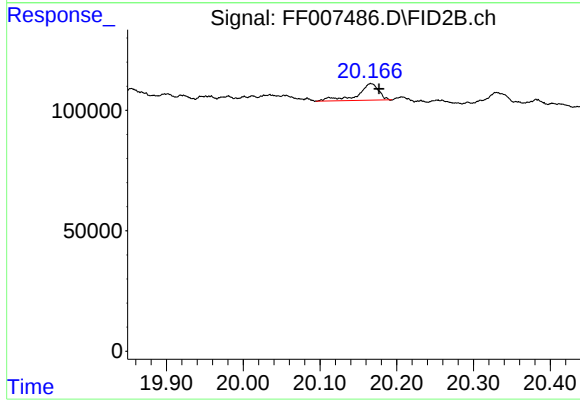

#16 N-HEXATRIACONTANE

R.T.: 20.166 min
Delta R.T.: -0.011 min
Response: 129512
Conc: 1.08 ug/ml