

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
 Data File : FF007480.D
 Signal(s) : FID2B.ch
 Acq On : 08 Sep 2020 15:54
 Operator : DD\AJ
 Sample : L3808-09MSD
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 09 01:23:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	2324842	15.807 ug/mlm
Target Compounds			
2) N-DECANE	4.454	3466266	21.732 ug/ml
3) N-DODECANE	6.479	3566700	21.924 ug/ml
4) N-TETRADECANE	8.276	3661391	22.250 ug/ml
5) N-HEXADECANE	9.879	3568716	21.147 ug/ml
6) N-OCTADECANE	11.322	3675663	21.570 ug/ml
7) N-EICOSANE	12.635	3509026	20.871 ug/ml
8) N-DOCOSANE	13.837	3304292	20.055 ug/ml
10) N-TETRACOSANE	14.944	3379532	20.721 ug/mlm
11) N-HEXACOSANE	15.968	3119344	19.733 ug/mlm
12) N-OCTACOSANE	16.921	2959047	19.281 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090820\
Data File : FF007480.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2020 15:54
Operator : DD\AJ
Sample : L3808-09MSD
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 09 01:23:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

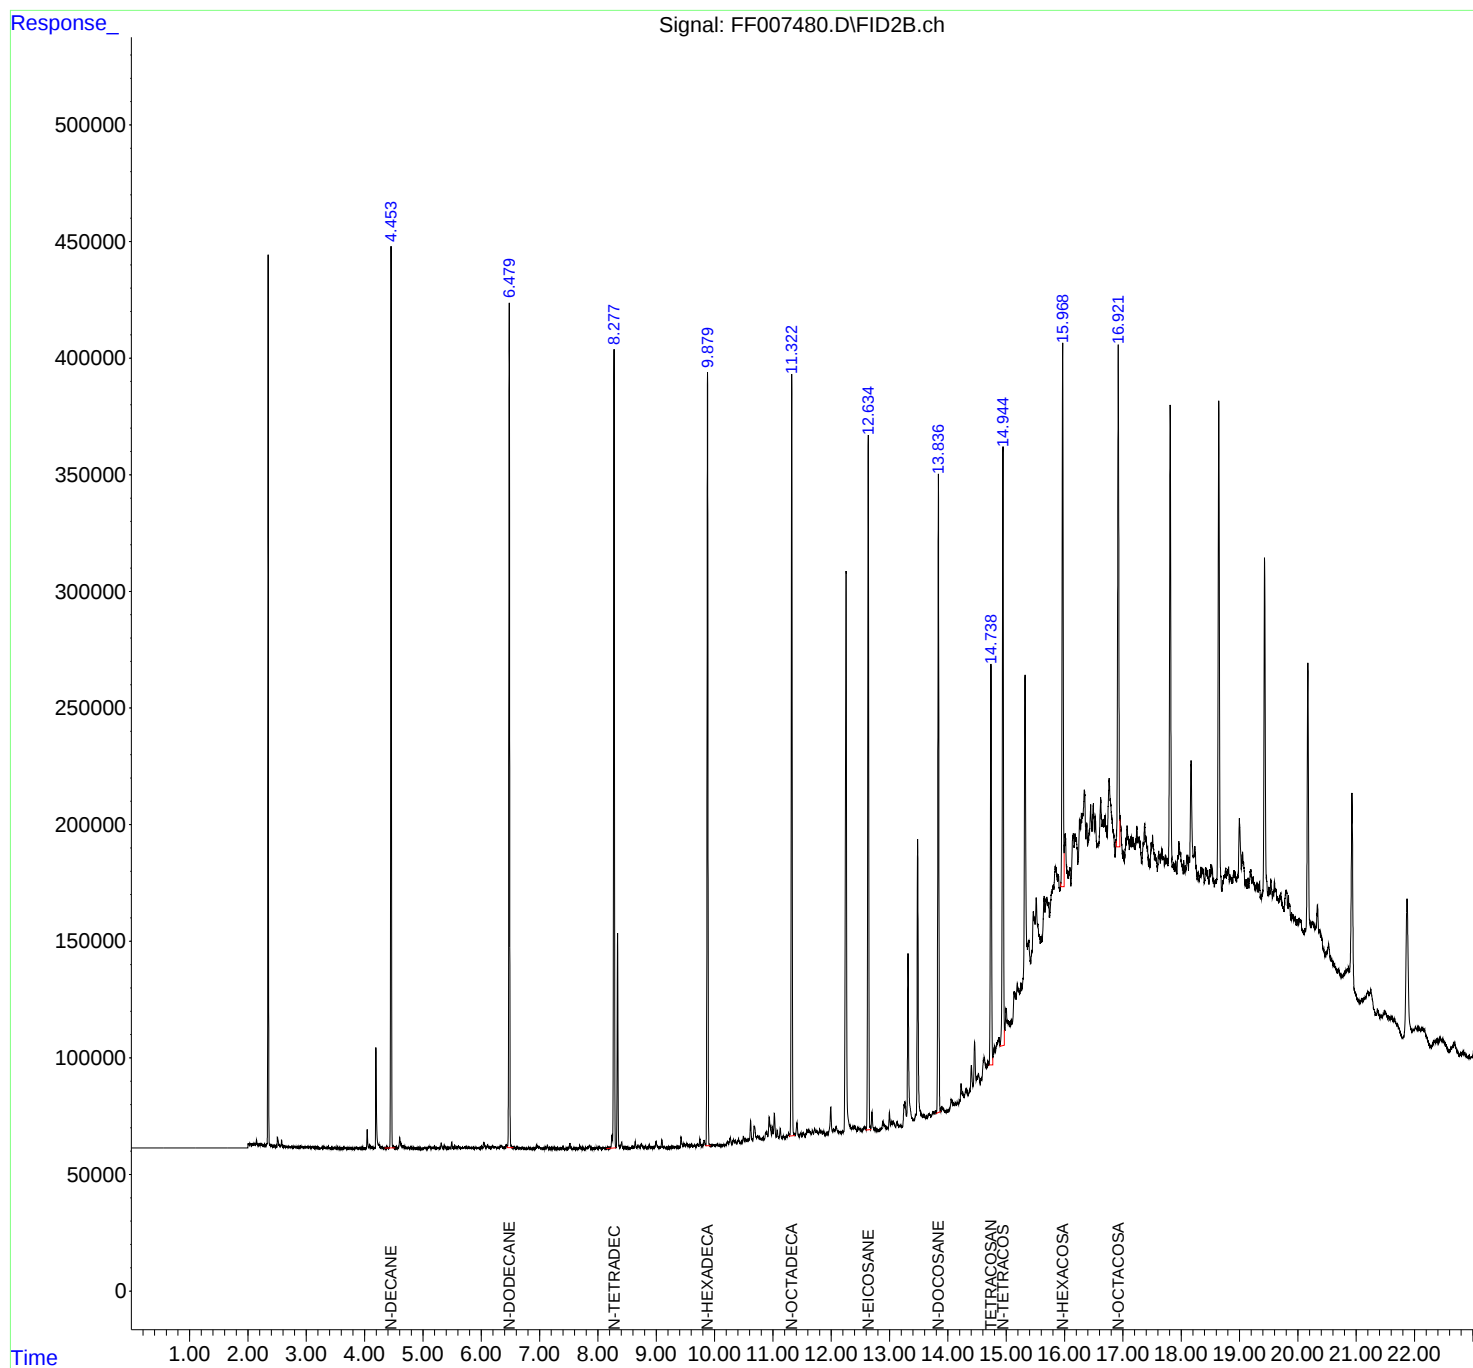

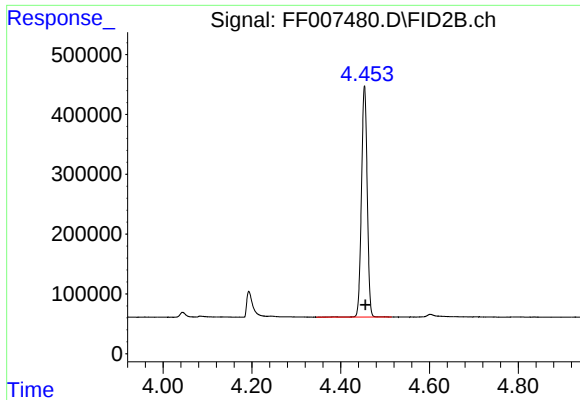


#2 N-DECANE

R.T.: 4.454 min
Delta R.T.: -0.002 min
Response: 3466266
Conc: 21.73 ug/ml

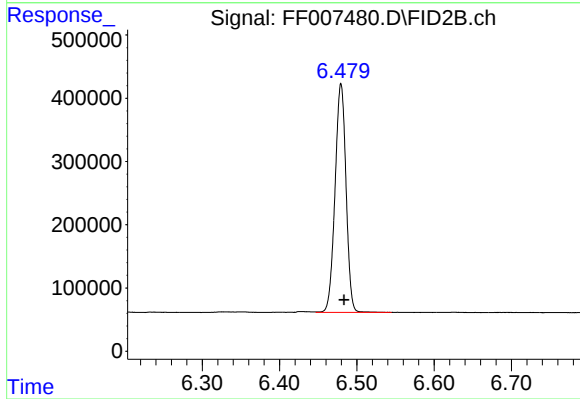


#3 N-DODECANE

R.T.: 6.479 min
Delta R.T.: -0.004 min
Response: 3566700
Conc: 21.92 ug/ml

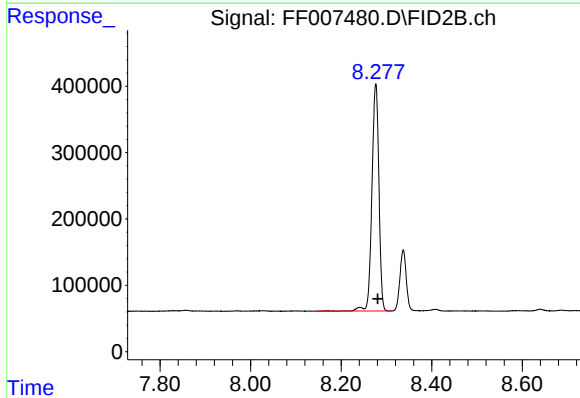


#4 N-TETRADECANE

R.T.: 8.276 min
Delta R.T.: -0.004 min
Response: 3661391
Conc: 22.25 ug/ml

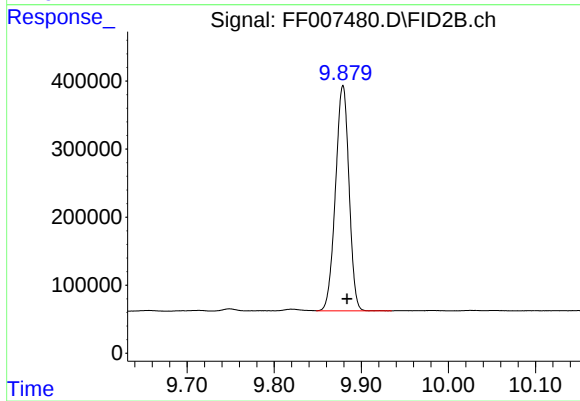


#5 N-HEXADECANE

R.T.: 9.879 min
Delta R.T.: -0.005 min
Response: 3568716
Conc: 21.15 ug/ml

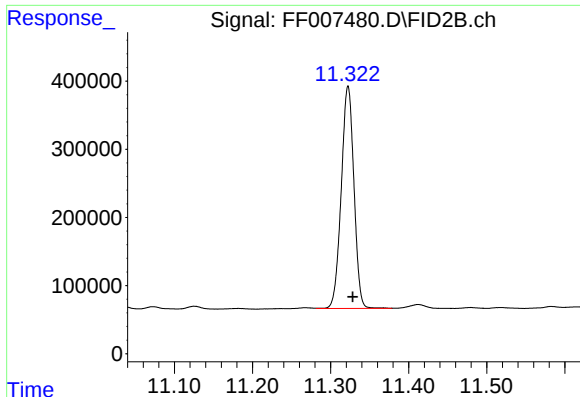


#6 N-OCTADECANE

R.T.: 11.322 min
Delta R.T.: -0.006 min
Response: 3675663
Conc: 21.57 ug/ml

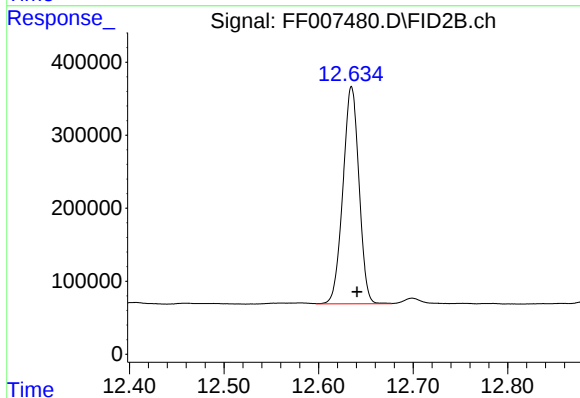


#7 N-EICOSANE

R.T.: 12.635 min
Delta R.T.: -0.006 min
Response: 3509026
Conc: 20.87 ug/ml

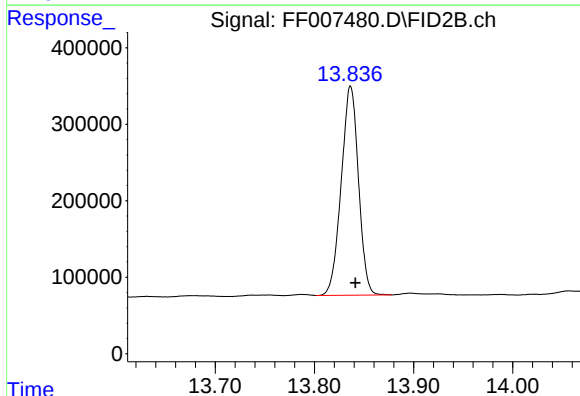


#8 N-DOCOSANE

R.T.: 13.837 min
Delta R.T.: -0.005 min
Response: 3304292
Conc: 20.06 ug/ml

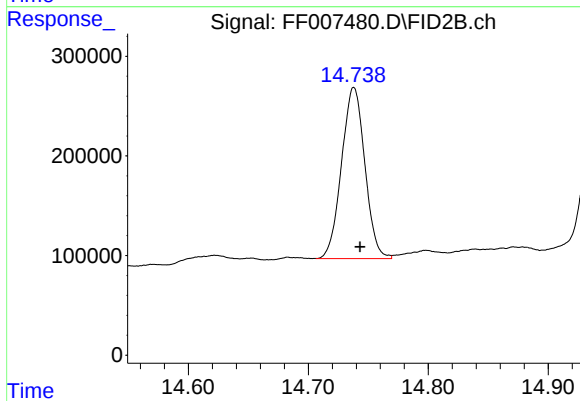


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.738 min
Delta R.T.: -0.006 min
Response: 2324842
Conc: 15.81 ug/ml m

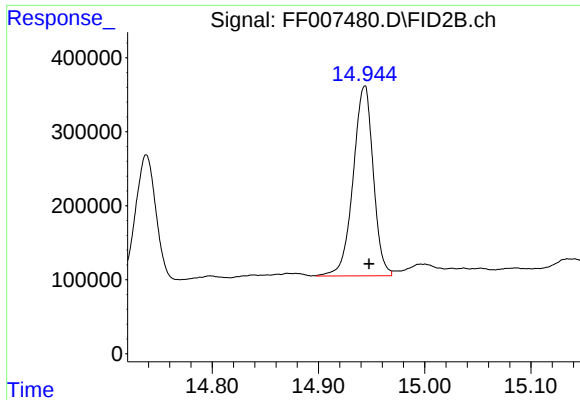


#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: -0.004 min
Response: 3379532
Conc: 20.72 ug/ml m

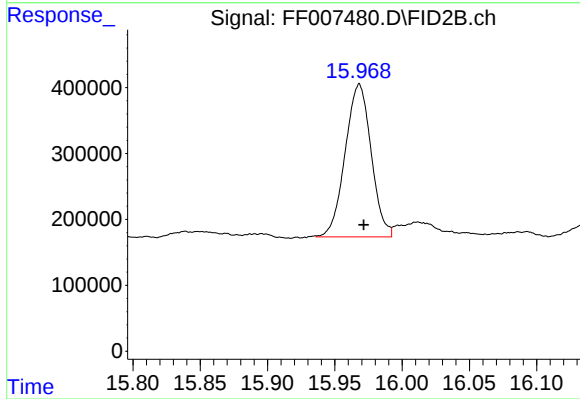

#11 N-HEXACOSANE

R.T.: 15.968 min
Delta R.T.: -0.003 min
Response: 3119344
Conc: 19.73 ug/ml m

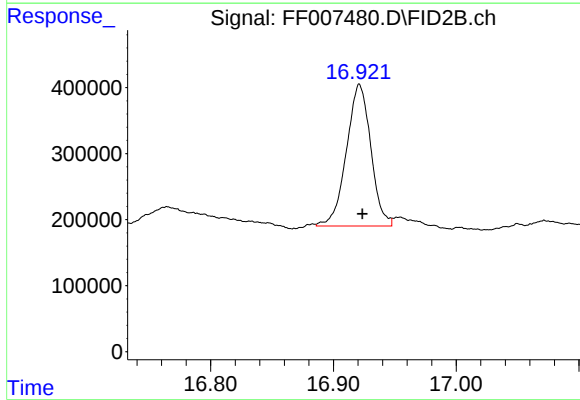

#12 N-OCTACOSANE

R.T.: 16.921 min
Delta R.T.: -0.003 min
Response: 2959047
Conc: 19.28 ug/ml m