

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090822\
Data File : FF011409.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2022 12:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 09 07:06:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.513	1664562	12.711 ug/ml
12)	N-OCTACOSANE	16.951	1621345	13.236 ug/ml
13)	N-TRIACONTANE	17.835	234269	1.942 ug/ml
14)	N-DOTRIACONTANE	18.666	328778	2.779 ug/ml
15)	N-TETRATRIACONTANE	19.446	284003	2.488 ug/ml
16)	N-HEXATRIACONTANE	20.184	203953	1.916 ug/ml
17)	N-OCTATRIACONTANE	20.889	137312	1.320 ug/ml
18)	N-TETRACONTANE	21.700	84560	0.801 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090822\
Data File : FF011409.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2022 12:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 09 07:06:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

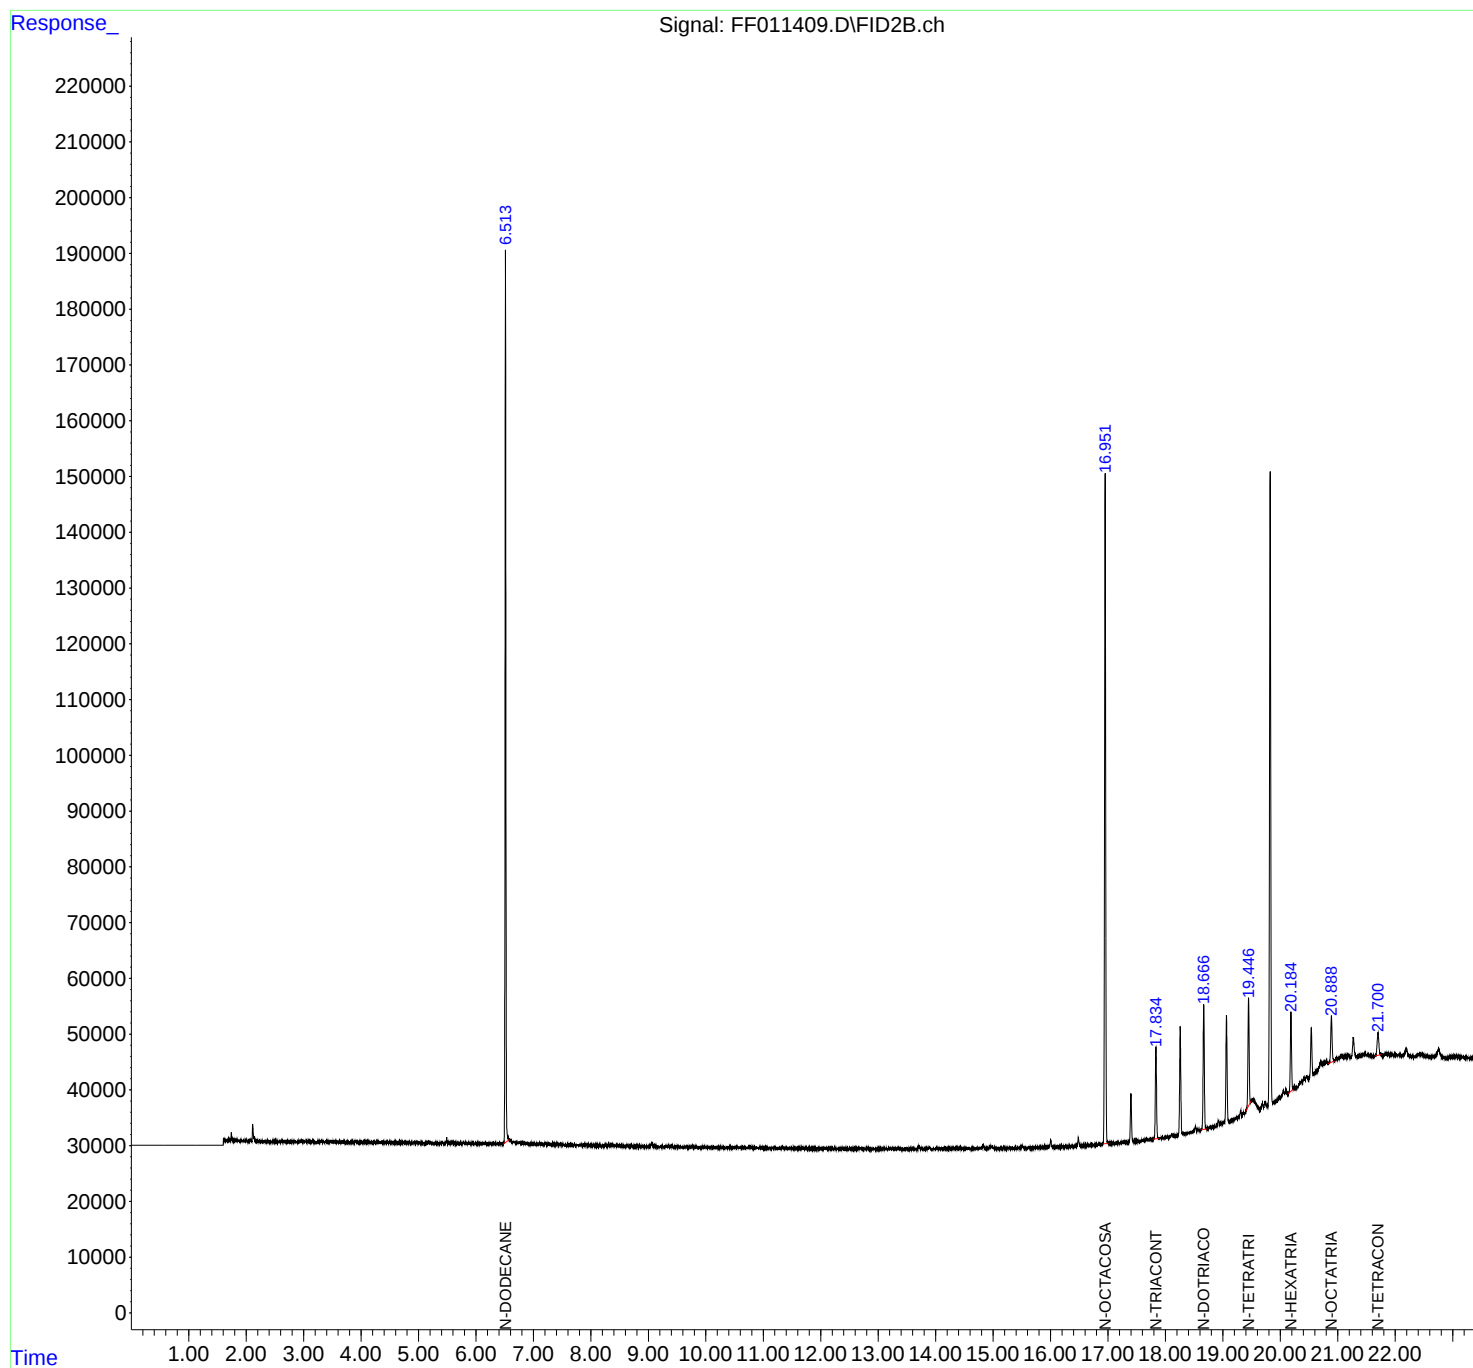


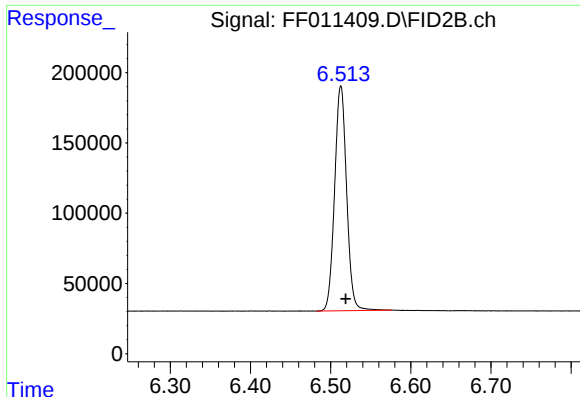

#3 N-DODECANE


R.T.: 6.513 min
Delta R.T.: -0.006 min
Response: 1664562
Conc: 12.71 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

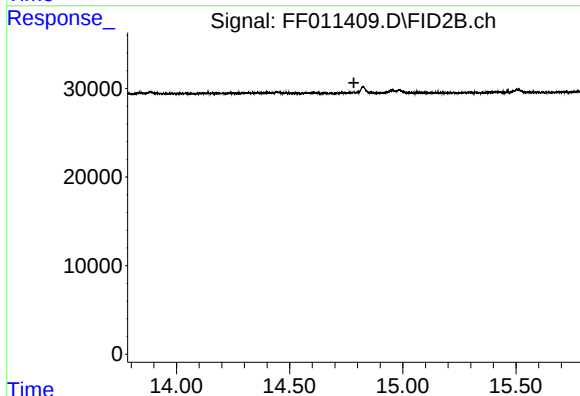


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

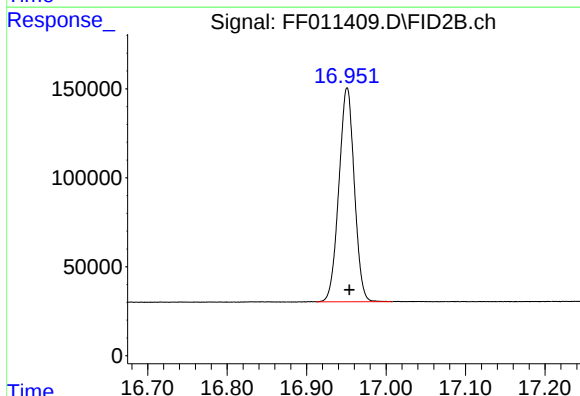


#12 N-OCTACOSANE

R.T.: 16.951 min
Delta R.T.: -0.003 min
Response: 1621345
Conc: 13.24 ug/ml

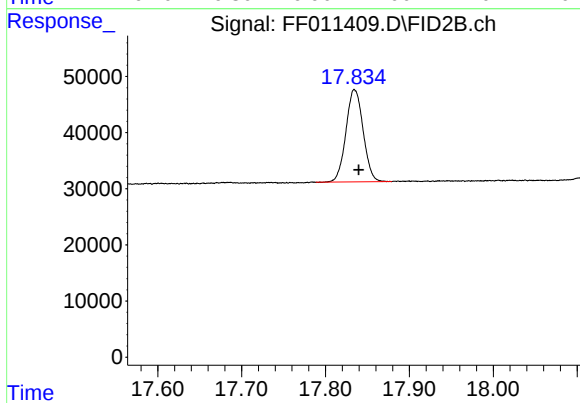

#13 N-TRIACONTANE


R.T.: 17.835 min
Delta R.T.: -0.005 min
Response: 234269
Conc: 1.94 ug/ml

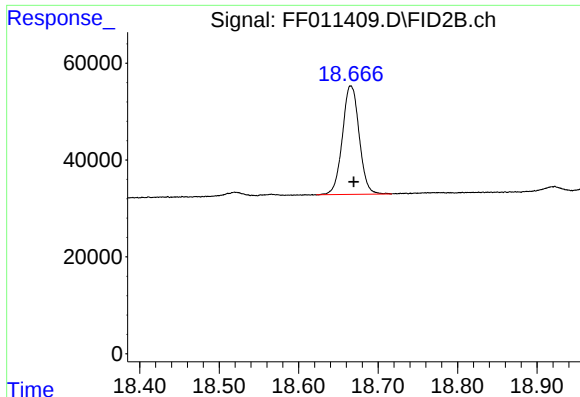

#14 N-DOTRIACONTANE


R.T.: 18.666 min
Delta R.T.: -0.004 min
Response: 328778
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

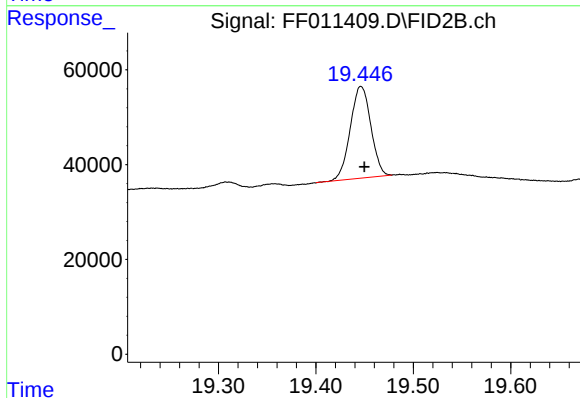


#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: -0.004 min
Response: 284003
Conc: 2.49 ug/ml

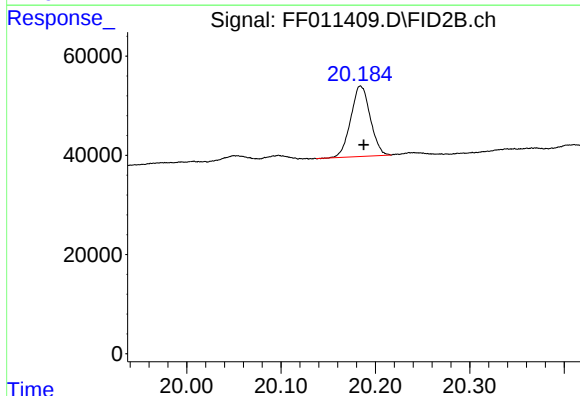


#16 N-HEXATRIACONTANE

R.T.: 20.184 min
Delta R.T.: -0.003 min
Response: 203953
Conc: 1.92 ug/ml

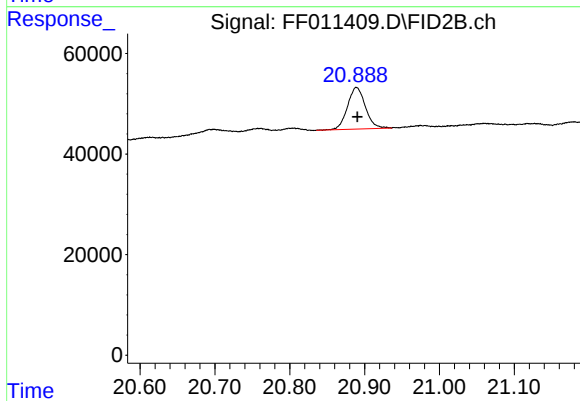

#17 N-OCTATRIACONTANE

R.T.: 20.889 min
Delta R.T.: -0.001 min
Response: 137312
Conc: 1.32 ug/ml

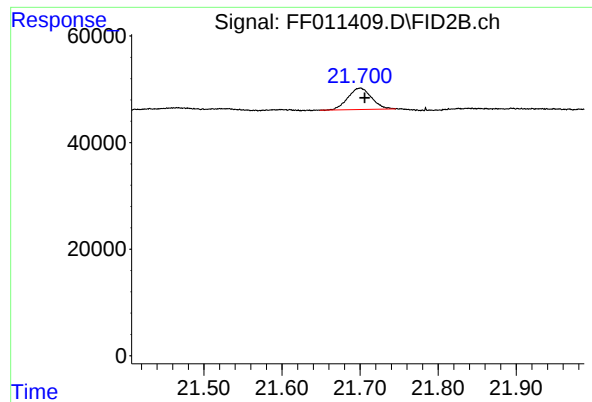

#18 N-TETRACONTANE

R.T.: 21.700 min
Delta R.T.: -0.006 min
Response: 84560
Conc: 0.80 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER