

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090822\
Data File : FF011419.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2022 20:39
Operator : YP\AJ
Sample : N4530-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-20-COMP

Integration File: autoint1.e
Quant Time: Sep 09 07:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	1344320	11.993 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.837	59228	0.491 ug/ml
14) N-DOTRIACONTANE	18.659	167894	1.419 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090822\
Data File : FF011419.D
Signal(s) : FID2B.ch
Acq On : 08 Sep 2022 20:39
Operator : YP\AJ
Sample : N4530-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-20-COMP

Integration File: autoint1.e
Quant Time: Sep 09 07:08:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

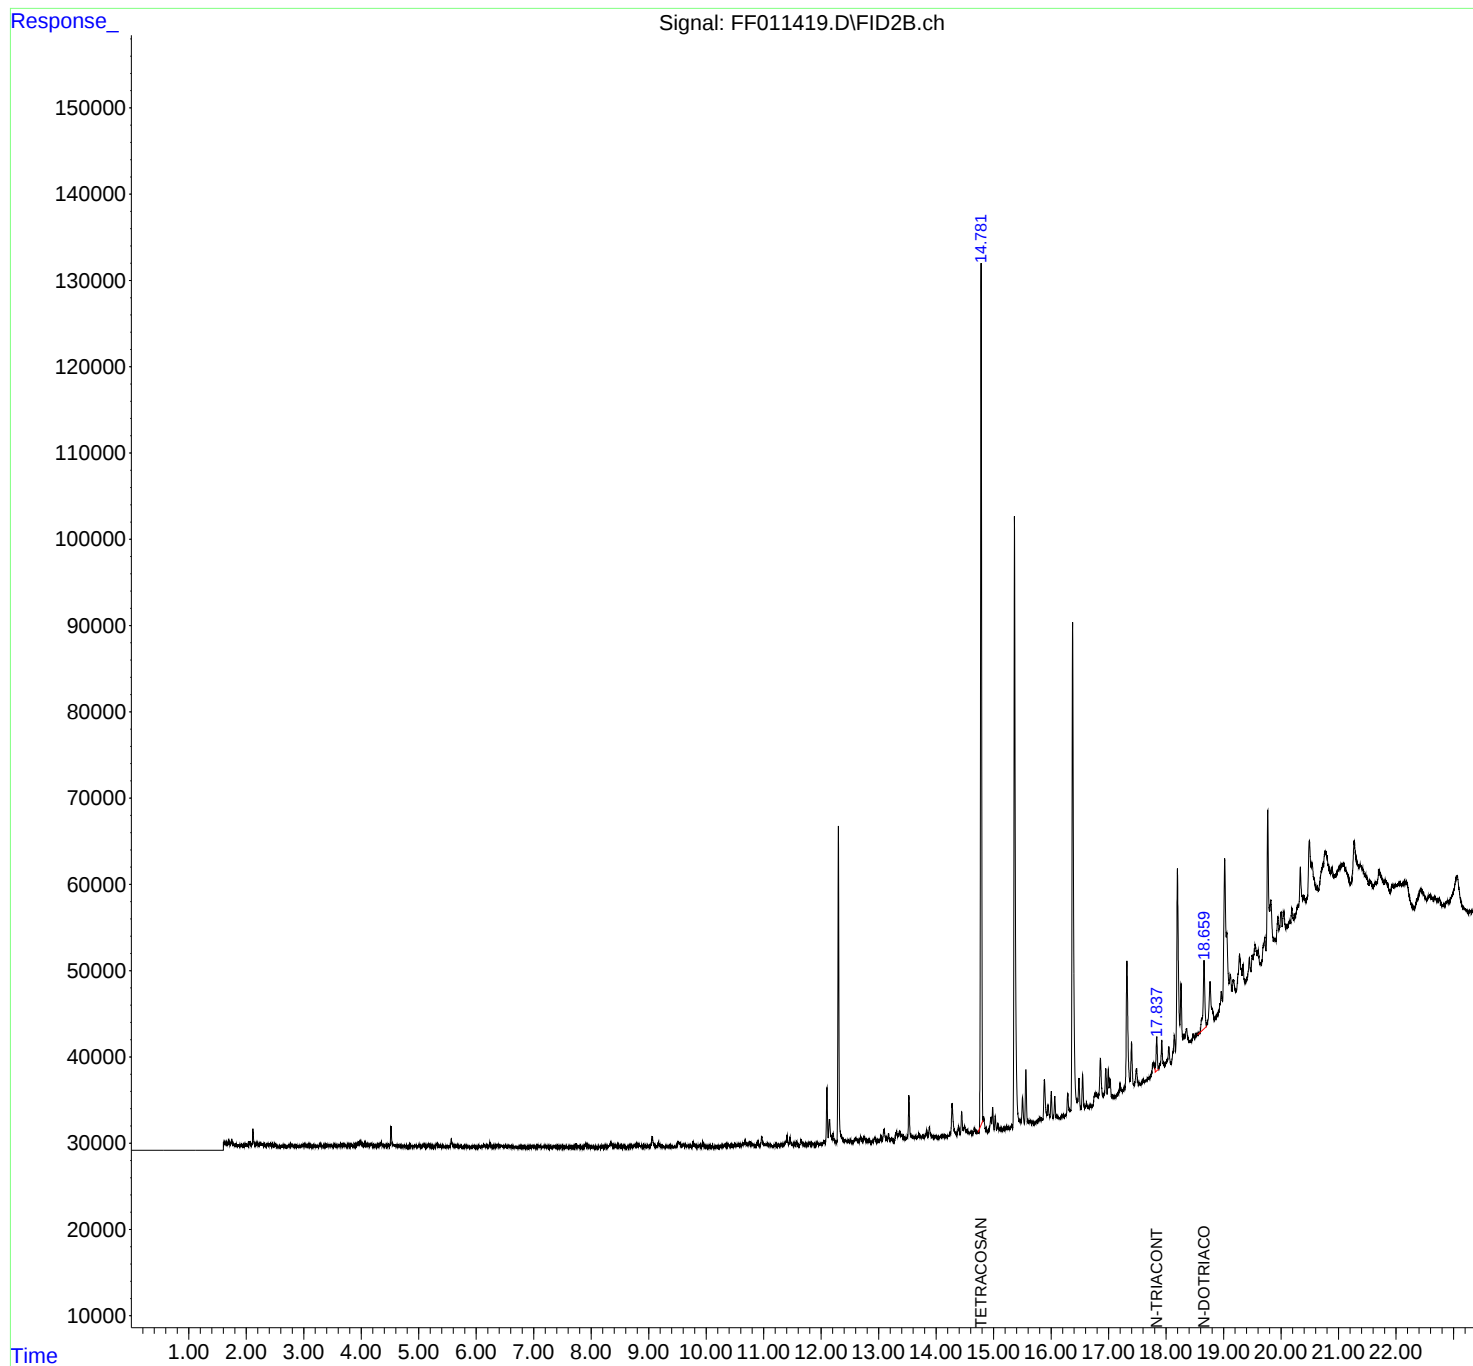


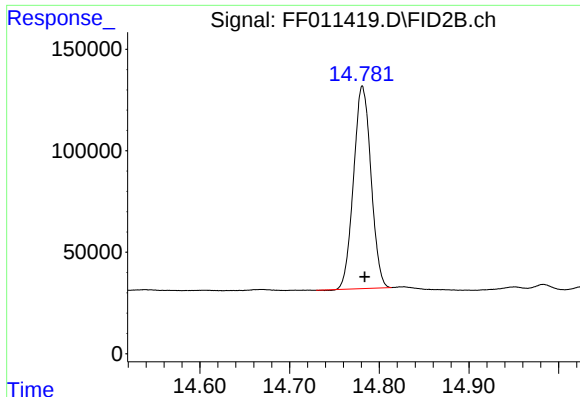

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.781 min
Delta R.T.: -0.003 min
Response: 1344320
Conc: 11.99 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-20-COMP

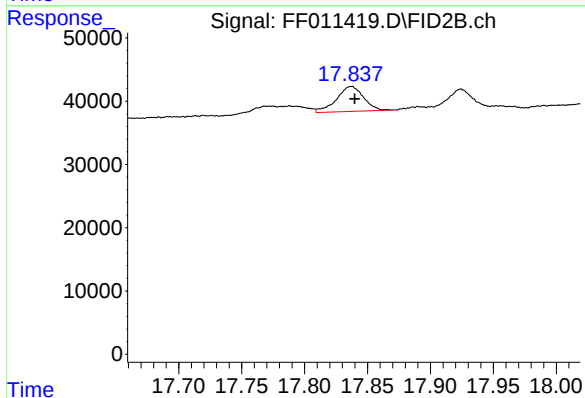

#13 N-TRIACONTANE

R.T.: 17.837 min
Delta R.T.: -0.003 min
Response: 59228
Conc: 0.49 ug/ml

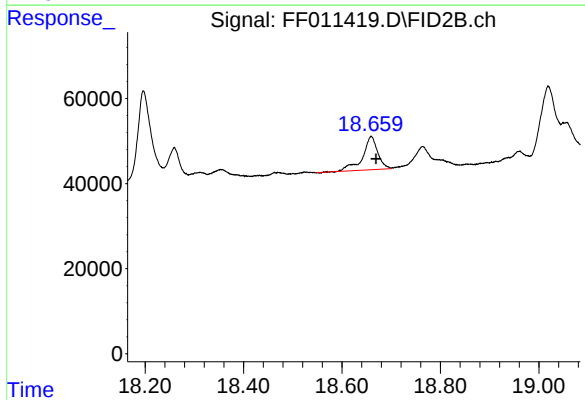

#14 N-DOTRIACONTANE

R.T.: 18.659 min
Delta R.T.: -0.010 min
Response: 167894
Conc: 1.42 ug/ml