

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005476.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 09:57
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Sep 09 16:21:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	306663	2.866 ug/ml
Target Compounds			
3) N-DODECANE	6.377	6760095	47.158 ug/ml
11) N-HEXACOSANE	15.857	109922	0.918 ug/ml
12) N-OCTACOSANE	16.816	6698448	56.136 ug/ml
13) N-TRIACONTANE	17.704	371965	3.075 ug/ml
14) N-DOTRIACONTANE	18.543	404866	3.266 ug/ml
15) N-TETRATRIACONTANE	19.335	271906	2.256 ug/ml
16) N-HEXATRIACONTANE	20.084	172776	1.440 ug/ml
18) N-TETRACONTANE	21.760	379064	2.982 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005476.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 09:57
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 09 16:21:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

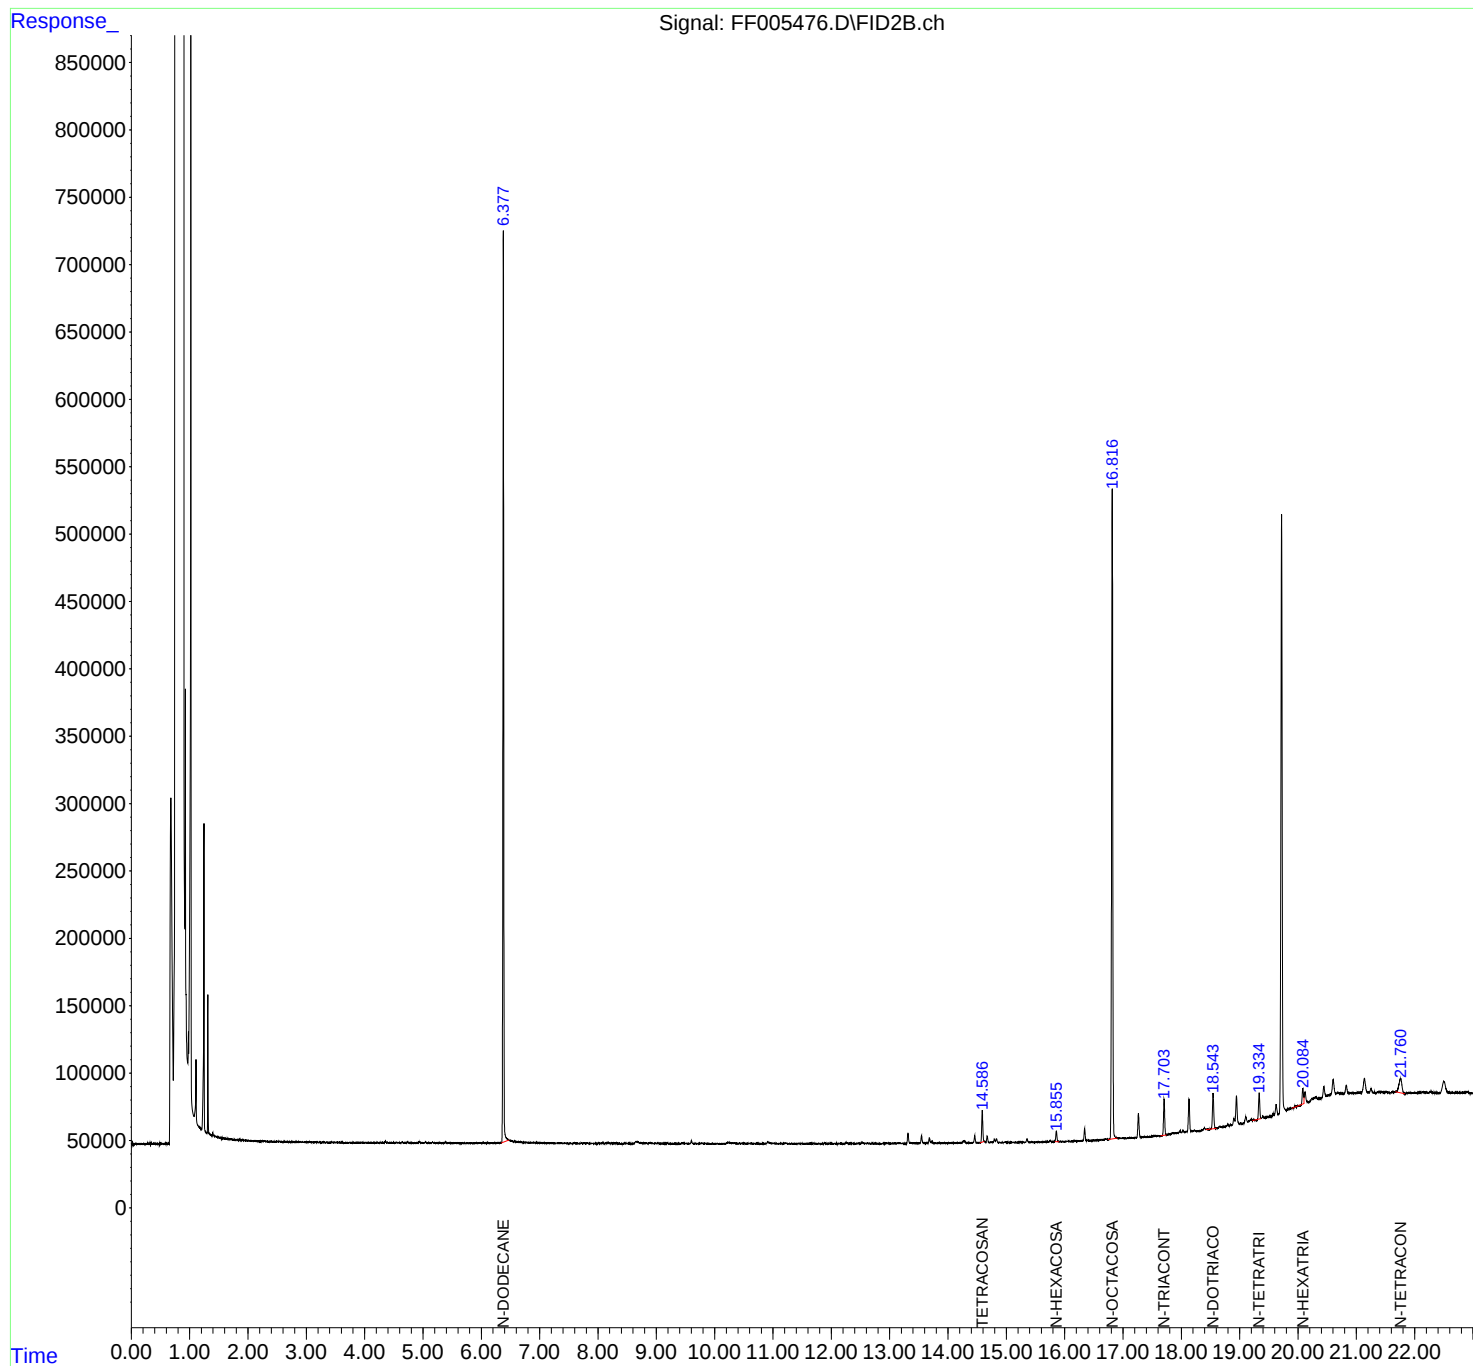


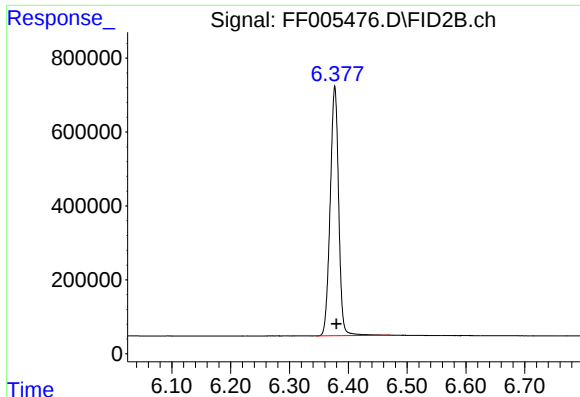

#3 N-DODECANE


R.T.: 6.377 min
Delta R.T.: -0.003 min
Response: 6760095
Conc: 47.16 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

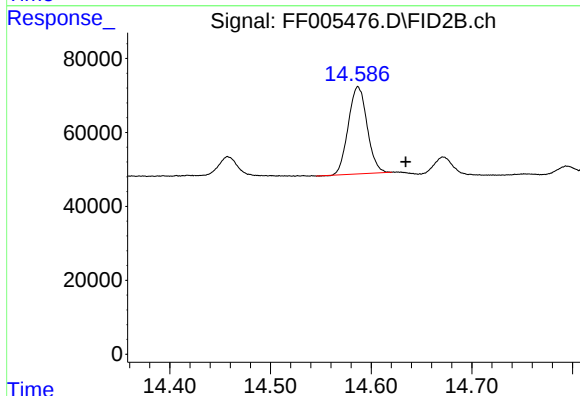


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min
Delta R.T.: -0.048 min
Response: 306663
Conc: 2.87 ug/ml

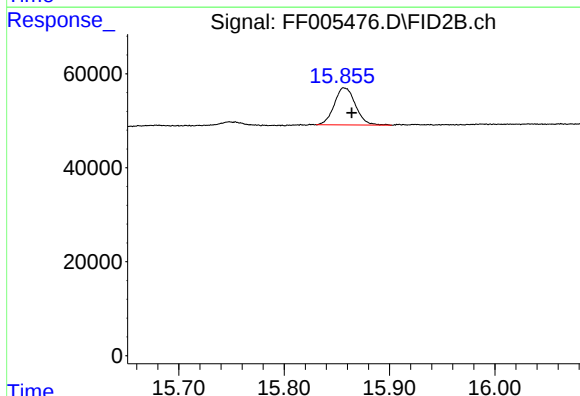


#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.007 min
Response: 109922
Conc: 0.92 ug/ml

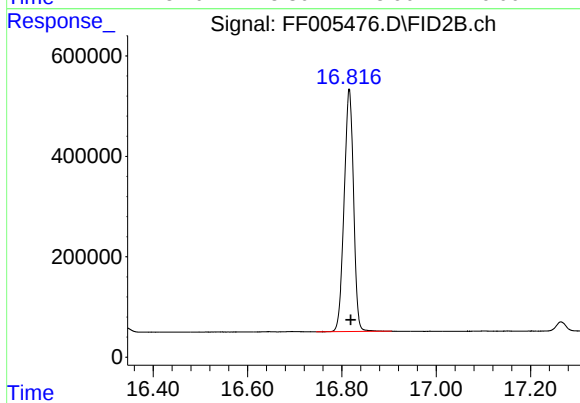

#12 N-OCTACOSANE


R.T.: 16.816 min
Delta R.T.: -0.003 min
Response: 6698448
Conc: 56.14 ug/ml

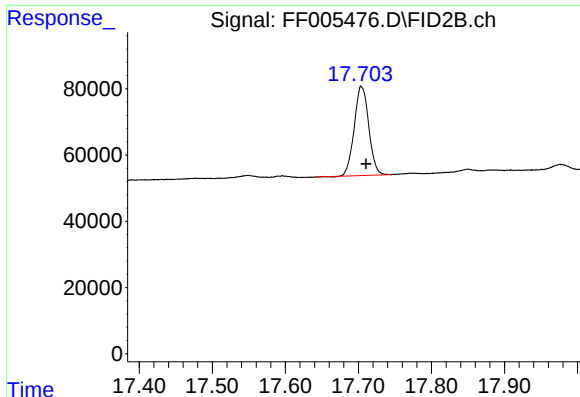

#13 N-TRIACONTANE


R.T.: 17.704 min
Delta R.T.: -0.007 min
Response: 371965
Conc: 3.07 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

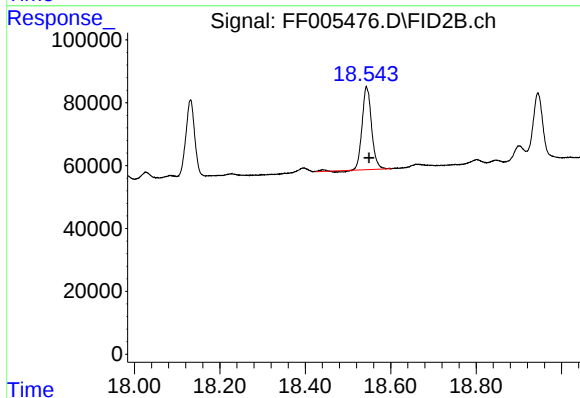


#14 N-DOTRIACONTANE

R.T.: 18.543 min
Delta R.T.: -0.006 min
Response: 404866
Conc: 3.27 ug/ml

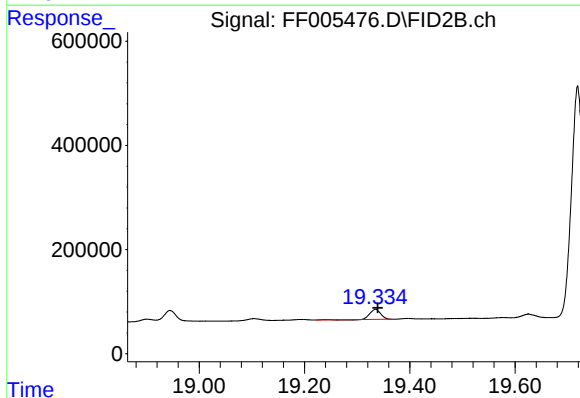


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: -0.004 min
Response: 271906
Conc: 2.26 ug/ml

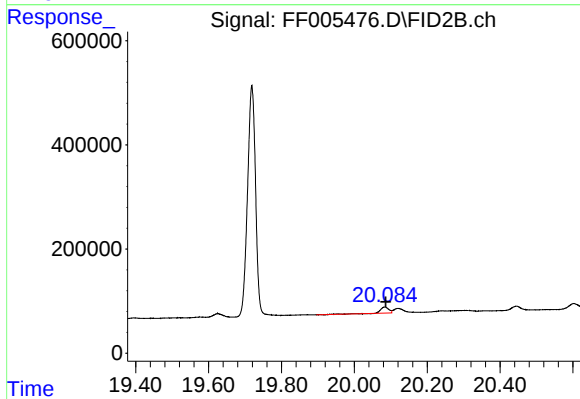

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: -0.003 min
Response: 172776
Conc: 1.44 ug/ml

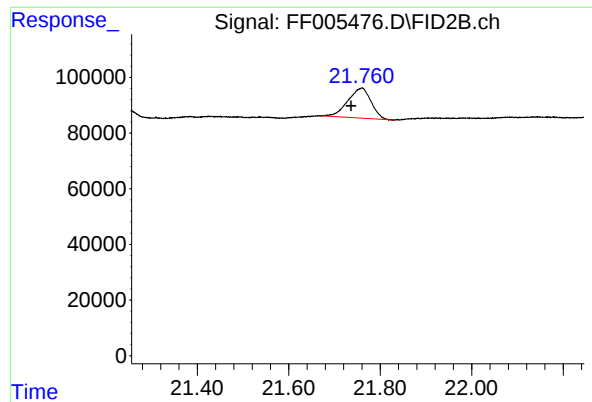

#18 N-TETRACONTANE

R.T.: 21.760 min
Delta R.T.: 0.023 min
Response: 379064
Conc: 2.98 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER