

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005479.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 11:31
 Operator : DD\AJ
 Sample : K4762-01 25X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 09 16:21:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.628	113032	1.056 ug/ml
Target Compounds			
3) N-DODECANE	6.396	116533	0.813 ug/ml
4) N-TETRADECANE	8.175	1529411	10.847 ug/ml
5) N-HEXADECANE	9.718f	265838	1.901 ug/ml
14) N-DOTRIACONTANE	18.547	160043	1.291 ug/ml
16) N-HEXATRIACONTANE	20.124	297279	2.477 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005479.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 11:31
Operator : DD\AJ
Sample : K4762-01 25X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 09 16:21:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

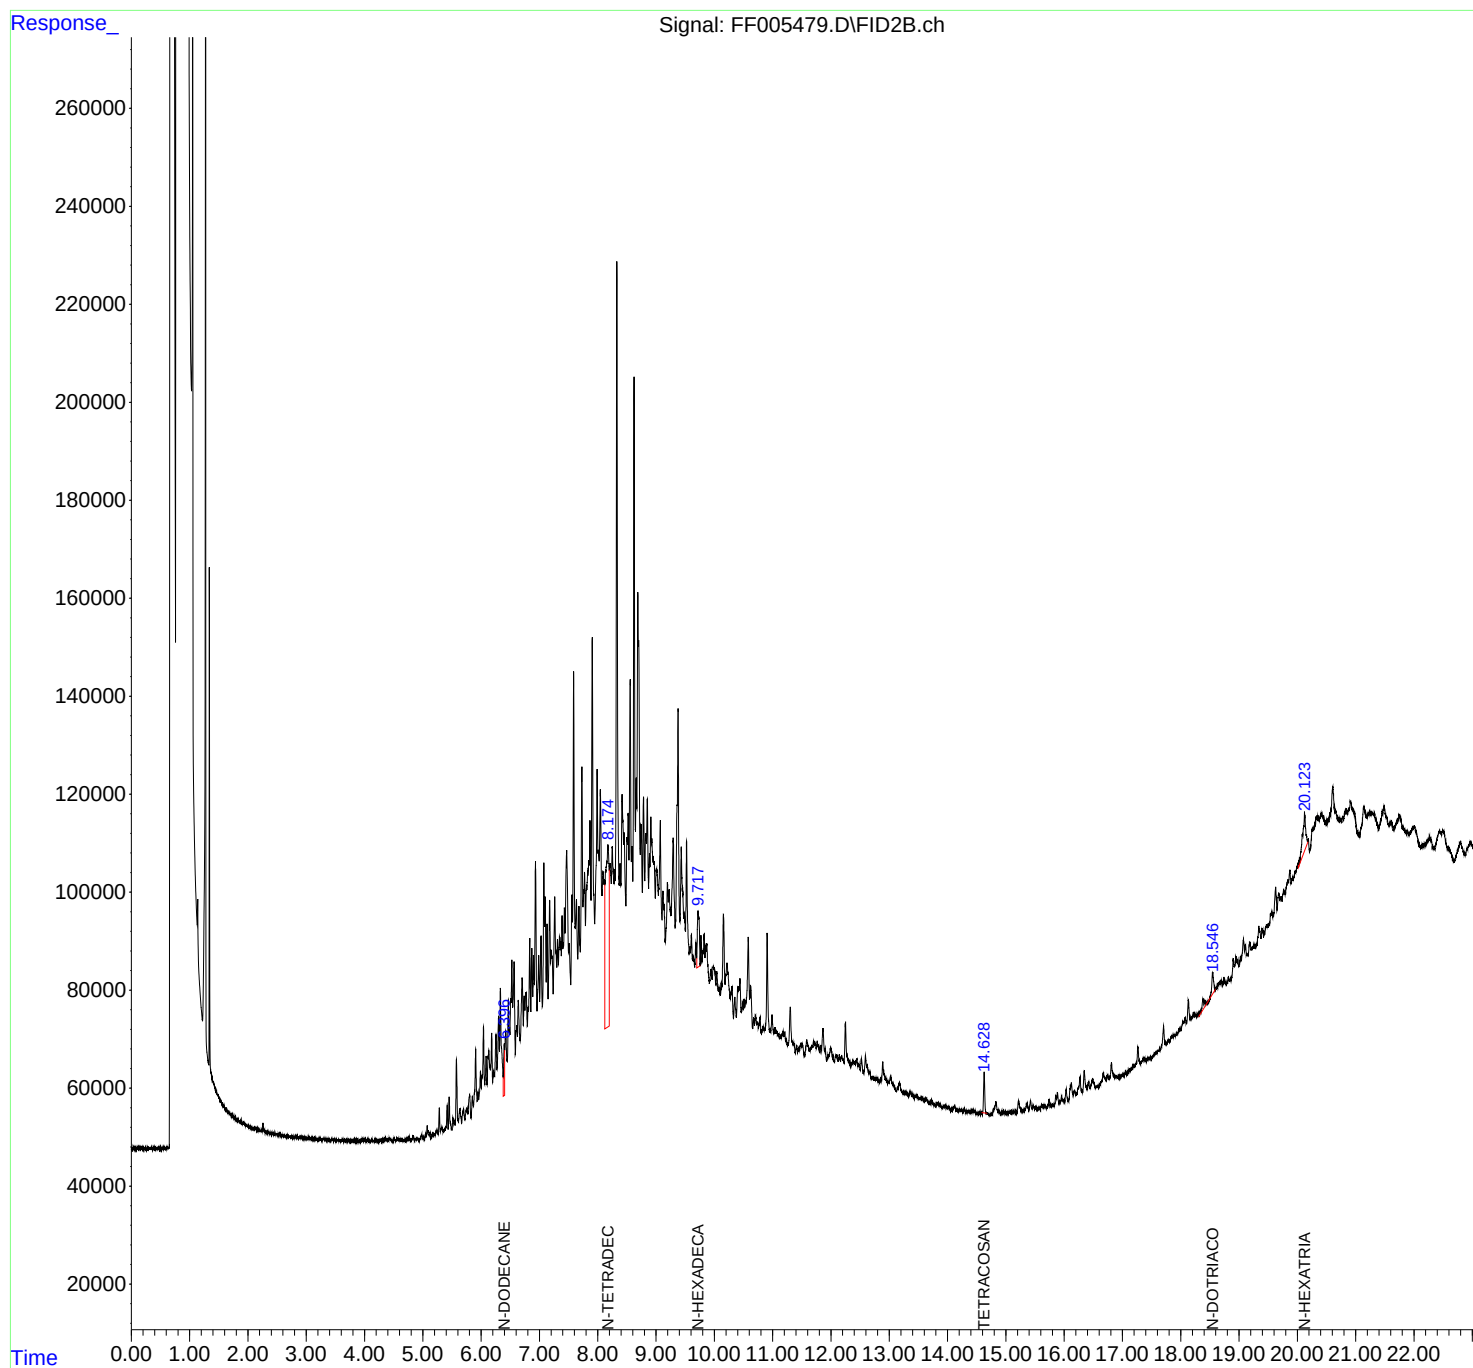


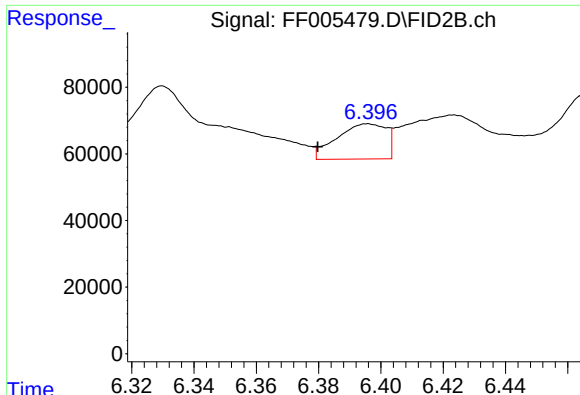

#3 N-DODECANE


R.T.: 6.396 min
Delta R.T.: 0.016 min
Response: 116533
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :

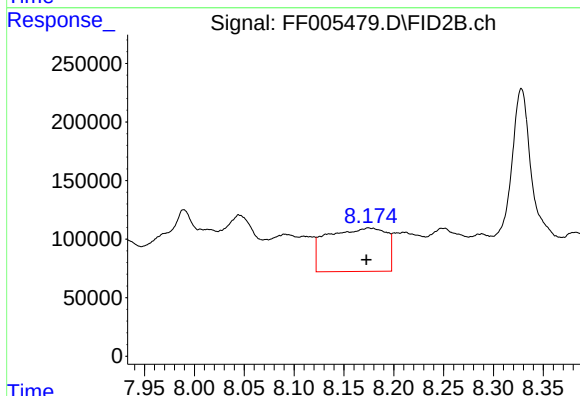


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: 0.002 min
Response: 1529411
Conc: 10.85 ug/ml

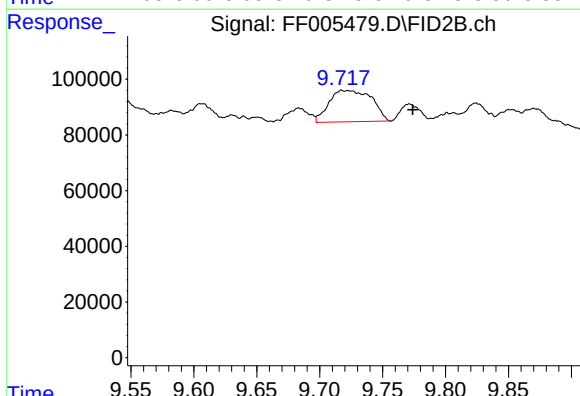


#5 N-HEXADECANE

R.T.: 9.718 min
Delta R.T.: -0.056 min
Response: 265838
Conc: 1.90 ug/ml

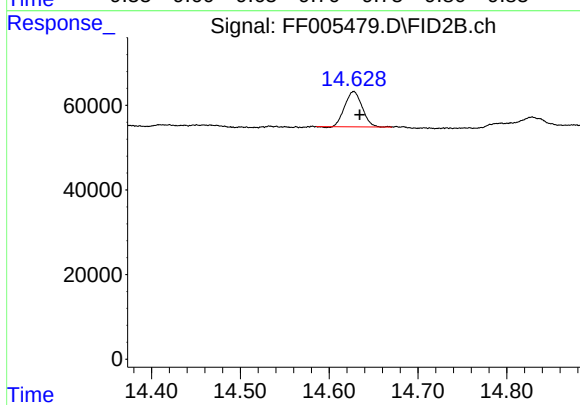

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.628 min
Delta R.T.: -0.007 min
Response: 113032
Conc: 1.06 ug/ml

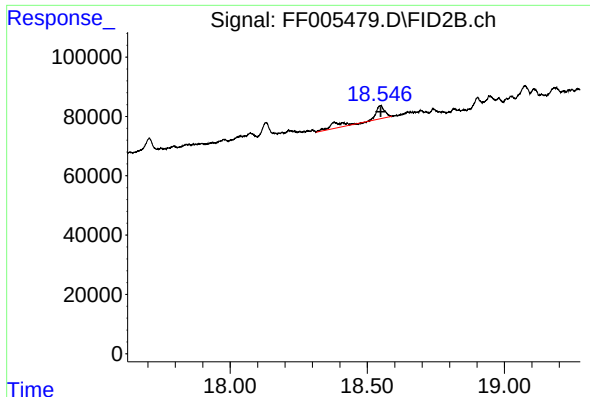

#14 N-DOTRIACONTANE

R.T.: 18.547 min
Delta R.T.: -0.002 min
Response: 160043
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :

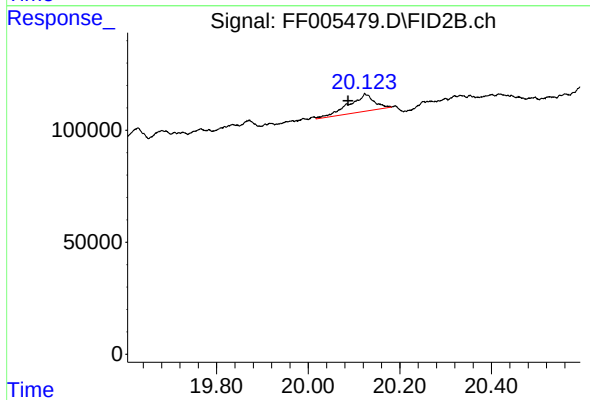

#16 N-HEXATRIACONTANE

R.T.: 20.124 min
Delta R.T.: 0.037 min
Response: 297279
Conc: 2.48 ug/ml