

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005484.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 14:04
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 10 03:37:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.585	351266	3.283 ug/ml
Target Compounds			
3) N-DODECANE	6.376	7178871	50.080 ug/ml
11) N-HEXACOSANE	15.856	113616	0.949 ug/ml
12) N-OCTACOSANE	16.815	6919866	57.992 ug/ml
13) N-TRIACONTANE	17.704	394589	3.262 ug/ml
14) N-DOTRIACONTANE	18.543	435409	3.512 ug/ml
15) N-TETRATRIACONTANE	19.335	303848	2.521 ug/ml
16) N-HEXATRIACONTANE	20.084	126099	1.051 ug/ml
17) N-OCTATRIACONTANE	20.829	131843	1.208 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005484.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 14:04
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 03:37:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

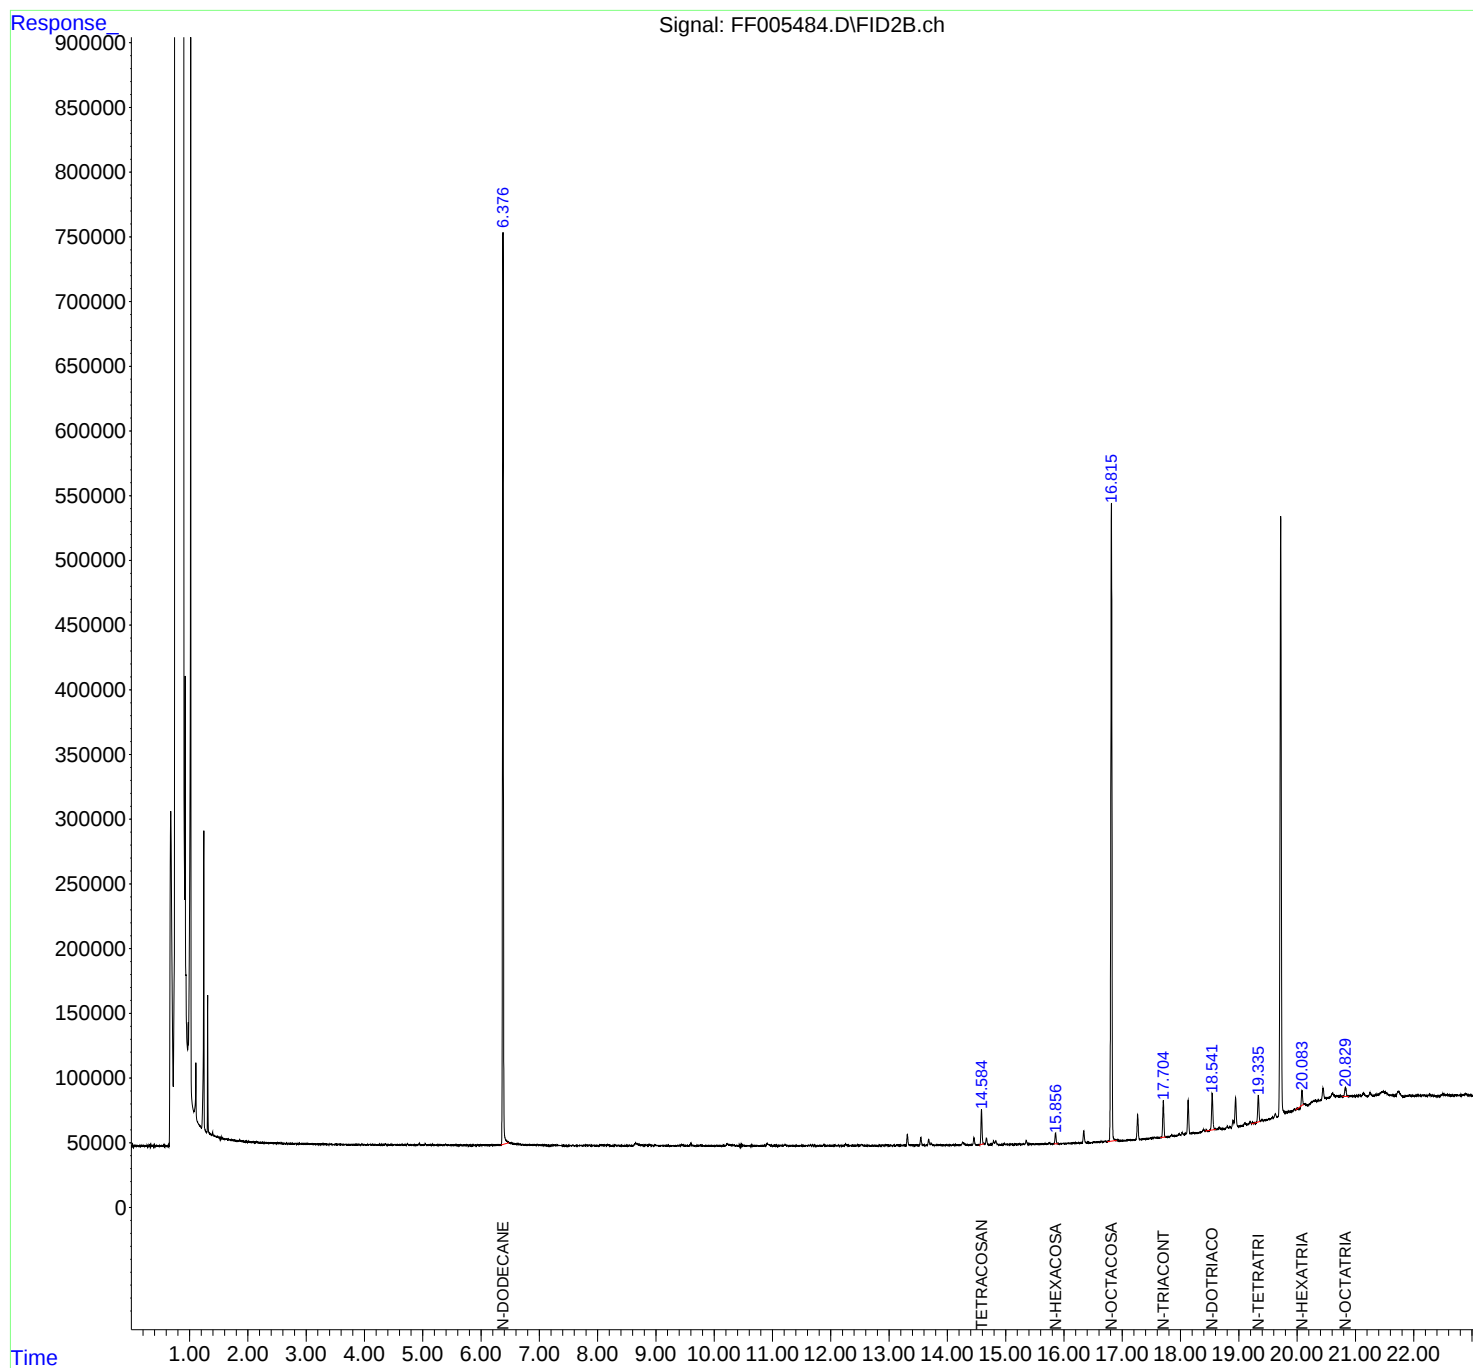


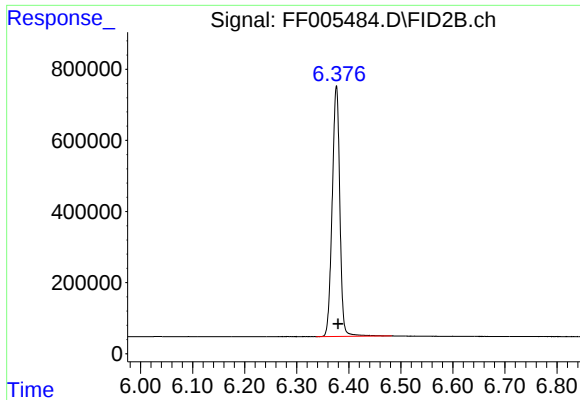

#3 N-DODECANE


R.T.: 6.376 min
Delta R.T.: -0.003 min
Response: 7178871
Conc: 50.08 ug/ml

Instrument :
FID_F
ClientSampleId :

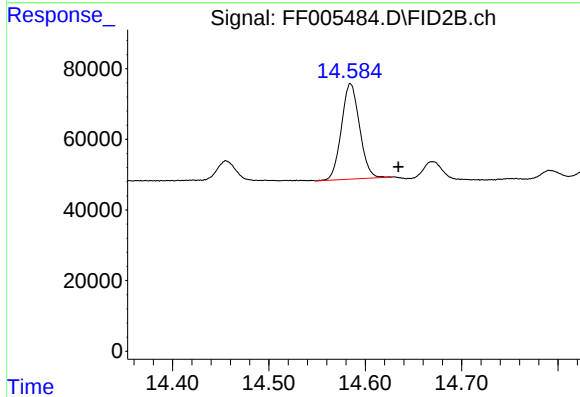


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.585 min
Delta R.T.: -0.050 min
Response: 351266
Conc: 3.28 ug/ml

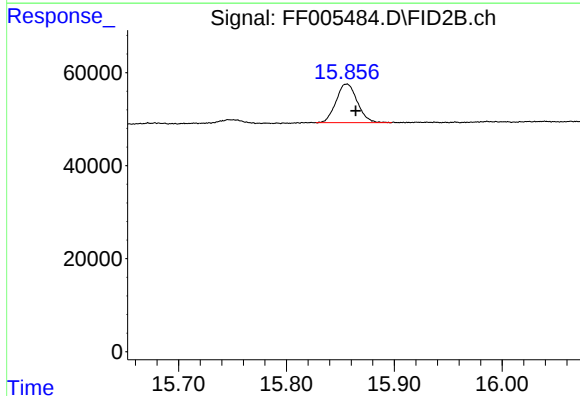


#11 N-HEXACOSANE

R.T.: 15.856 min
Delta R.T.: -0.008 min
Response: 113616
Conc: 0.95 ug/ml

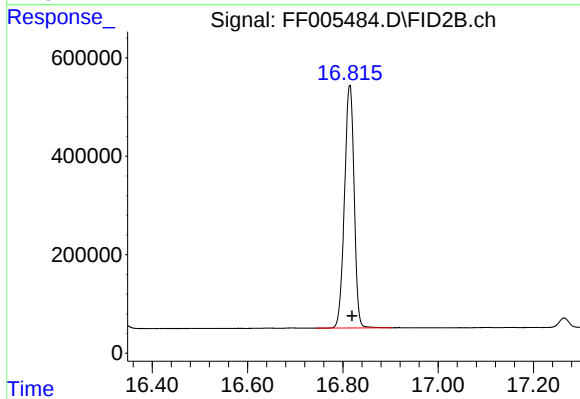

#12 N-OCTACOSANE


R.T.: 16.815 min
Delta R.T.: -0.004 min
Response: 6919866
Conc: 57.99 ug/ml

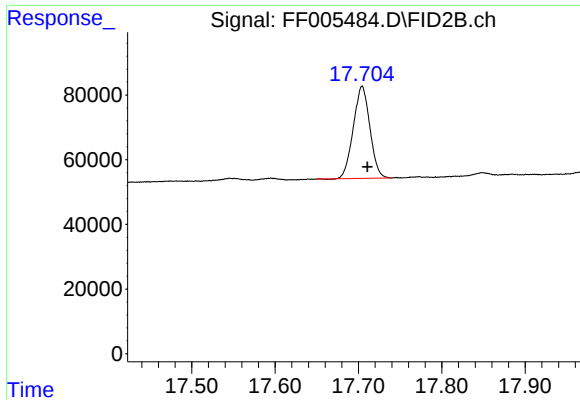

#13 N-TRIACONTANE


R.T.: 17.704 min
Delta R.T.: -0.006 min
Response: 394589
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :

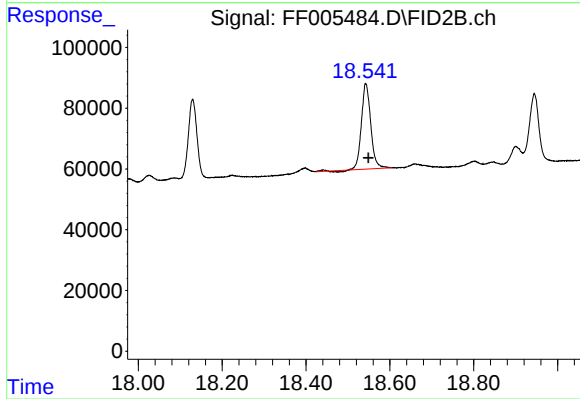


#14 N-DOTRIACONTANE

R.T.: 18.543 min
Delta R.T.: -0.007 min
Response: 435409
Conc: 3.51 ug/ml

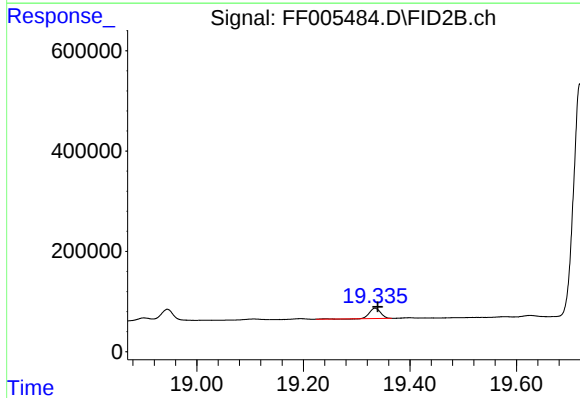


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: -0.005 min
Response: 303848
Conc: 2.52 ug/ml

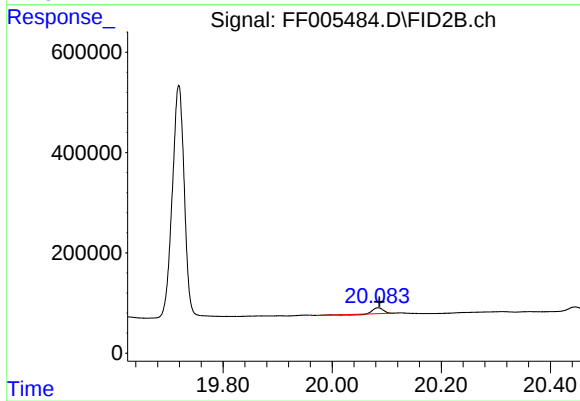

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: -0.002 min
Response: 126099
Conc: 1.05 ug/ml

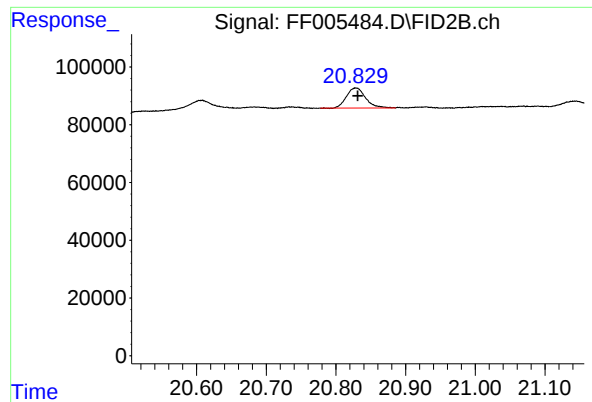

#17 N-OCTATRIACONTANE

R.T.: 20.829 min
Delta R.T.: -0.003 min
Response: 131843
Conc: 1.21 ug/ml

Instrument :
FID_F
ClientSampleId :