

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005496.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 20:05
Operator : DD\AJ
Sample : K4752-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 03:41:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	1758073	16.429 ug/ml
Target Compounds			
4) N-TETRADECANE	8.227f	393405	2.790 ug/ml
13) N-TRIACONTANE	17.701	137815	1.139 ug/ml
14) N-DOTRIACONTANE	18.538	168080	1.356 ug/ml
16) N-HEXATRIACONTANE	20.079	32717	0.273 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005496.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 20:05
Operator : DD\AJ
Sample : K4752-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 10 03:41:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

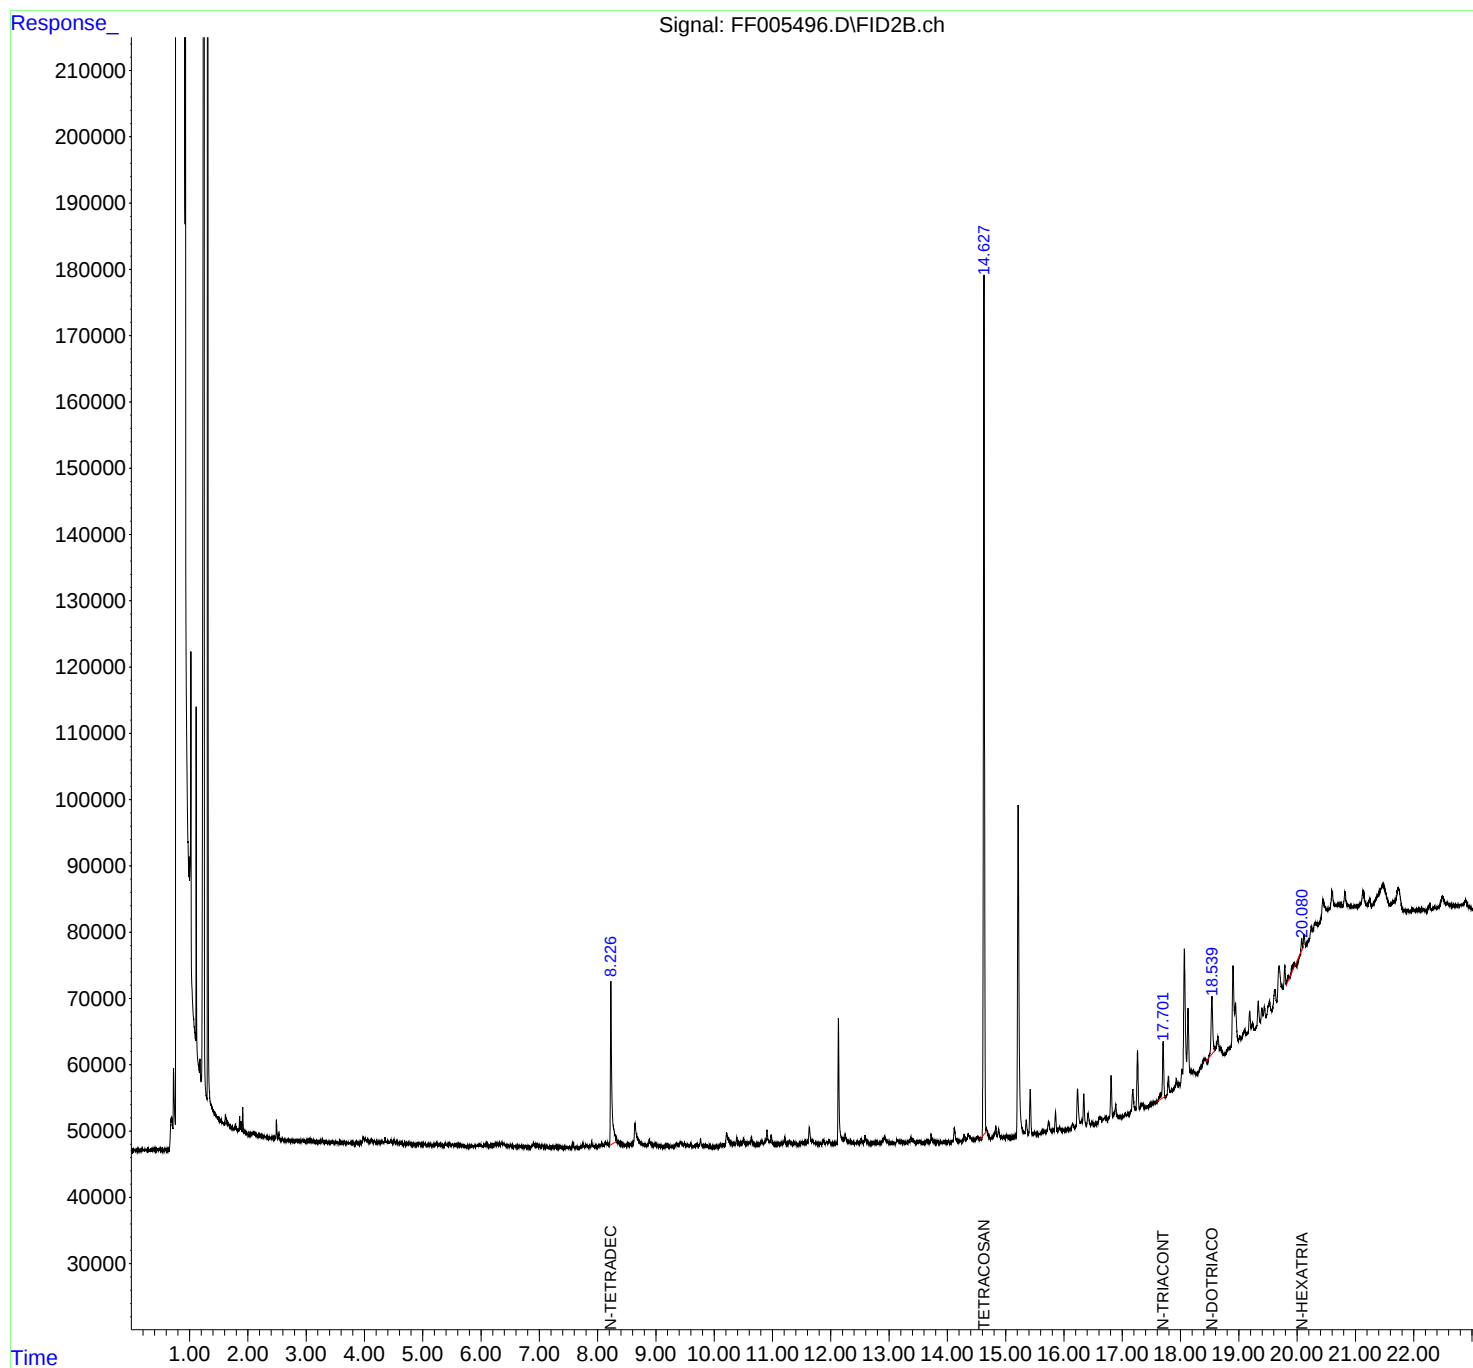


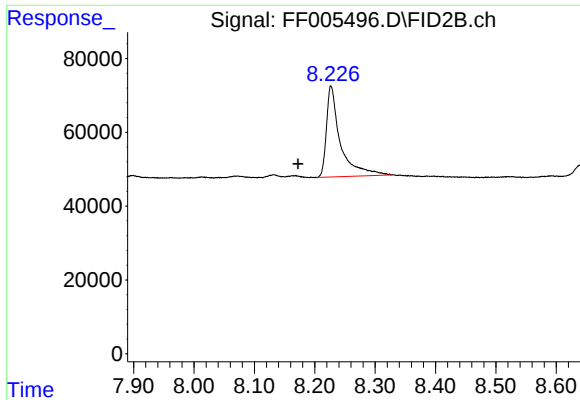

#4 N-TETRADECANE


R.T.: 8.227 min
Delta R.T.: 0.055 min
Response: 393405
Conc: 2.79 ug/ml

Instrument :
FID_F
ClientSampleId :

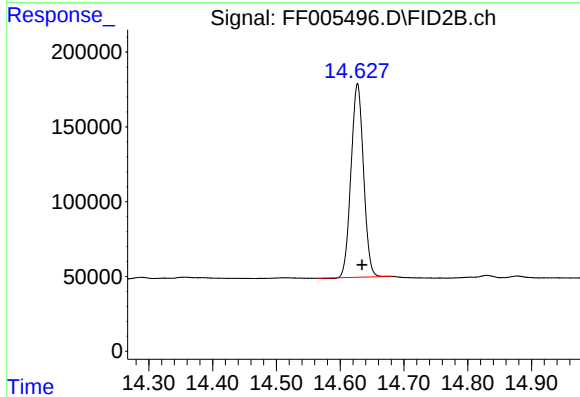


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.007 min
Response: 1758073
Conc: 16.43 ug/ml

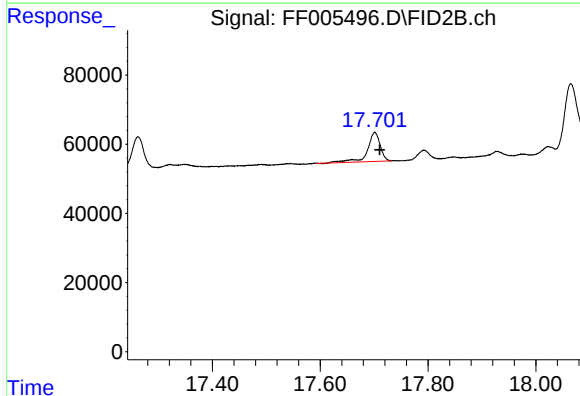


#13 N-TRIACONTANE

R.T.: 17.701 min
Delta R.T.: -0.009 min
Response: 137815
Conc: 1.14 ug/ml

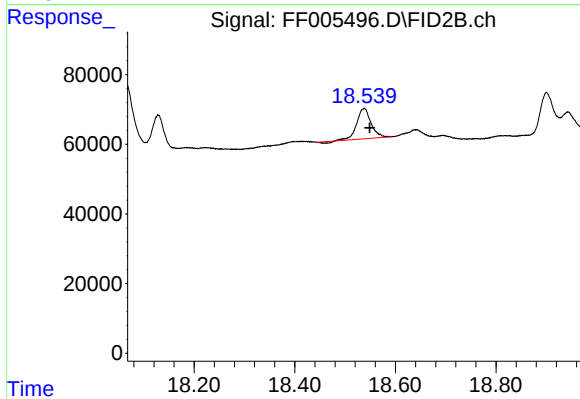

#14 N-DOTRIACONTANE

R.T.: 18.538 min
Delta R.T.: -0.011 min
Response: 168080
Conc: 1.36 ug/ml

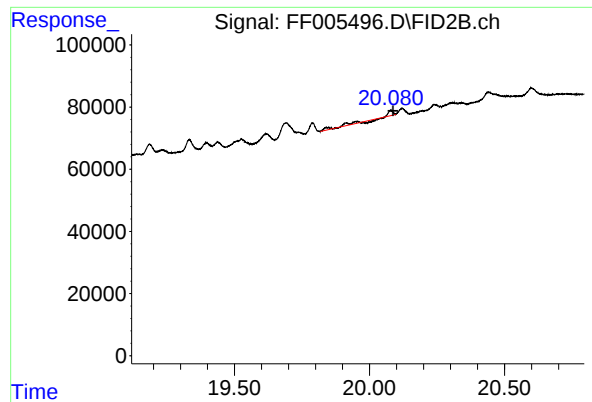

#16 N-HEXATRIACONTANE

R.T.: 20.079 min
Delta R.T.: -0.008 min
Response: 32717
Conc: 0.27 ug/ml

Instrument :
FID_F
ClientSampleId :