

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005497.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 20:35
 Operator : DD\AJ
 Sample : K4752-06
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-13-COMP

Integration File: autoint1.e
 Quant Time: Sep 10 03:42:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	1854987	17.335 ug/ml
Target Compounds			
4) N-TETRADECANE	8.131	179791	1.275 ug/ml
10) N-TETRACOSANE	14.830	141975	1.161 ug/ml
11) N-HEXACOSANE	15.855	215789	1.803 ug/ml
12) N-OCTACOSANE	16.809	211844	1.775 ug/ml
13) N-TRIACONTANE	17.702	223757	1.850 ug/ml
14) N-DOTRIACONTANE	18.539	223898	1.806 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005497.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 20:35
Operator : DD\AJ
Sample : K4752-06
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-13-COMP

Integration File: autoint1.e
Quant Time: Sep 10 03:42:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

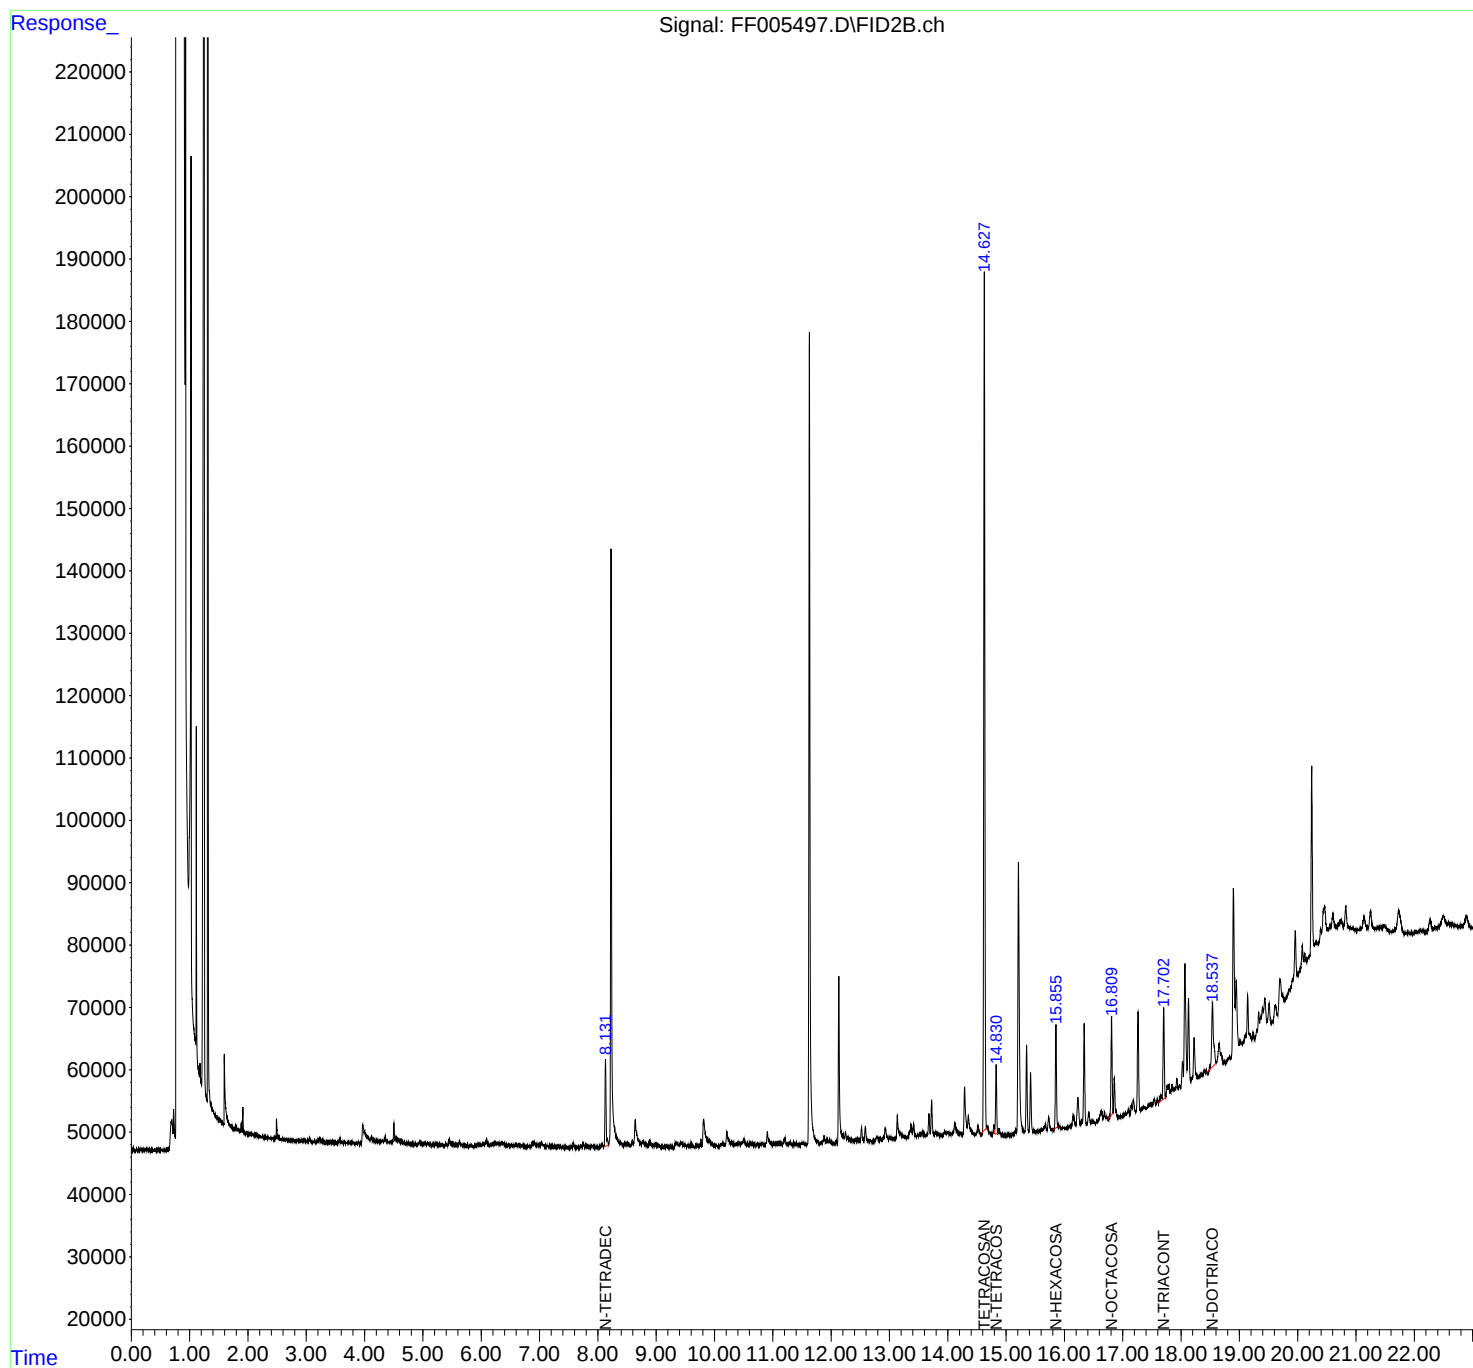


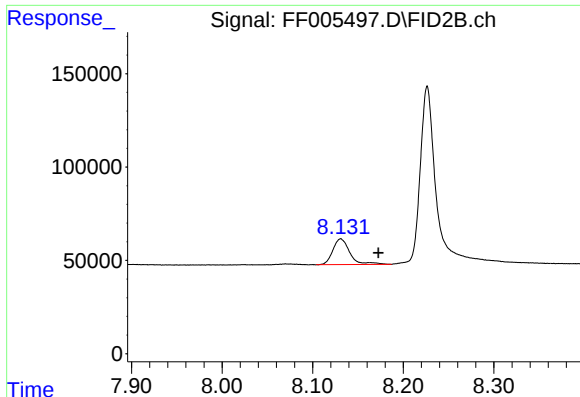

#4 N-TETRADECANE


R.T.: 8.131 min
Delta R.T.: -0.042 min
Response: 179791
Conc: 1.28 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-13-COMP

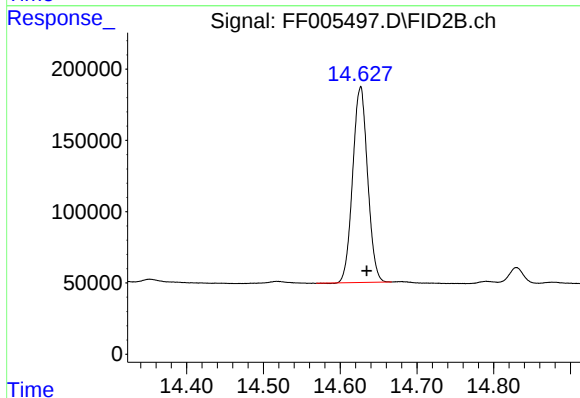


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.008 min
Response: 1854987
Conc: 17.33 ug/ml

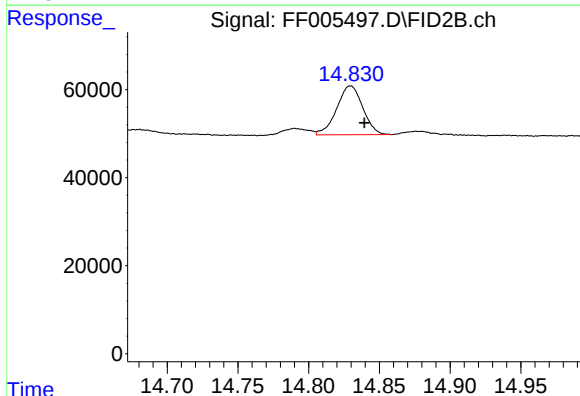


#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: -0.010 min
Response: 141975
Conc: 1.16 ug/ml

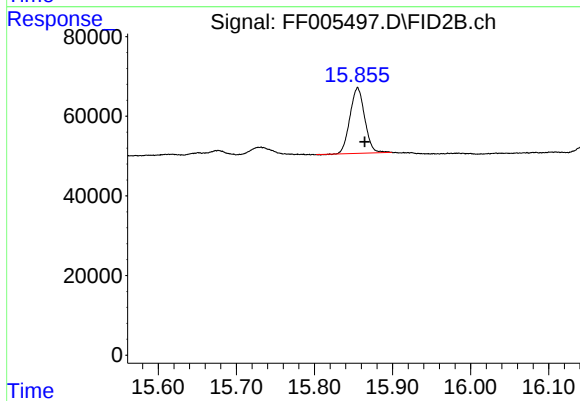

#11 N-HEXACOSANE


R.T.: 15.855 min
Delta R.T.: -0.009 min
Response: 215789
Conc: 1.80 ug/ml

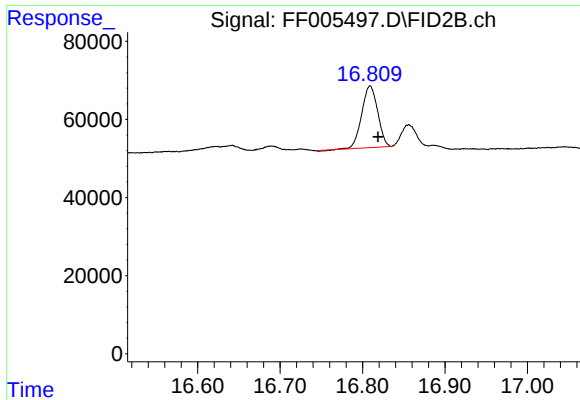

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.010 min
Response: 211844
Conc: 1.78 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-13-COMP

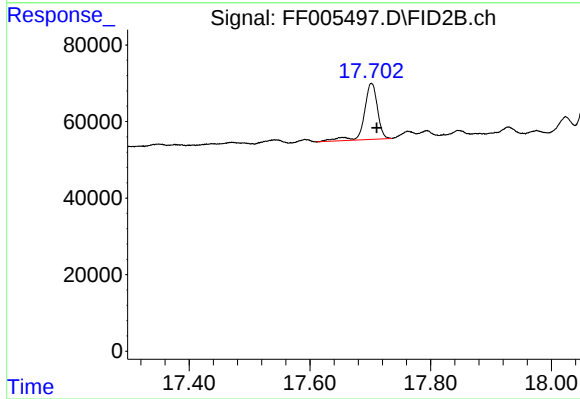

#13 N-TRIACONTANE

R.T.: 17.702 min
Delta R.T.: -0.009 min
Response: 223757
Conc: 1.85 ug/ml

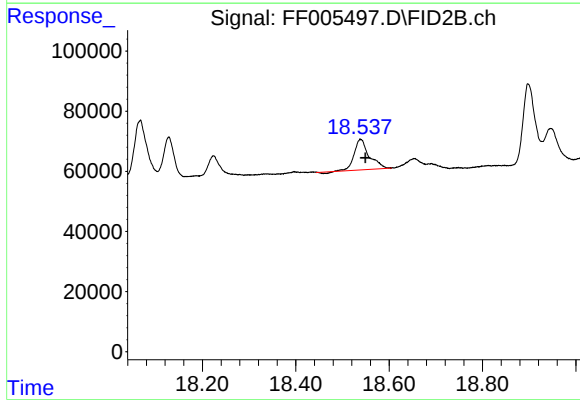

#14 N-DOTRIACONTANE

R.T.: 18.539 min
Delta R.T.: -0.010 min
Response: 223898
Conc: 1.81 ug/ml