

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005500.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 22:04
 Operator : DD\AJ
 Sample : K4752-10
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-12-COMP

Integration File: autoint1.e
 Quant Time: Sep 10 03:43:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	1481635	13.846 ug/ml
Target Compounds			
4) N-TETRADECANE	8.131	430160	3.051 ug/ml
10) N-TETRACOSANE	14.829	155918	1.275 ug/ml
11) N-HEXACOSANE	15.854	268392	2.242 ug/ml
12) N-OCTACOSANE	16.809	343605	2.880 ug/ml
13) N-TRIACONTANE	17.700	415086	3.431 ug/ml
14) N-DOTRIACONTANE	18.538	373867	3.016 ug/ml
15) N-TETRATRIACONTANE	19.376	96680	0.802 ug/ml
16) N-HEXATRIACONTANE	20.100	233835	1.948 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005500.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 22:04
Operator : DD\AJ
Sample : K4752-10
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-12-COMP

Integration File: autoint1.e
Quant Time: Sep 10 03:43:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

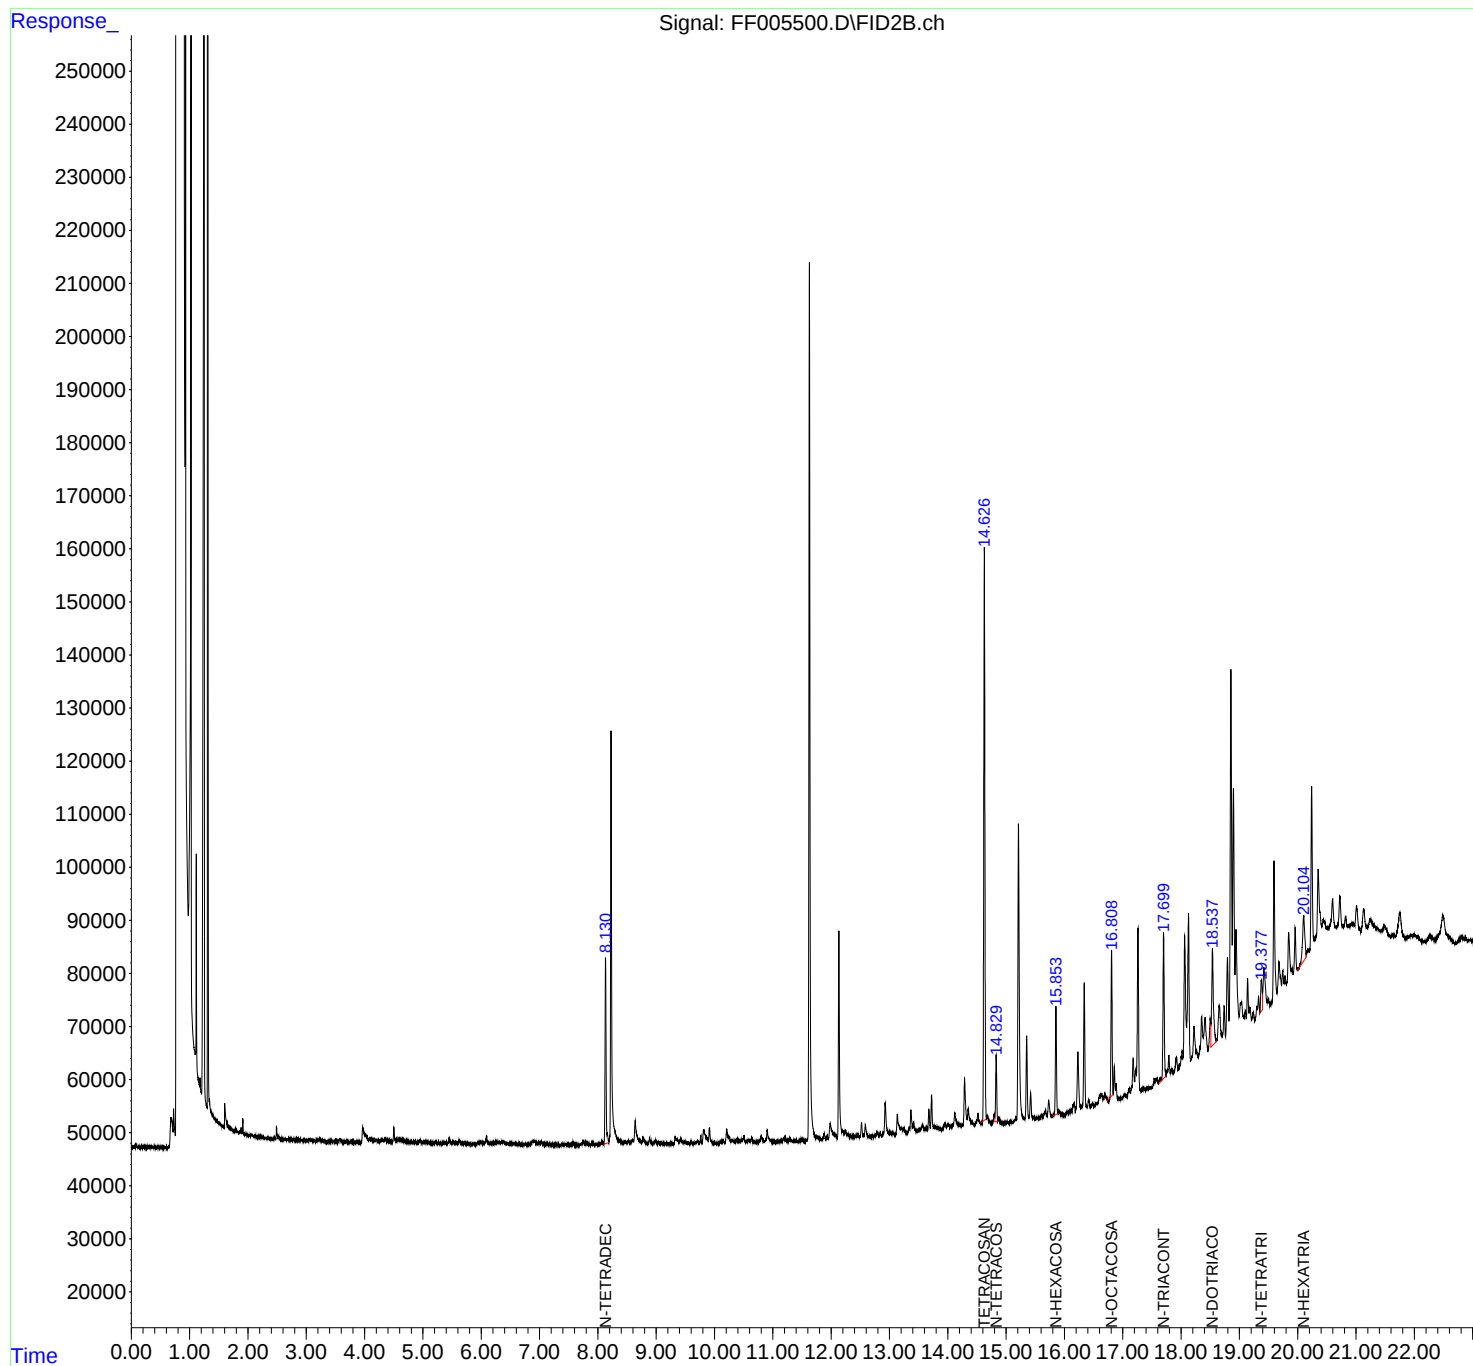


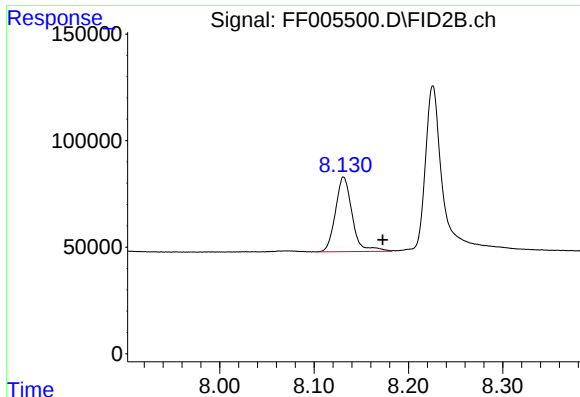

#4 N-TETRADECANE


R.T.: 8.131 min
Delta R.T.: -0.041 min
Response: 430160
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-12-COMP

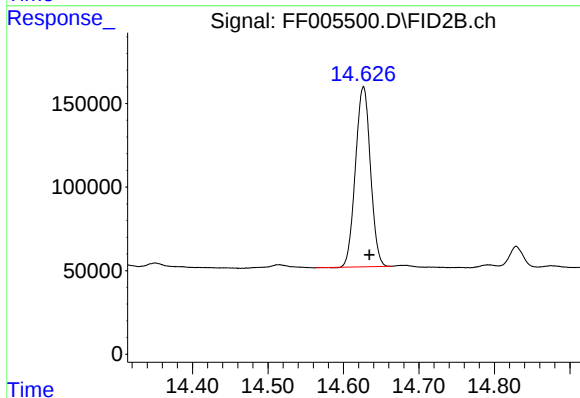


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.008 min
Response: 1481635
Conc: 13.85 ug/ml

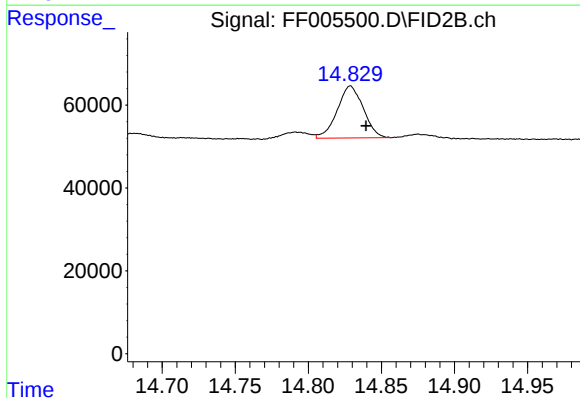


#10 N-TETRACOSANE

R.T.: 14.829 min
Delta R.T.: -0.011 min
Response: 155918
Conc: 1.27 ug/ml

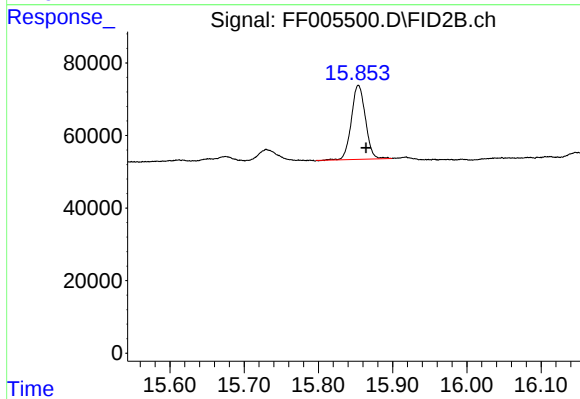

#11 N-HEXACOSANE


R.T.: 15.854 min
Delta R.T.: -0.010 min
Response: 268392
Conc: 2.24 ug/ml

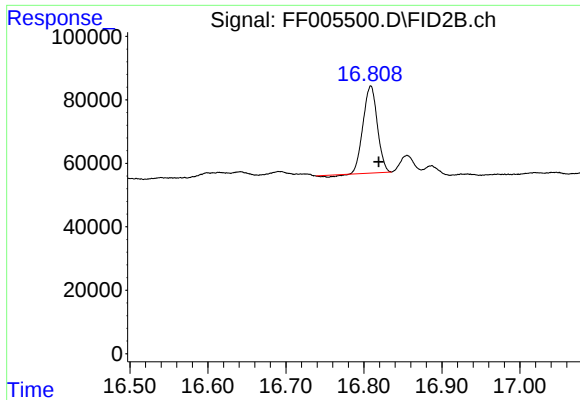

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.010 min
Response: 343605
Conc: 2.88 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-12-COMP

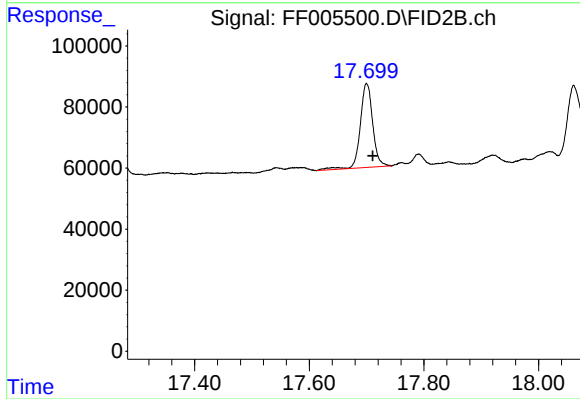


#13 N-TRIACONTANE

R.T.: 17.700 min
Delta R.T.: -0.011 min
Response: 415086
Conc: 3.43 ug/ml

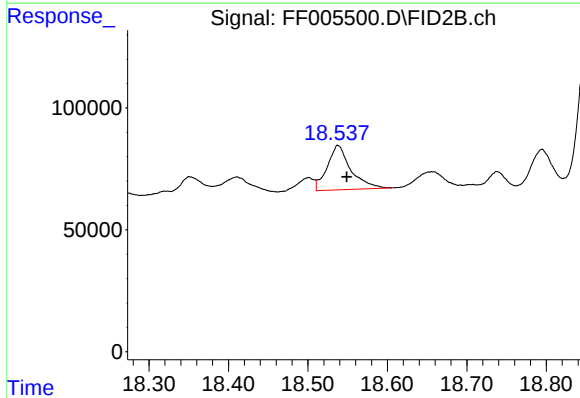


#14 N-DOTRIACONTANE

R.T.: 18.538 min
Delta R.T.: -0.011 min
Response: 373867
Conc: 3.02 ug/ml

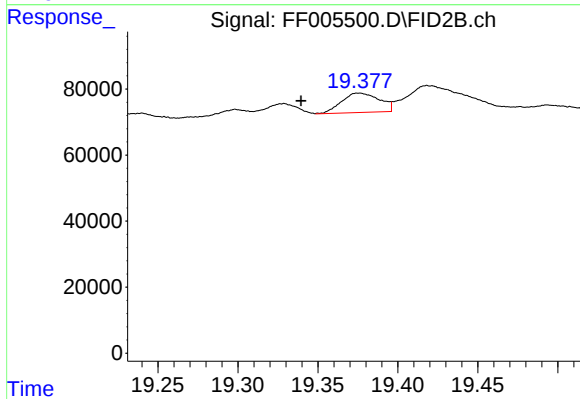

#15 N-TETRATRIACONTANE

R.T.: 19.376 min
Delta R.T.: 0.036 min
Response: 96680
Conc: 0.80 ug/ml

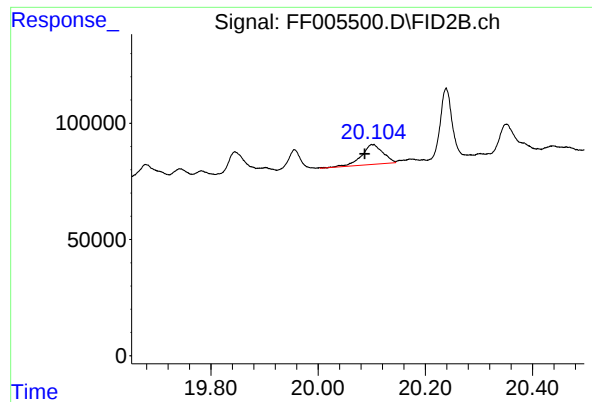

#16 N-HEXATRIACONTANE

R.T.: 20.100 min
Delta R.T.: 0.014 min
Response: 233835
Conc: 1.95 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-12-COMP