

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005501.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 22:33
 Operator : DD\AJ
 Sample : K4752-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-15-COMP

Integration File: autoint1.e
 Quant Time: Sep 10 03:43:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	1495716	13.978 ug/ml
Target Compounds			
4) N-TETRADECANE	8.133	620591	4.402 ug/ml
10) N-TETRACOSANE	14.829	302418	2.473 ug/ml
11) N-HEXACOSANE	15.855	263607	2.202 ug/ml
12) N-OCTACOSANE	16.809	422183	3.538 ug/ml
13) N-TRIACONTANE	17.701	467464	3.864 ug/ml
14) N-DOTRIACONTANE	18.537	379747	3.063 ug/ml
16) N-HEXATRIACONTANE	20.113	243547	2.029 ug/ml
18) N-TETRACONTANE	21.748	359911	2.831 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005501.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 22:33
Operator : DD\AJ
Sample : K4752-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-15-COMP

Integration File: autoint1.e
Quant Time: Sep 10 03:43:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

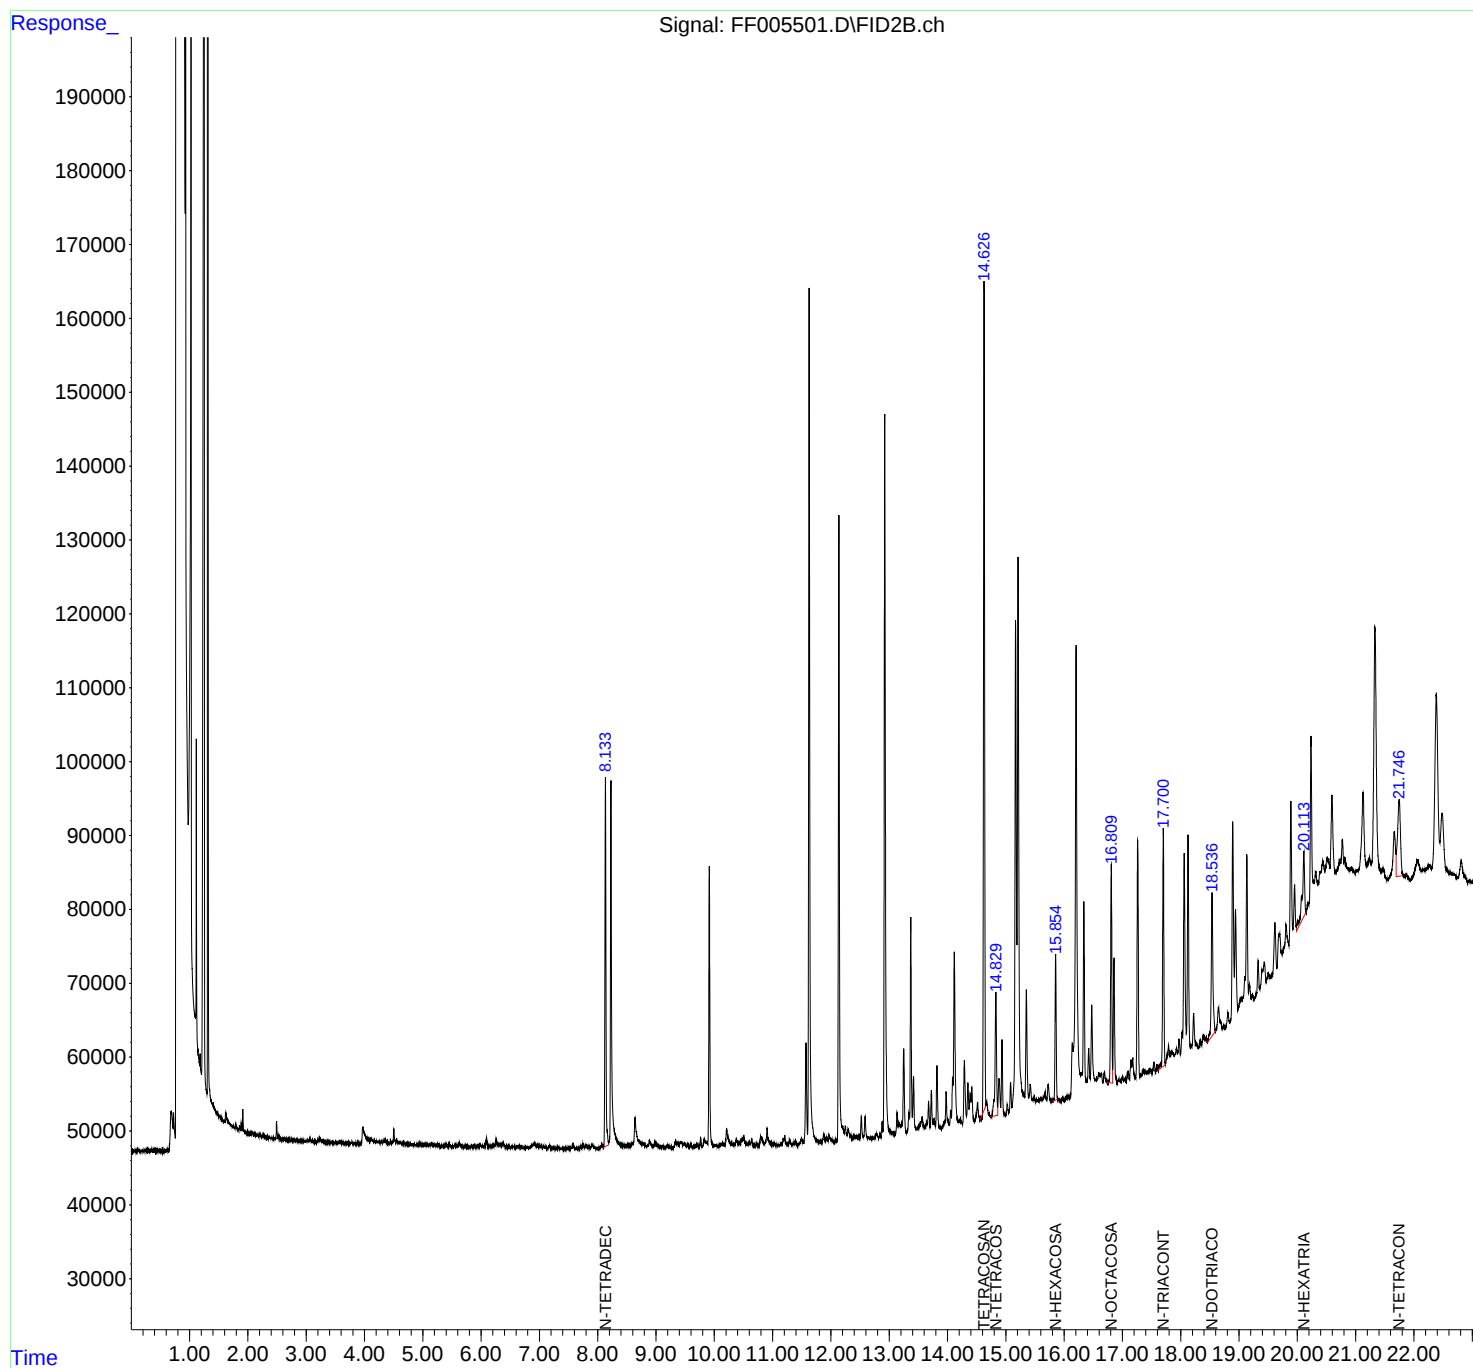


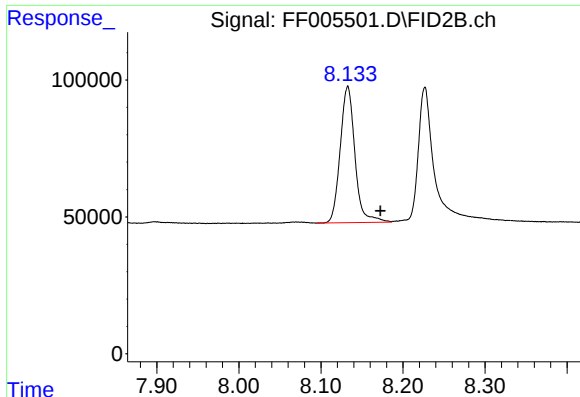

#4 N-TETRADECANE


R.T.: 8.133 min
Delta R.T.: -0.040 min
Response: 620591
Conc: 4.40 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-15-COMP

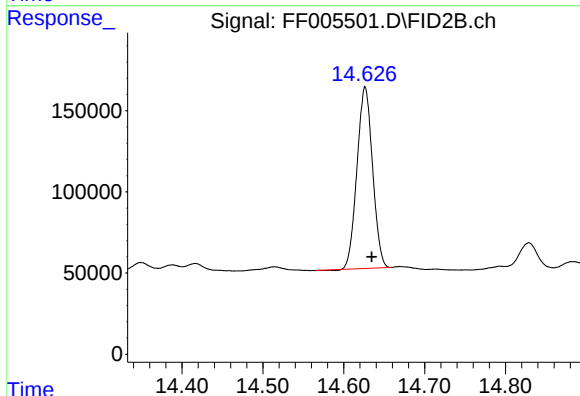


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: -0.008 min
Response: 1495716
Conc: 13.98 ug/ml

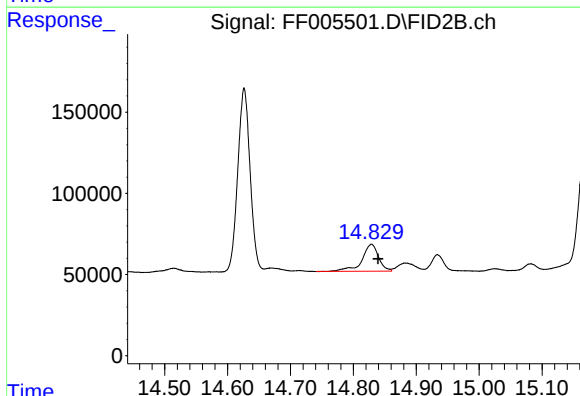


#10 N-TETRACOSANE

R.T.: 14.829 min
Delta R.T.: -0.011 min
Response: 302418
Conc: 2.47 ug/ml

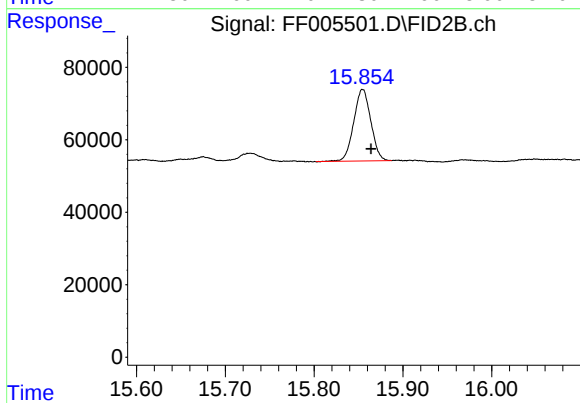

#11 N-HEXACOSANE


R.T.: 15.855 min
Delta R.T.: -0.010 min
Response: 263607
Conc: 2.20 ug/ml

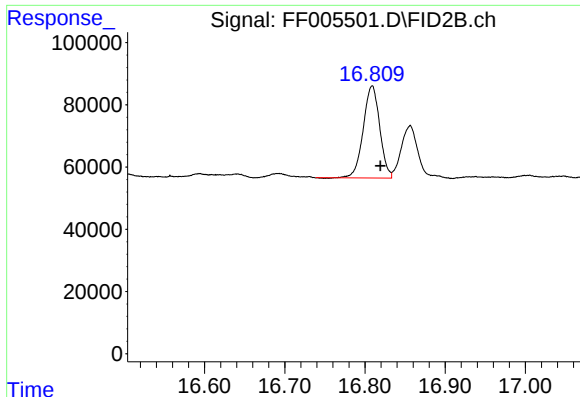

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.010 min
Response: 422183
Conc: 3.54 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-15-COMP

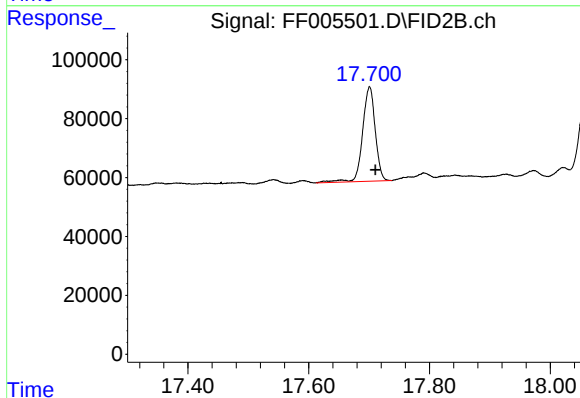


#13 N-TRIACONTANE

R.T.: 17.701 min
Delta R.T.: -0.010 min
Response: 467464
Conc: 3.86 ug/ml

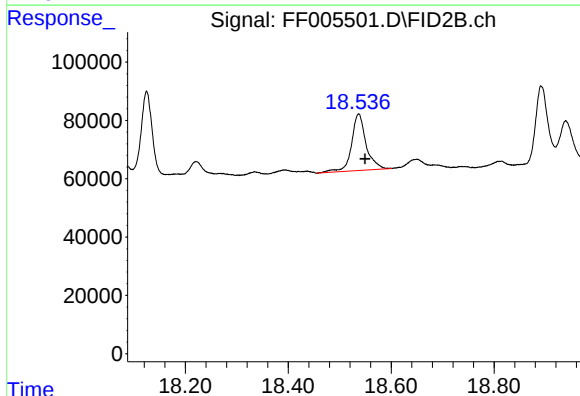


#14 N-DOTRIACONTANE

R.T.: 18.537 min
Delta R.T.: -0.012 min
Response: 379747
Conc: 3.06 ug/ml

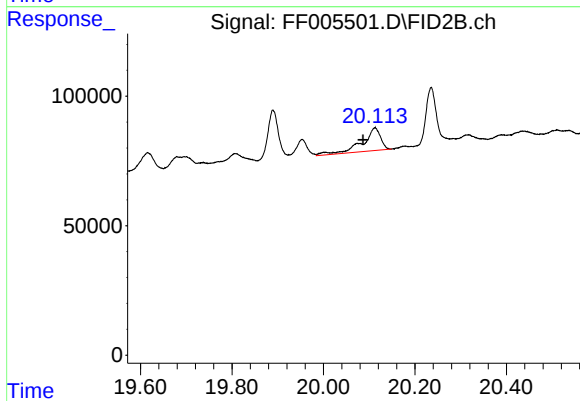

#16 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: 0.026 min
Response: 243547
Conc: 2.03 ug/ml

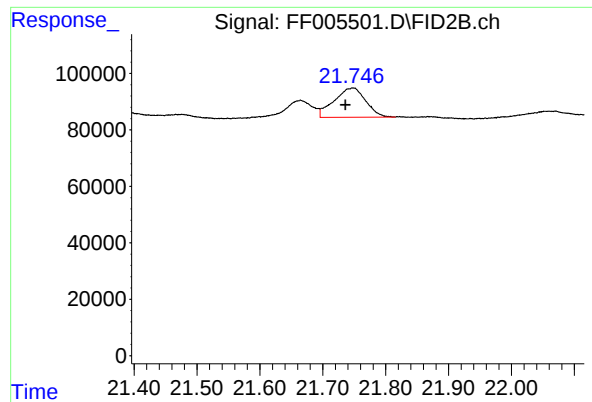

#18 N-TETRACONTANE

R.T.: 21.748 min
Delta R.T.: 0.012 min
Response: 359911
Conc: 2.83 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-15-COMP