

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005478.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 11:01
Operator : DD\AJ
Sample : K4762-05 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TPH-4-STOCK-PILE

Integration File: autoint1.e
Quant Time: Sep 09 16:21:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	1143400	10.685 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005478.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 11:01
Operator : DD\AJ
Sample : K4762-05 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TPH-4-STOCK-PILE

Integration File: autoint1.e
Quant Time: Sep 09 16:21:46 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

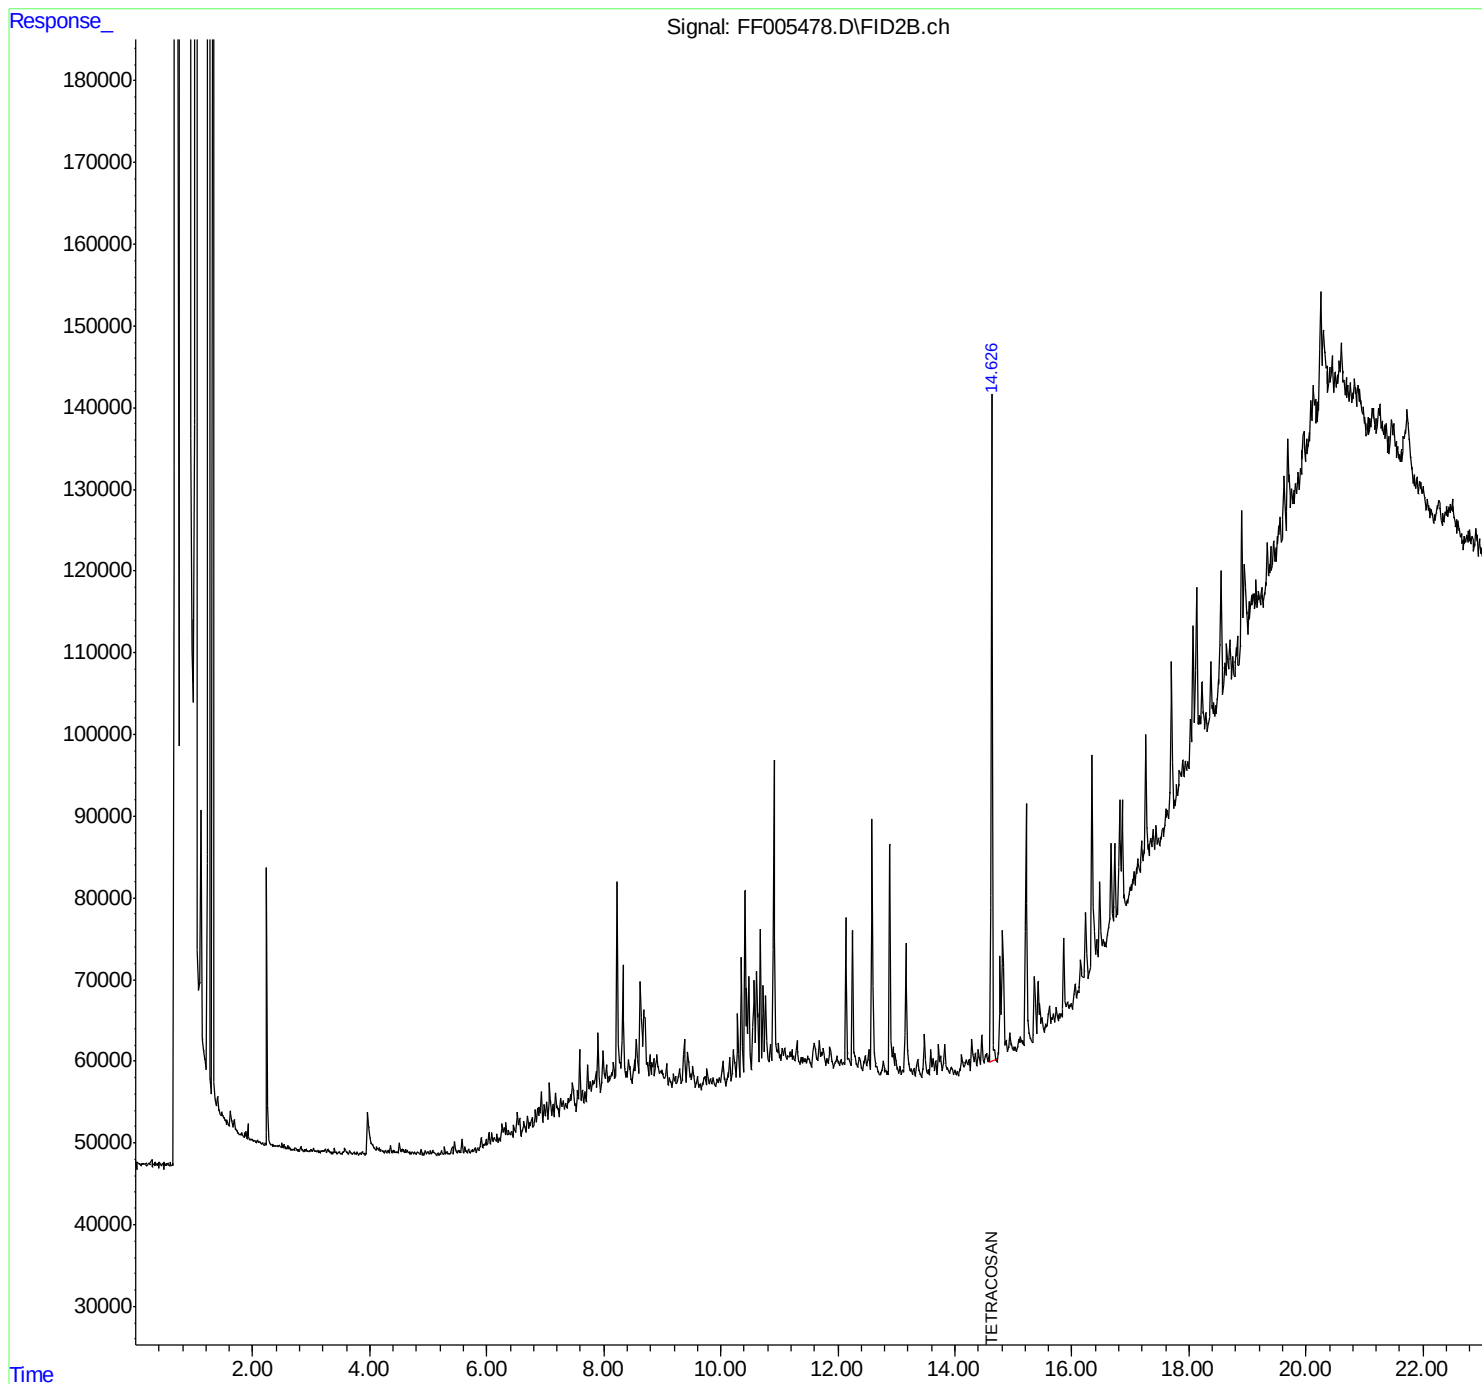

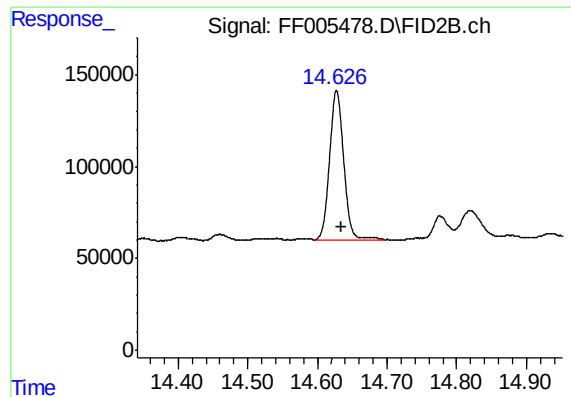

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.627 min
Delta R.T.: -0.007 min
Response: 1143400
Conc: 10.69 ug/ml

Instrument :
FID_F
ClientSampleId :
TPH-4-STOCK-PILE