

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
 Data File : FF005494.D
 Signal(s) : FID2B.ch
 Acq On : 09 Sep 2019 19:05
 Operator : DD\AJ
 Sample : PB122919BS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB122919BS

Integration File: autoint1.e
 Quant Time: Sep 10 04:13:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.627	2048474	19.143 ug/ml
Target Compounds			
2) N-DECANE	4.353	2597999	18.171 ug/ml
3) N-DODECANE	6.373	2580216	18.000 ug/ml
4) N-TETRADECANE	8.166	2534736	17.978 ug/ml
5) N-HEXADECANE	9.767	2522885	18.038 ug/ml
6) N-OCTADECANE	11.210	2462393	18.302 ug/ml
7) N-EICOSANE	12.523	2393143	18.248 ug/ml
8) N-DOCOSANE	13.725	2336636	18.558 ug/ml
10) N-TETRACOSANE	14.832	2354614	19.253 ug/ml
11) N-HEXACOSANE	15.857	2385046	19.924 ug/ml
12) N-OCTACOSANE	16.810	2465605	20.663 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090919\
Data File : FF005494.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2019 19:05
Operator : DD\AJ
Sample : PB122919BS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB122919BS

Integration File: autoint1.e
Quant Time: Sep 10 04:13:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

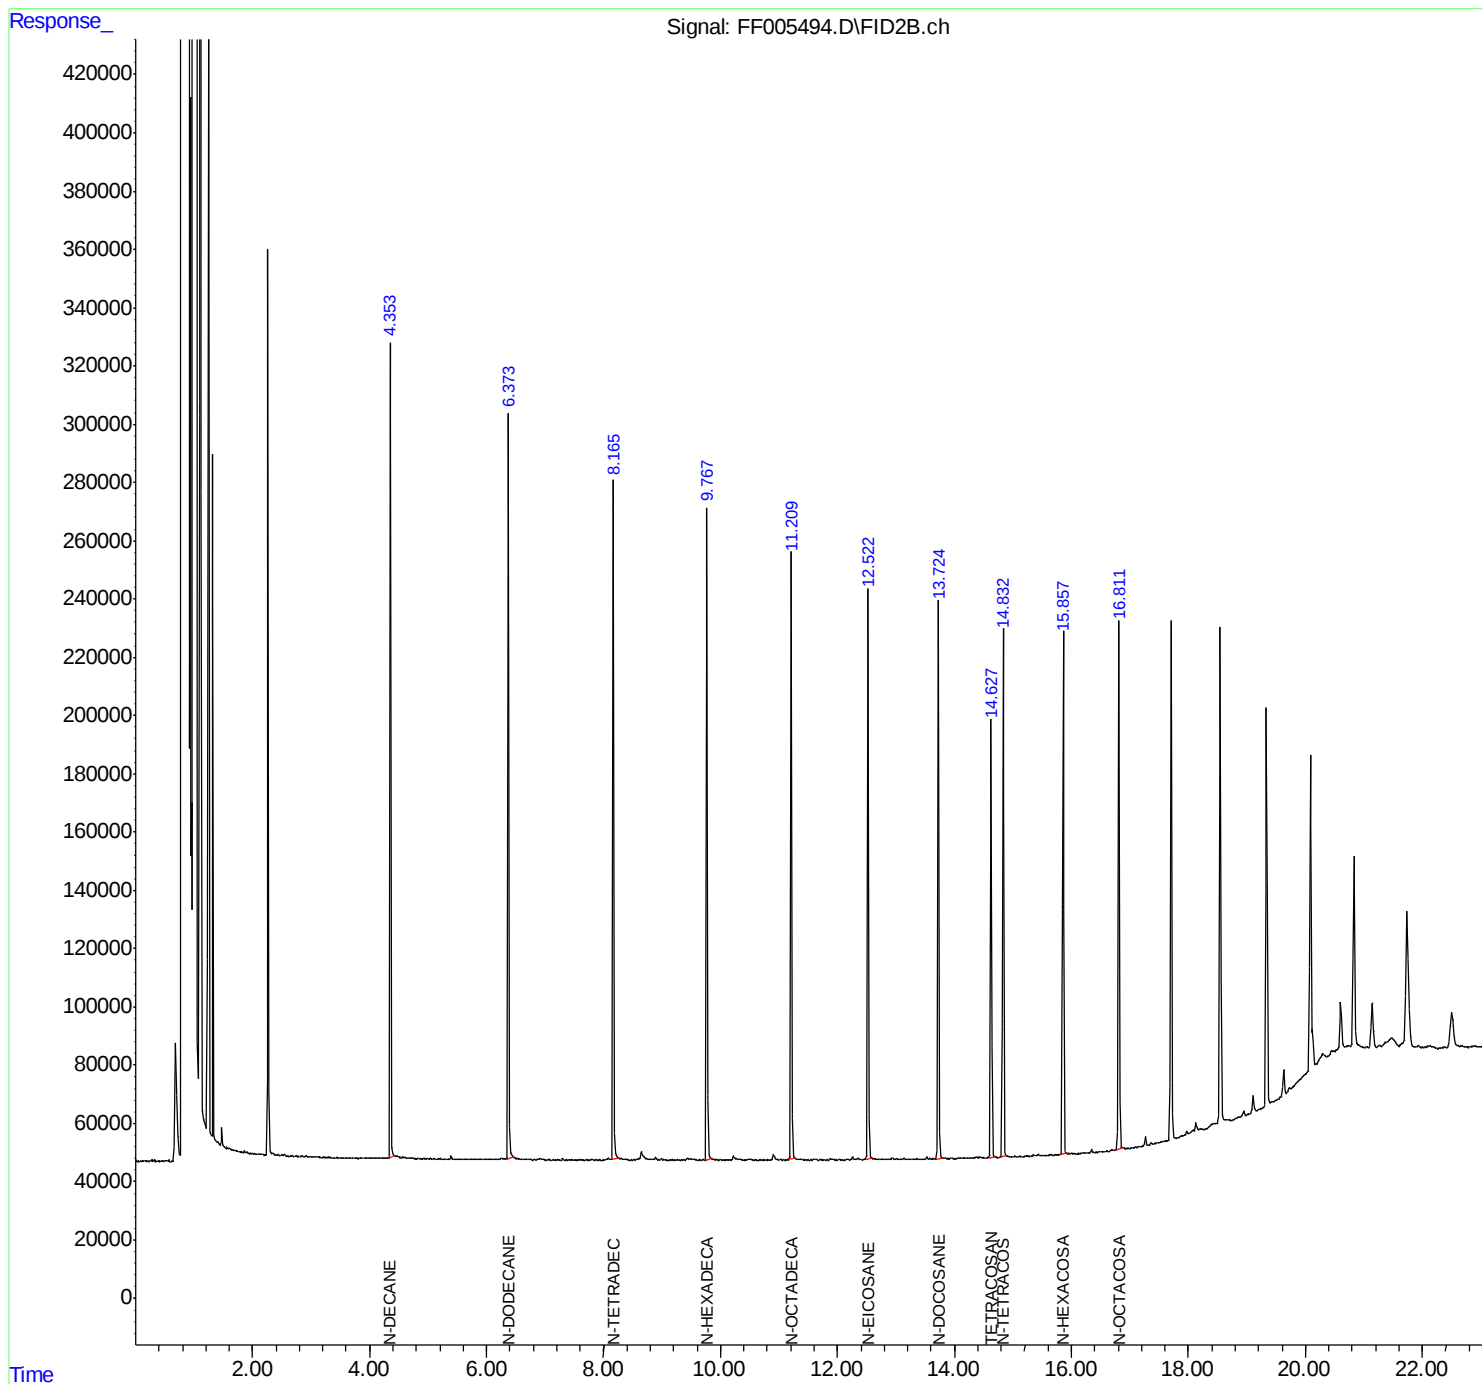


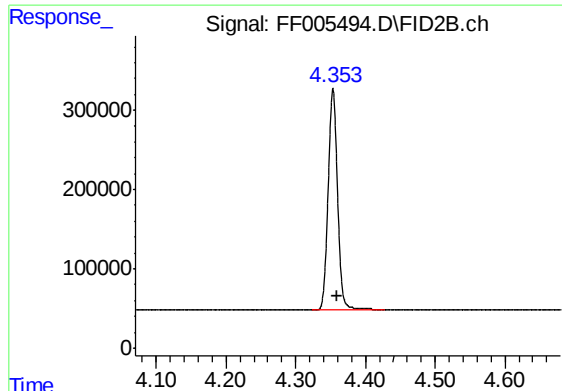

#2 N-DECANE


R.T.: 4.353 min
Delta R.T.: -0.005 min
Response: 2597999
Conc: 18.17 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122919BS

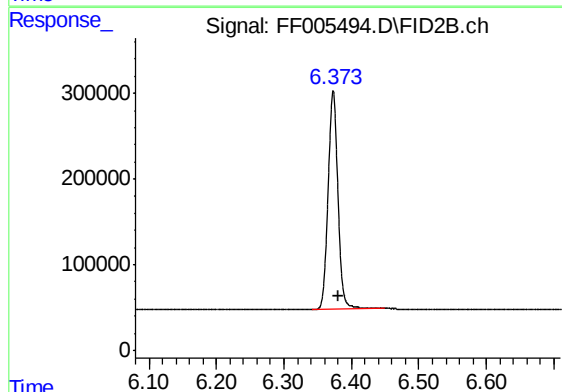


#3 N-DODECANE

R.T.: 6.373 min
Delta R.T.: -0.007 min
Response: 2580216
Conc: 18.00 ug/ml

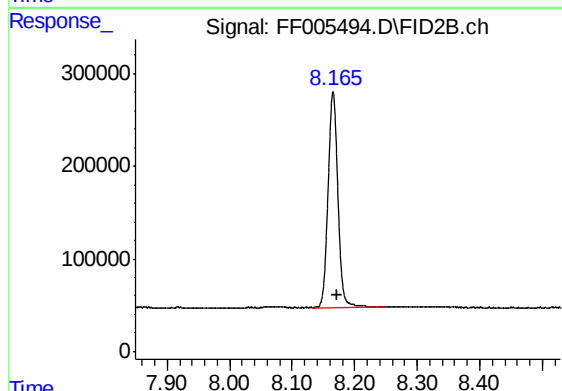


#4 N-TETRADECANE

R.T.: 8.166 min
Delta R.T.: -0.007 min
Response: 2534736
Conc: 17.98 ug/ml

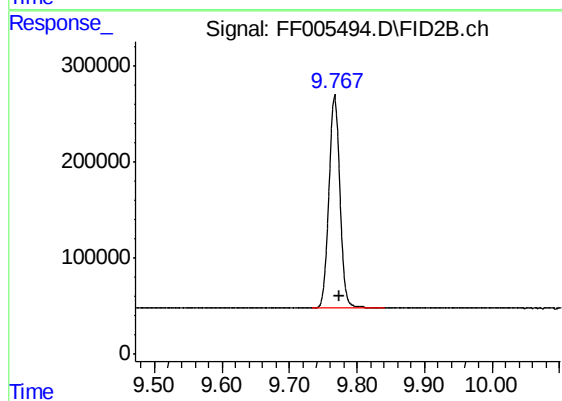

#5 N-HEXADECANE


R.T.: 9.767 min
Delta R.T.: -0.007 min
Response: 2522885
Conc: 18.04 ug/ml

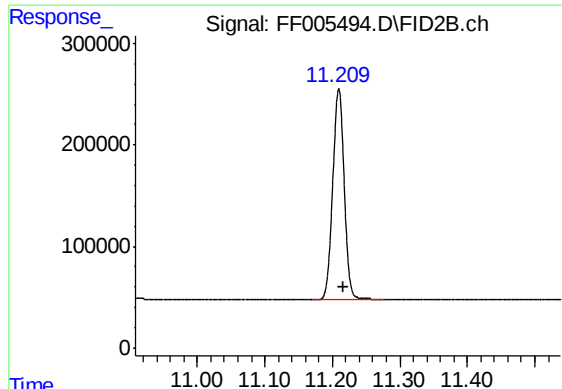

#6 N-OCTADECANE


R.T.: 11.210 min
Delta R.T.: -0.007 min
Response: 2462393
Conc: 18.30 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122919BS

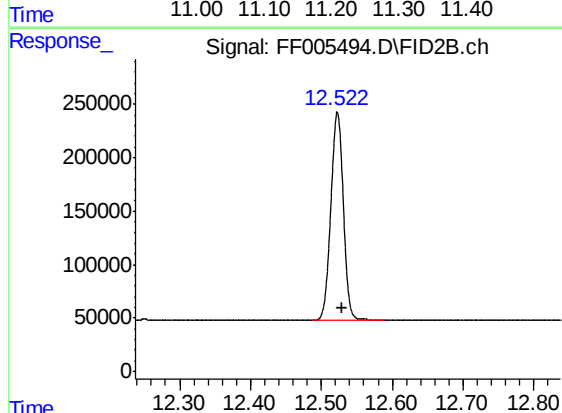


#7 N-EICOSANE

R.T.: 12.523 min
Delta R.T.: -0.007 min
Response: 2393143
Conc: 18.25 ug/ml

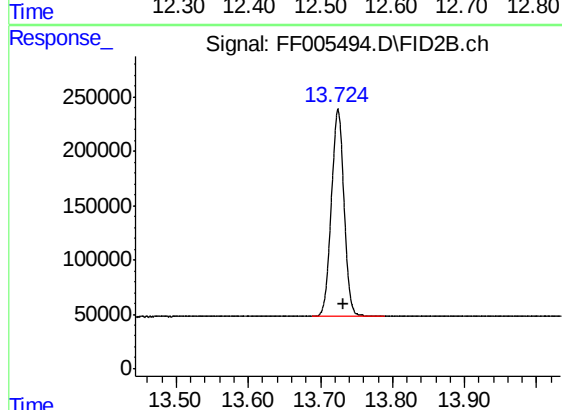


#8 N-DOCOSANE

R.T.: 13.725 min
Delta R.T.: -0.007 min
Response: 2336636
Conc: 18.56 ug/ml

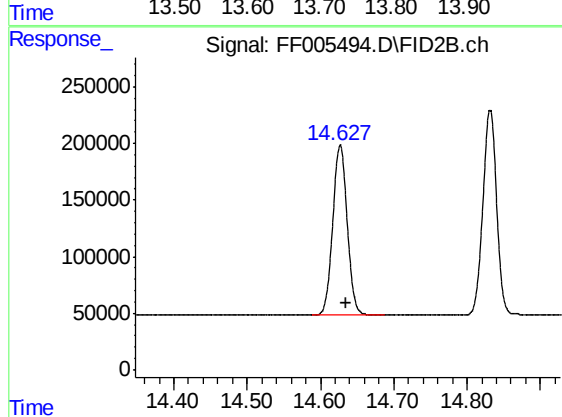

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.627 min
Delta R.T.: -0.007 min
Response: 2048474
Conc: 19.14 ug/ml

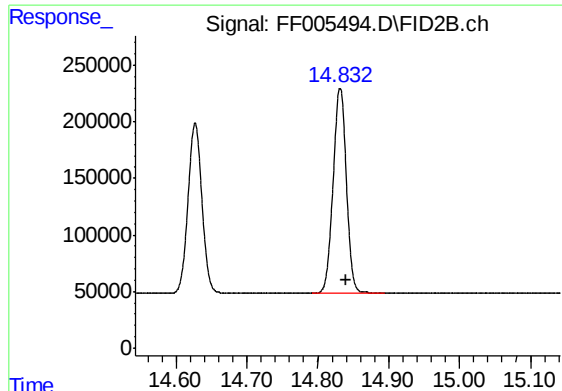

#10 N-TETRACOSANE


R.T.: 14.832 min
Delta R.T.: -0.008 min
Response: 2354614
Conc: 19.25 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122919BS

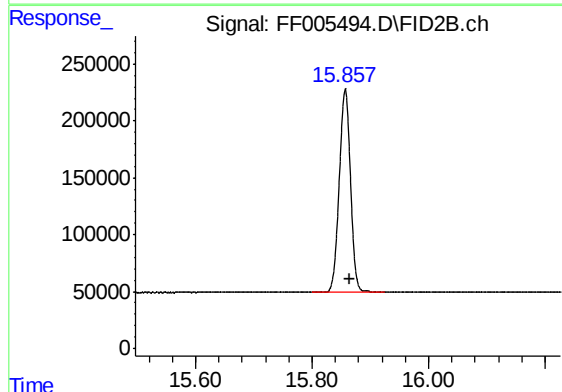

#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.007 min
Response: 2385046
Conc: 19.92 ug/ml

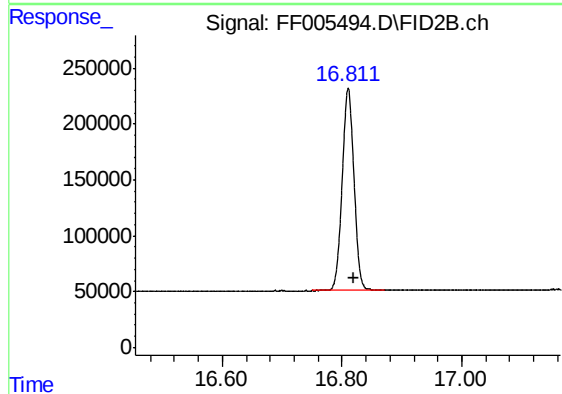

#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: -0.009 min
Response: 2465605
Conc: 20.66 ug/ml