

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090922\
Data File : FF011430.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2022 13:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 07:23:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.503	1641043	12.532 ug/ml
12)	N-OCTACOSANE	16.950	1597785	13.044 ug/ml
13)	N-TRIACONTANE	17.834	287468	2.383 ug/ml
14)	N-DOTRIACONTANE	18.666	408271	3.451 ug/ml
15)	N-TETRATRIACONTANE	19.446	357119	3.128 ug/ml
16)	N-HEXATRIACONTANE	20.185	239838	2.253 ug/ml
17)	N-OCTATRIACONTANE	20.887	158216	1.521 ug/ml
18)	N-TETRACONTANE	21.700	88398	0.838 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090922\
Data File : FF011430.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2022 13:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 07:23:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

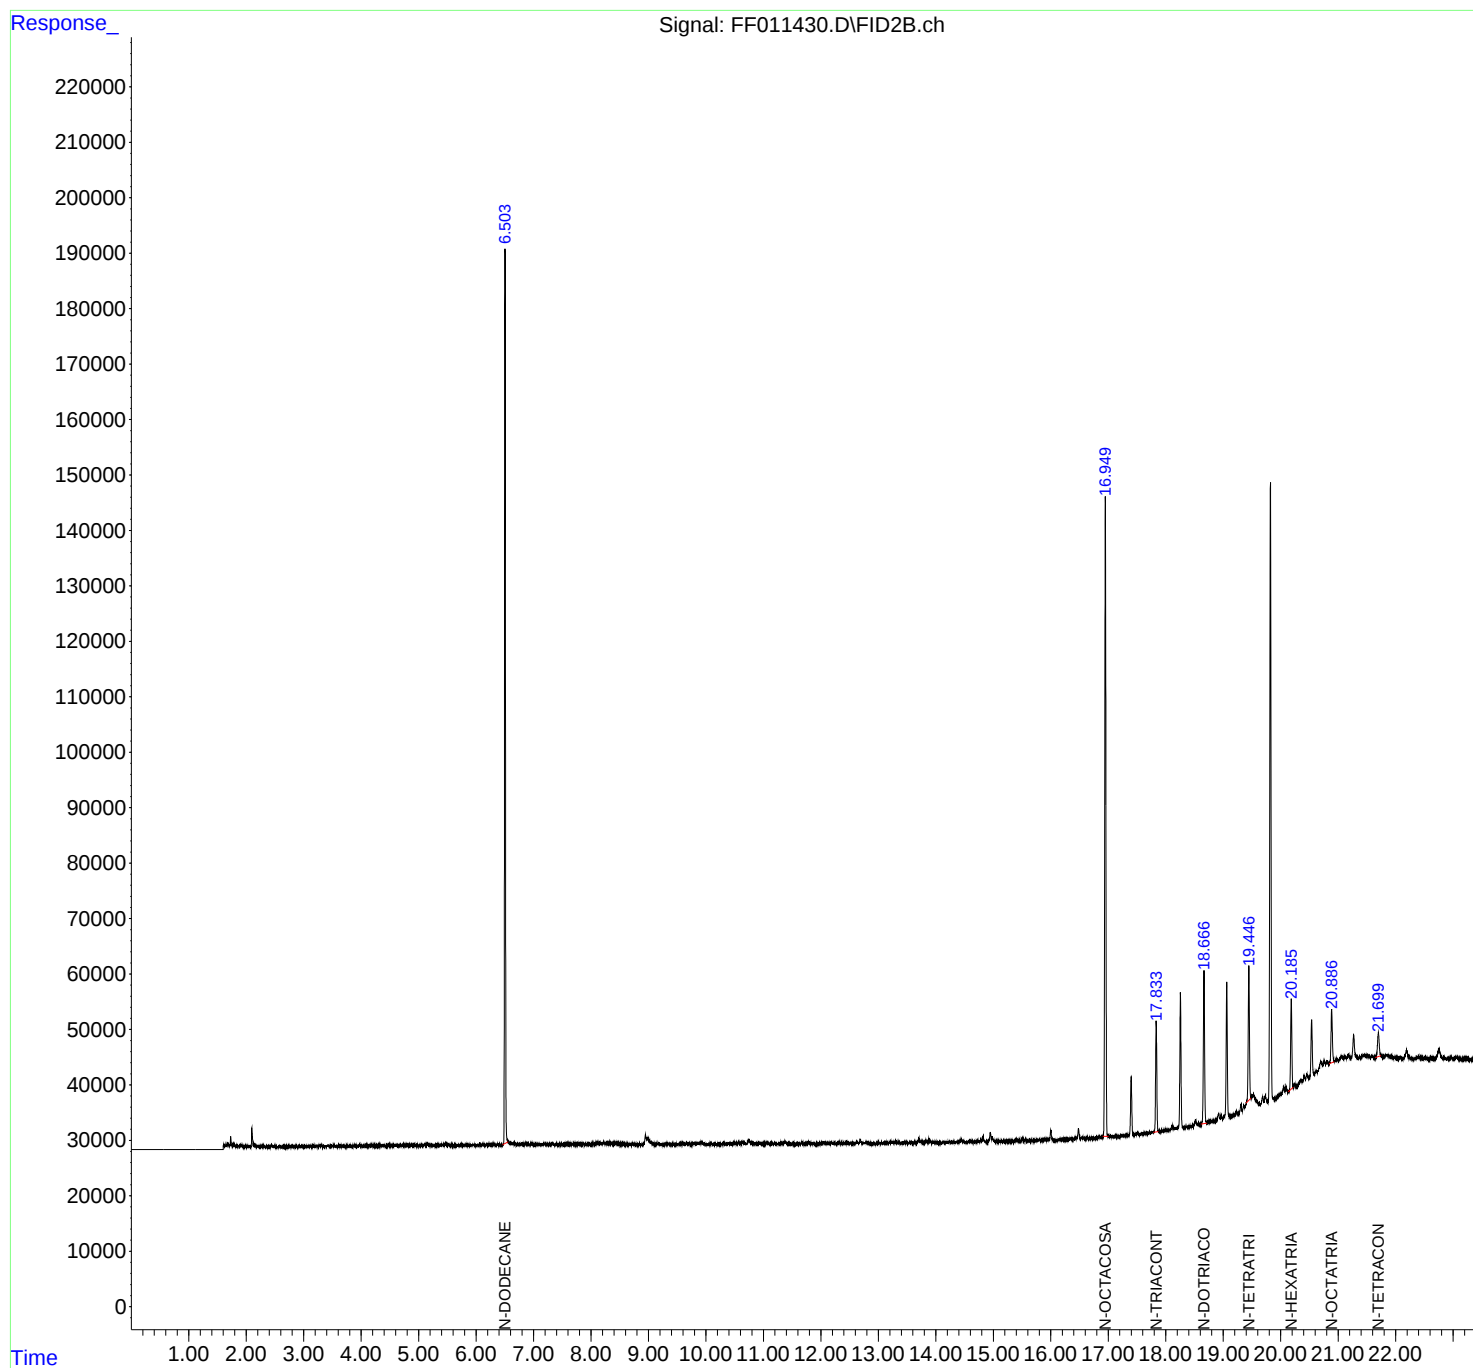


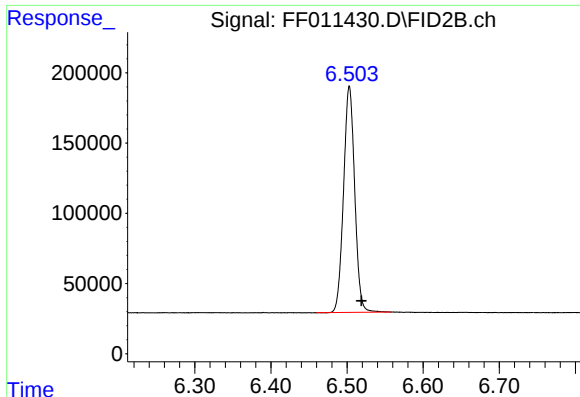

#3 N-DODECANE


R.T.: 6.503 min
Delta R.T.: -0.016 min
Response: 1641043
Conc: 12.53 ug/ml

Instrument :
FID_F
ClientSampleId :

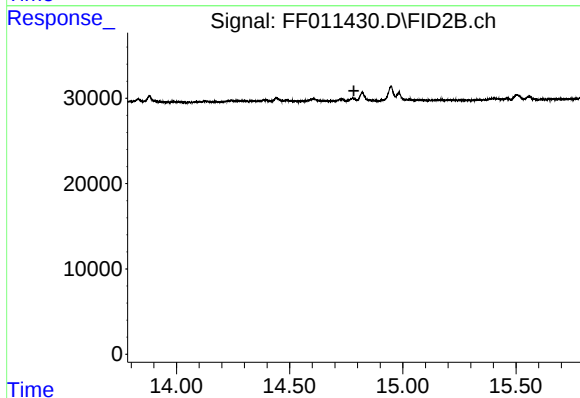


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.784 min
Response: 0
Conc: N.D.

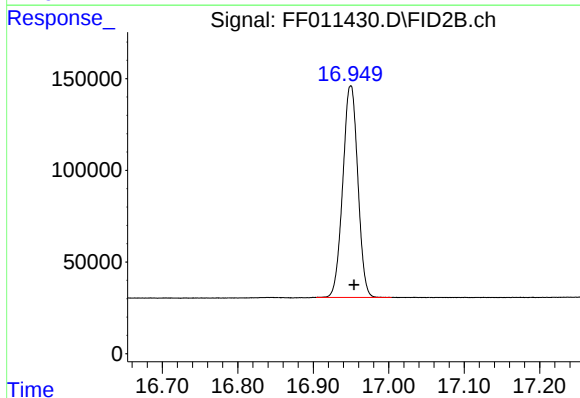


#12 N-OCTACOSANE

R.T.: 16.950 min
Delta R.T.: -0.004 min
Response: 1597785
Conc: 13.04 ug/ml

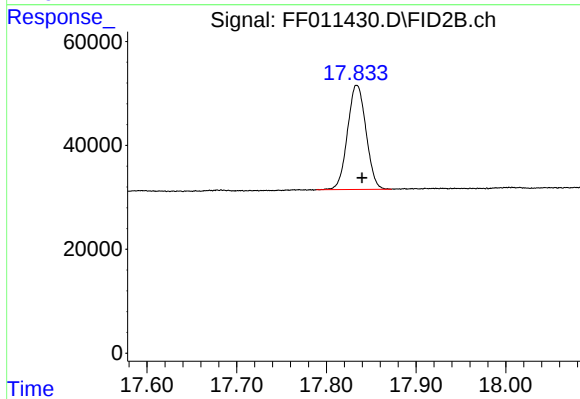

#13 N-TRIACONTANE


R.T.: 17.834 min
Delta R.T.: -0.006 min
Response: 287468
Conc: 2.38 ug/ml

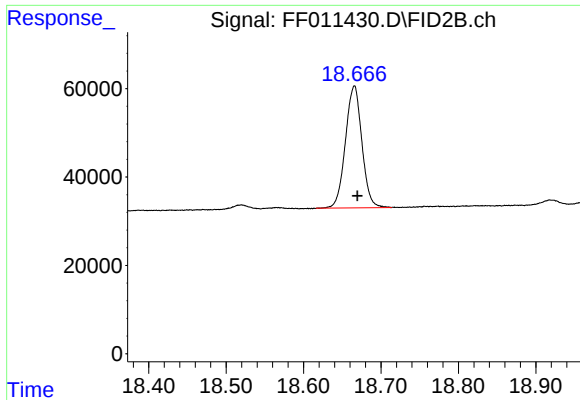

#14 N-DOTRIACONTANE


R.T.: 18.666 min
Delta R.T.: -0.004 min
Response: 408271
Conc: 3.45 ug/ml

Instrument :
FID_F
ClientSampleId :

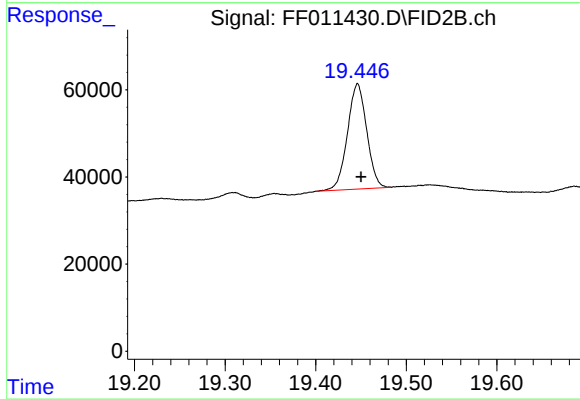


#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: -0.004 min
Response: 357119
Conc: 3.13 ug/ml

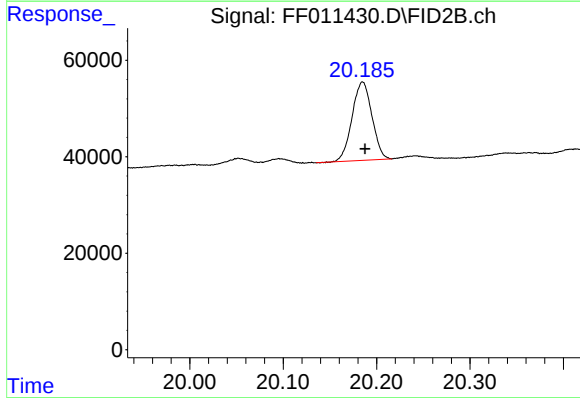


#16 N-HEXATRIACONTANE

R.T.: 20.185 min
Delta R.T.: -0.002 min
Response: 239838
Conc: 2.25 ug/ml

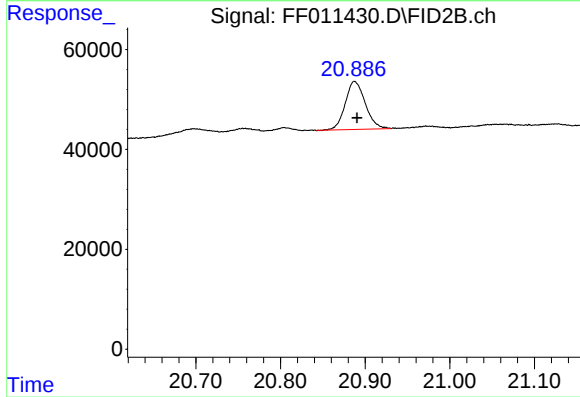

#17 N-OCTATRIACONTANE

R.T.: 20.887 min
Delta R.T.: -0.003 min
Response: 158216
Conc: 1.52 ug/ml

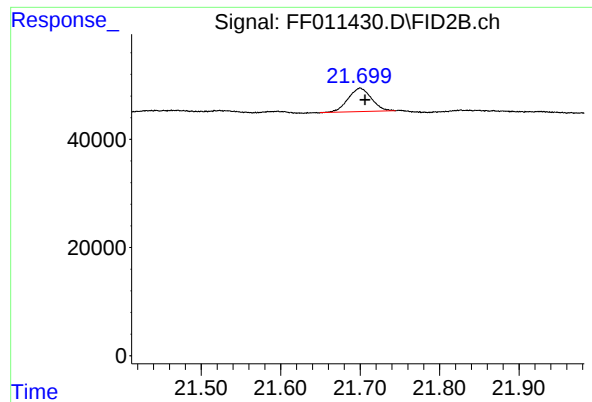

#18 N-TETRACONTANE

R.T.: 21.700 min
Delta R.T.: -0.006 min
Response: 88398
Conc: 0.84 ug/ml

Instrument :

FID_F

ClientSampleId :