

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090922\
Data File : FF011431.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2022 14:01
Operator : YP\AJ
Sample : N4538-07 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MBD-SB-1-2-0-5

Integration File: autoint1.e
Quant Time: Sep 11 07:23:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	157829	1.408 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF090922\
Data File : FF011431.D
Signal(s) : FID2B.ch
Acq On : 09 Sep 2022 14:01
Operator : YP\AJ
Sample : N4538-07 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MBD-SB-1-2-0-5

Integration File: autoint1.e
Quant Time: Sep 11 07:23:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF082722.M
Quant Title :
QLast Update : Mon Aug 29 01:24:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

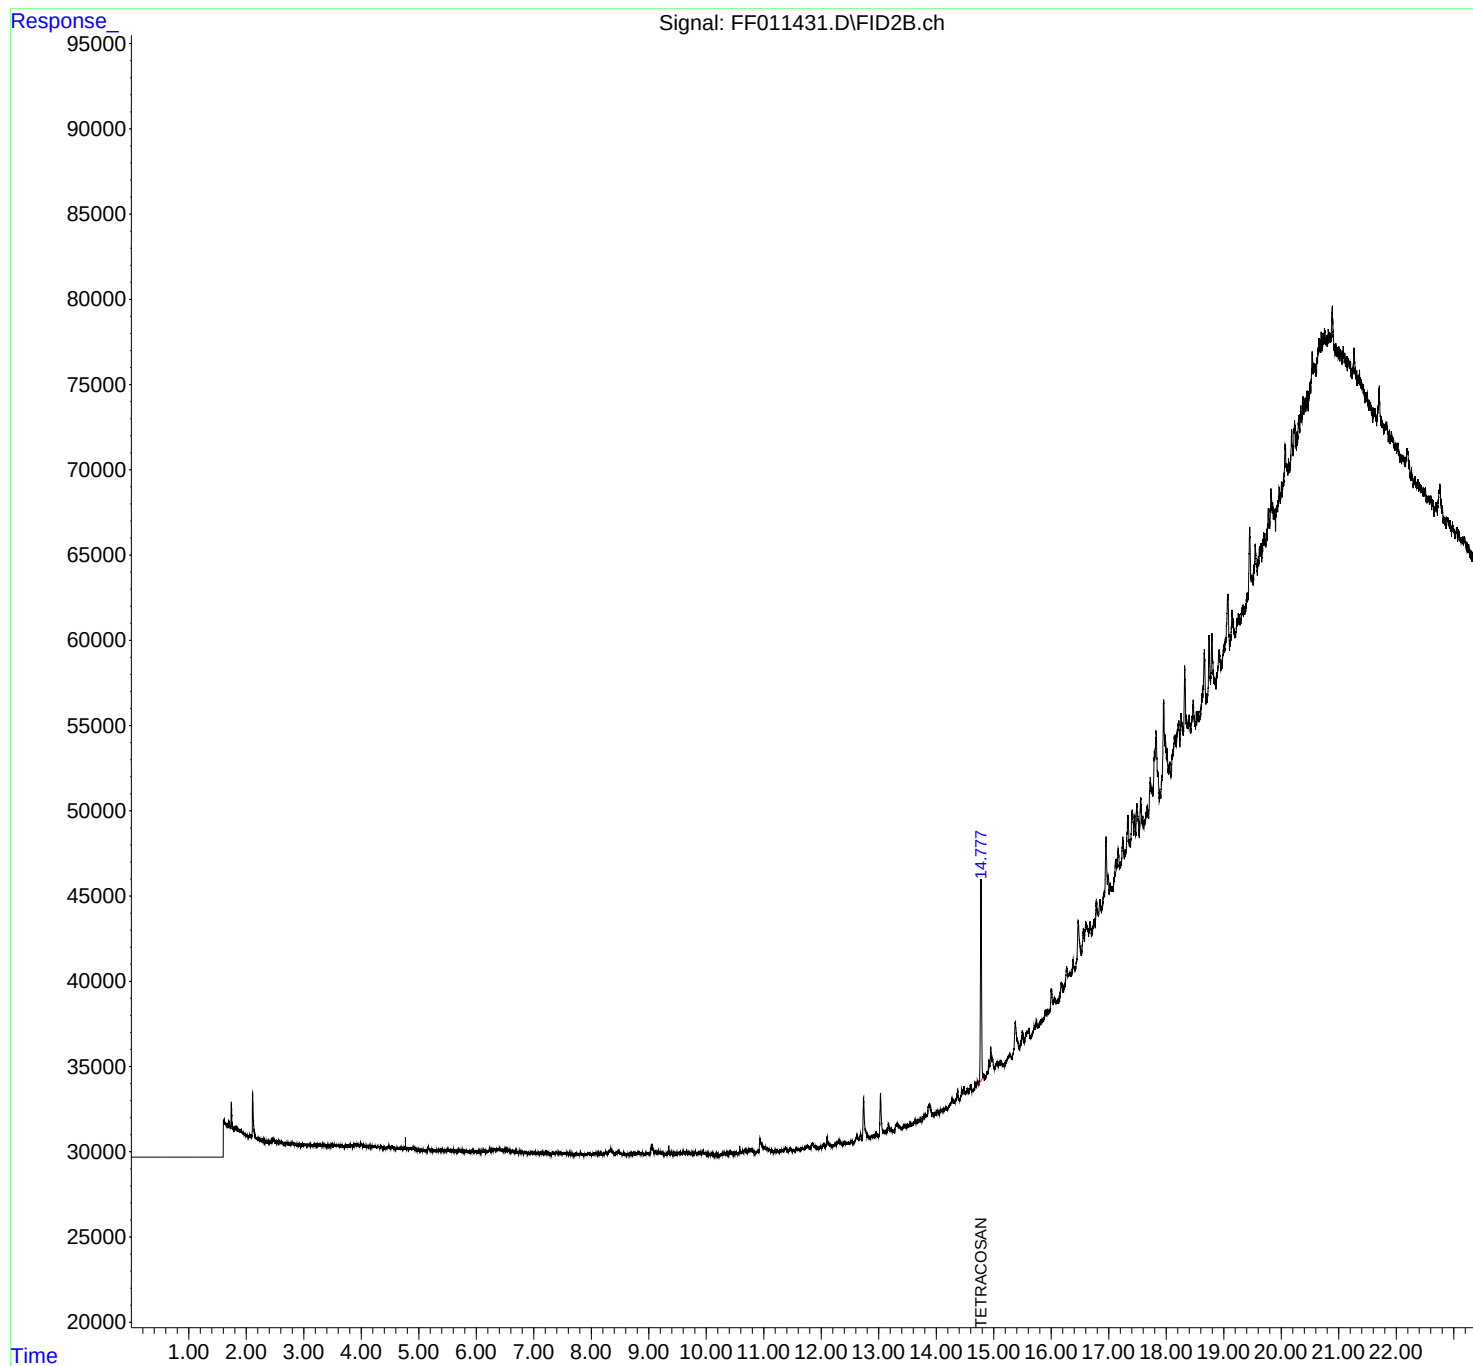

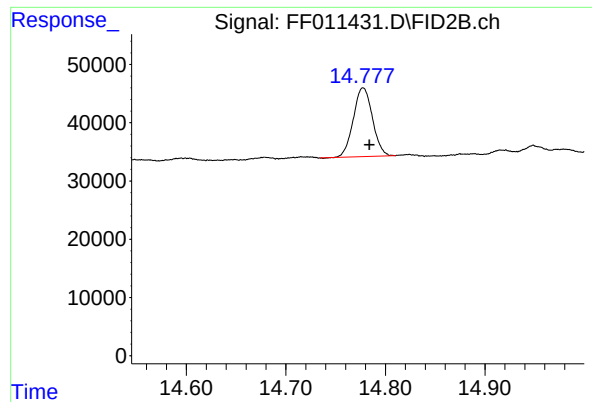

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.006 min
Response: 157829
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :
MBD-SB-1-2-0-5