

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091018\
Data File : FF002087.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2018 23:08
Operator : AJ\SJ
Sample : J4825-13 2X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 11 02:33:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.275	1011423	8.070 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.473	623955	4.397 ug/ml
11)	N-HEXACOSANE	15.494	165368	1.163 ug/ml
12)	N-OCTACOSANE	16.438	432691	3.016 ug/ml
13)	N-TRIACONTANE	17.325	349306	2.409 ug/ml
14)	N-DOTRIACONTANE	18.156	441041	3.128 ug/ml
15)	N-TETRATRIACONTANE	18.938	243168	1.808 ug/ml
16)	N-HEXATRIACONTANE	19.676	344813	2.769 ug/ml
17)	N-OCTATRIACONTANE	20.374	544000	4.968 ug/ml
18)	N-TETRACONTANE	21.179	256801	2.426 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091018\
Data File : FF002087.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2018 23:08
Operator : AJ\SJ
Sample : J4825-13 2X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 11 02:33:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083018.M
Quant Title :
QLast Update : Thu Aug 30 14:20:53 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

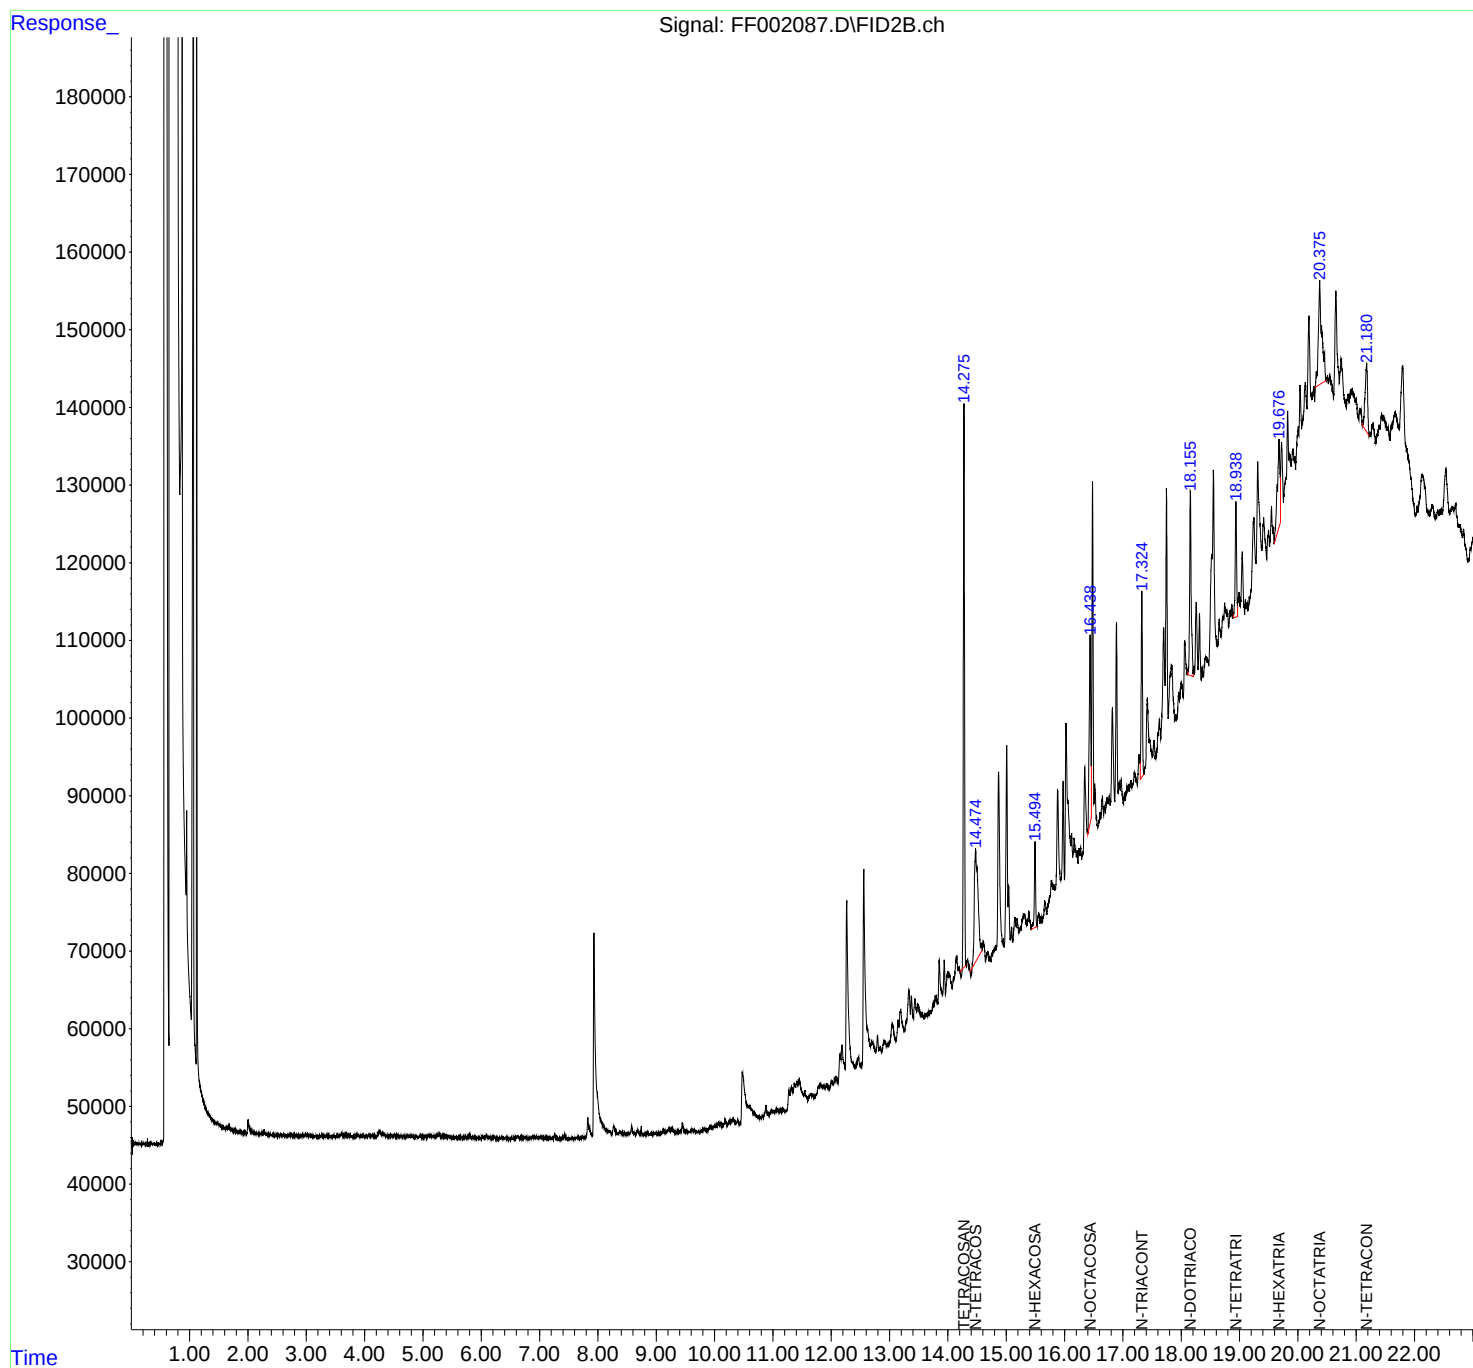

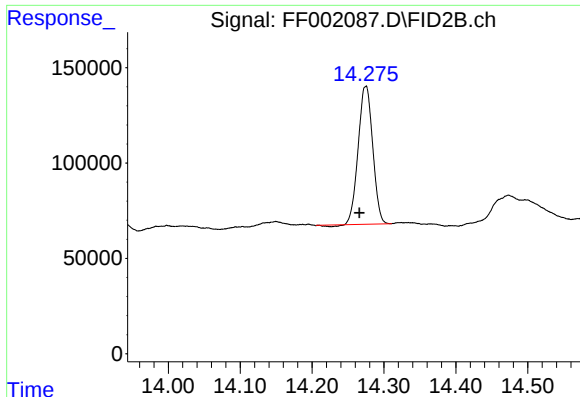


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.275 min
Delta R.T.: 0.009 min
Response: 1011423
Conc: 8.07 ug/ml

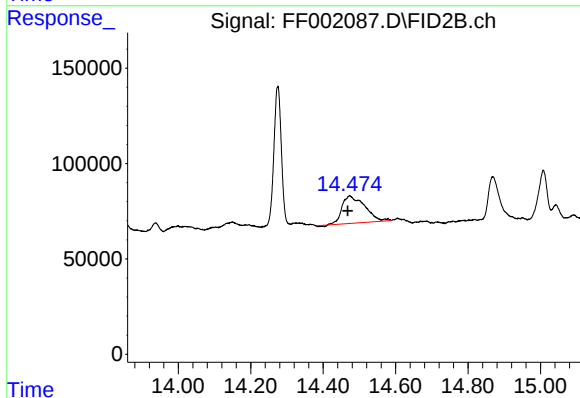


#10 N-TETRACOSANE

R.T.: 14.473 min
Delta R.T.: 0.005 min
Response: 623955
Conc: 4.40 ug/ml

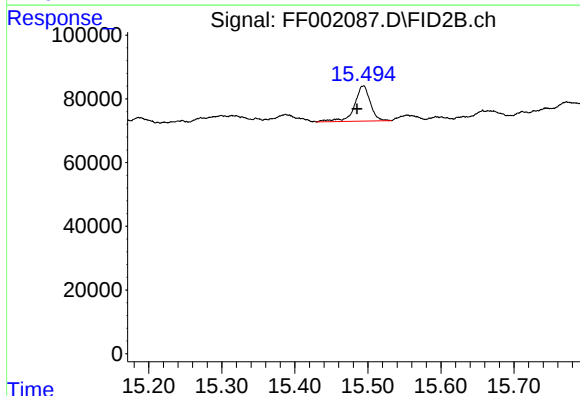


#11 N-HEXACOSANE

R.T.: 15.494 min
Delta R.T.: 0.009 min
Response: 165368
Conc: 1.16 ug/ml

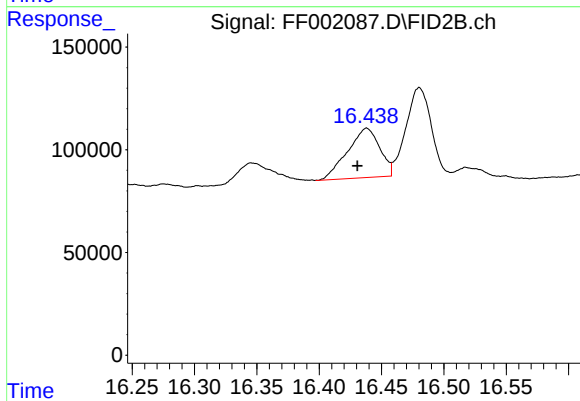


#12 N-OCTACOSANE

R.T.: 16.438 min
Delta R.T.: 0.007 min
Response: 432691
Conc: 3.02 ug/ml

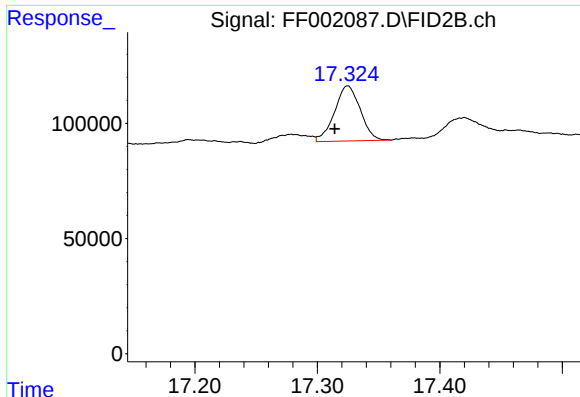


#13 N-TRIACONTANE

R.T.: 17.325 min
Delta R.T.: 0.011 min
Response: 349306
Conc: 2.41 ug/ml

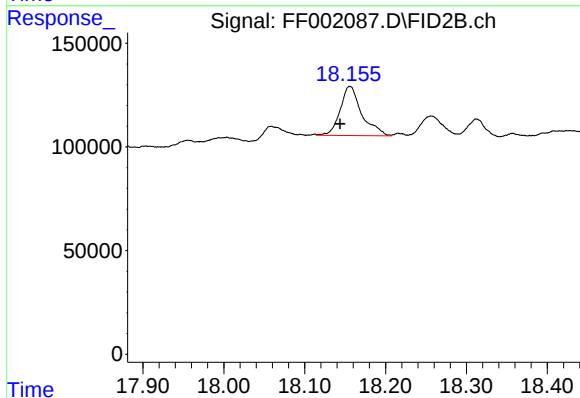


#14 N-DOTRIACONTANE

R.T.: 18.156 min
Delta R.T.: 0.012 min
Response: 441041
Conc: 3.13 ug/ml

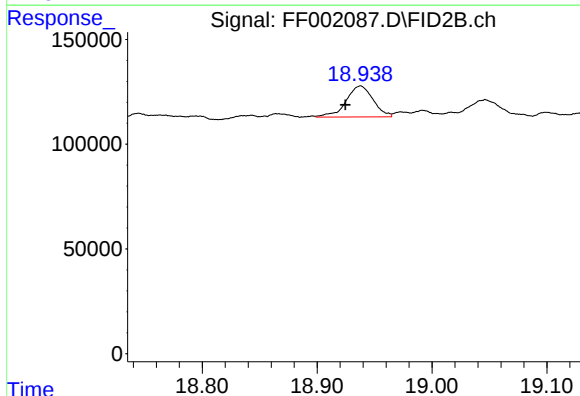


#15 N-TETRATRIACONTANE

R.T.: 18.938 min
Delta R.T.: 0.013 min
Response: 243168
Conc: 1.81 ug/ml

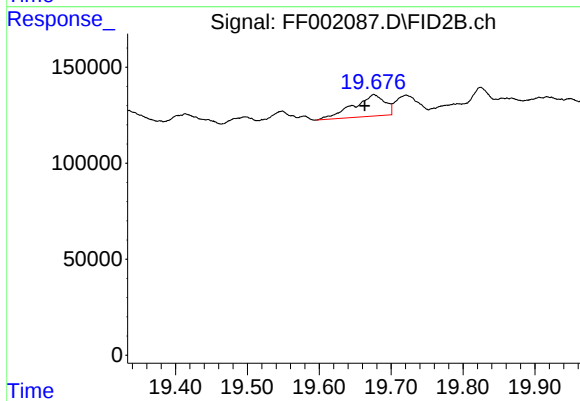


#16 N-HEXATRIACONTANE

R.T.: 19.676 min
Delta R.T.: 0.013 min
Response: 344813
Conc: 2.77 ug/ml

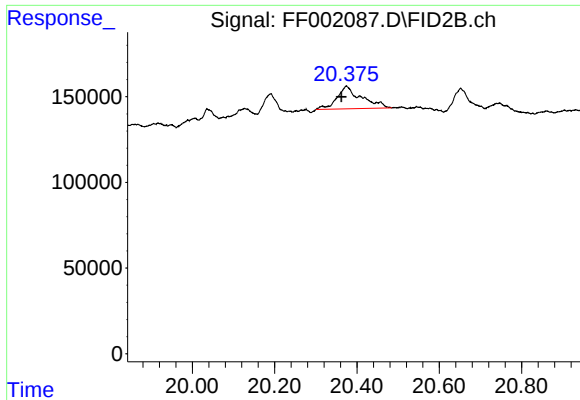

#17 N-OCTATRIACONTANE

R.T.: 20.374 min
Delta R.T.: 0.012 min
Response: 544000
Conc: 4.97 ug/ml

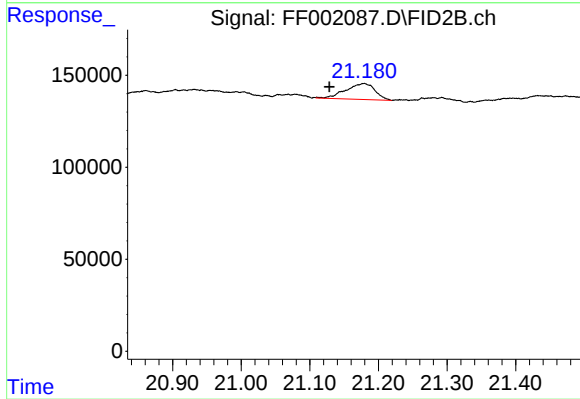

#18 N-TETRACONTANE

R.T.: 21.179 min
Delta R.T.: 0.050 min
Response: 256801
Conc: 2.43 ug/ml