

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
 Data File : FF005511.D
 Signal(s) : FID2B.ch
 Acq On : 10 Sep 2019 11:06
 Operator : DD\AJ
 Sample : PB122920BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB122920BL

Integration File: autoint1.e
 Quant Time: Sep 11 01:46:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	2363553	22.087 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.702	133769	1.106 ug/ml
14) N-DOTRIACONTANE	18.542	185303	1.495 ug/ml
15) N-TETRATRIACONTANE	19.333	117566	0.976 ug/ml
16) N-HEXATRIACONTANE	20.082	104224	0.868 ug/ml
18) N-TETRACONTANE	21.757	512136	4.028 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005511.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 11:06
Operator : DD\AJ
Sample : PB122920BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB122920BL

Integration File: autoint1.e
Quant Time: Sep 11 01:46:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

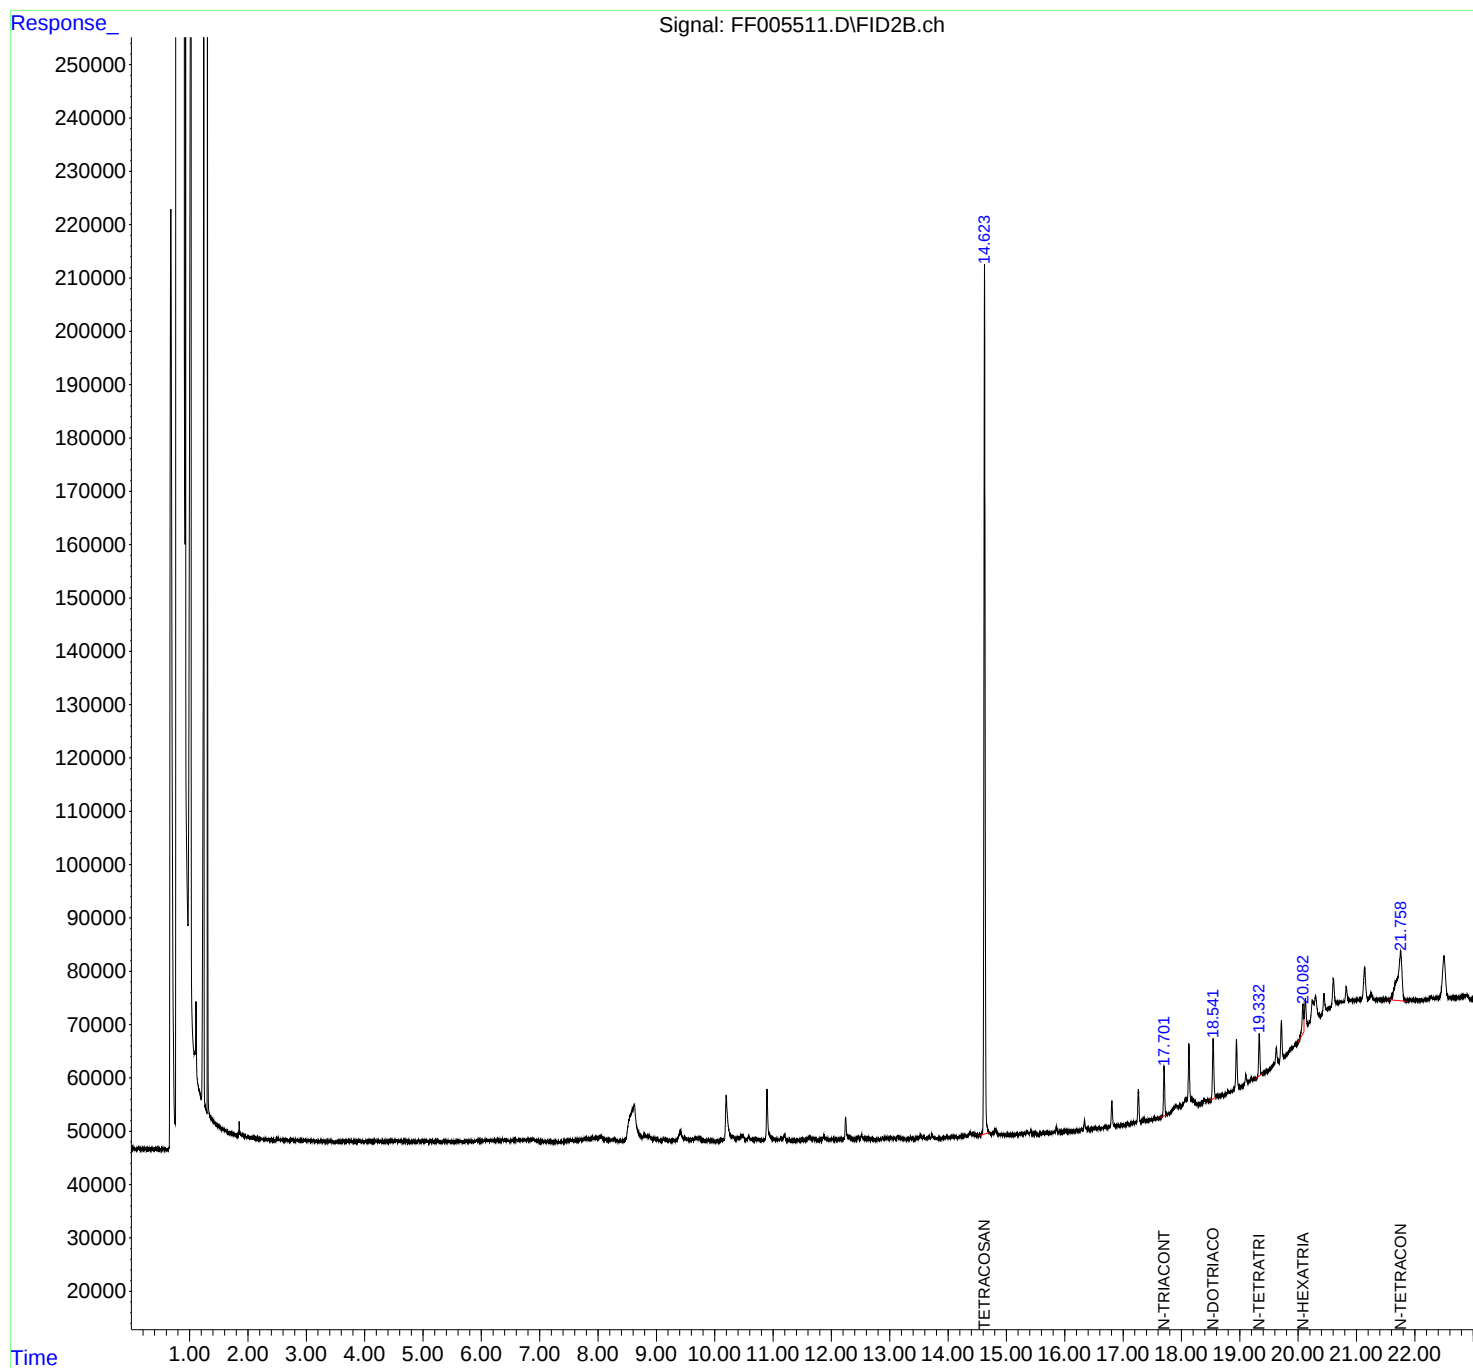


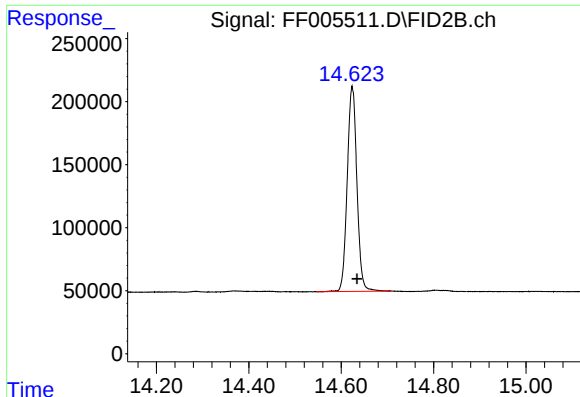

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.624 min
Delta R.T.: -0.011 min
Response: 2363553
Conc: 22.09 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122920BL

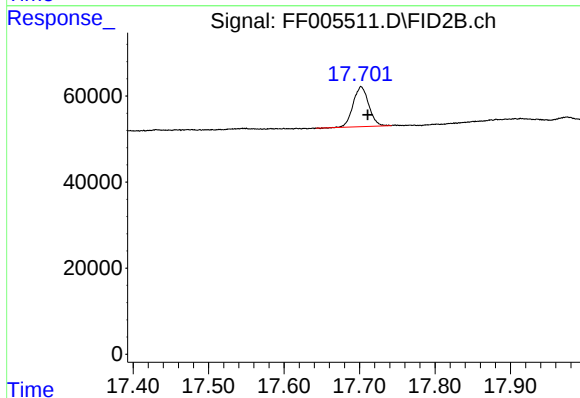


#13 N-TRIACONTANE

R.T.: 17.702 min
Delta R.T.: -0.008 min
Response: 133769
Conc: 1.11 ug/ml

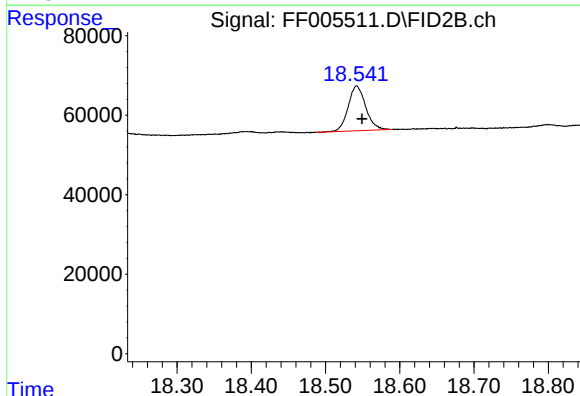


#14 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: -0.007 min
Response: 185303
Conc: 1.49 ug/ml

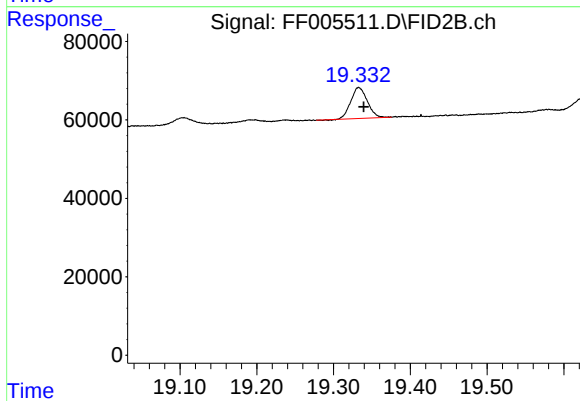

#15 N-TETRATRIACONTANE


R.T.: 19.333 min
Delta R.T.: -0.007 min
Response: 117566
Conc: 0.98 ug/ml

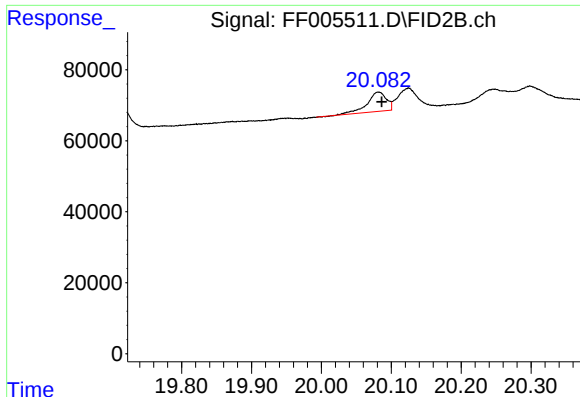

#16 N-HEXATRIACONTANE

R.T.: 20.082 min
Delta R.T.: -0.005 min
Response: 104224
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122920BL

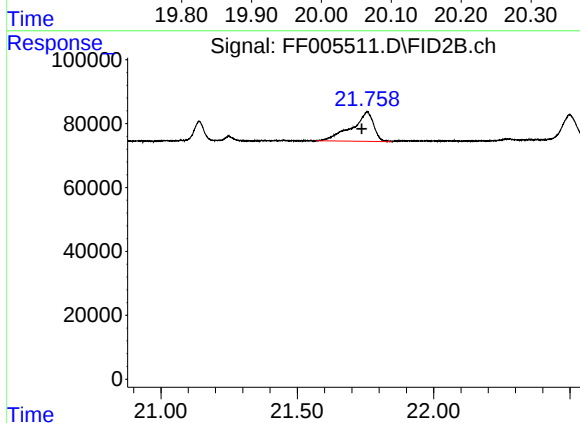

#18 N-TETRACONTANE

R.T.: 21.757 min
Delta R.T.: 0.021 min
Response: 512136
Conc: 4.03 ug/ml