

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005521.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 17:59
Operator : DD\AJ
Sample : K4764-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 01:50:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.623	1691740	15.809 ug/ml
Target Compounds			
4) N-TETRADECANE	8.225f	343594	2.437 ug/ml
12) N-OCTACOSANE	16.805	130826	1.096 ug/ml
13) N-TRIACONTANE	17.698	172810	1.429 ug/ml
14) N-DOTRIACONTANE	18.534	155080	1.251 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005521.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 17:59
Operator : DD\AJ
Sample : K4764-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 01:50:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

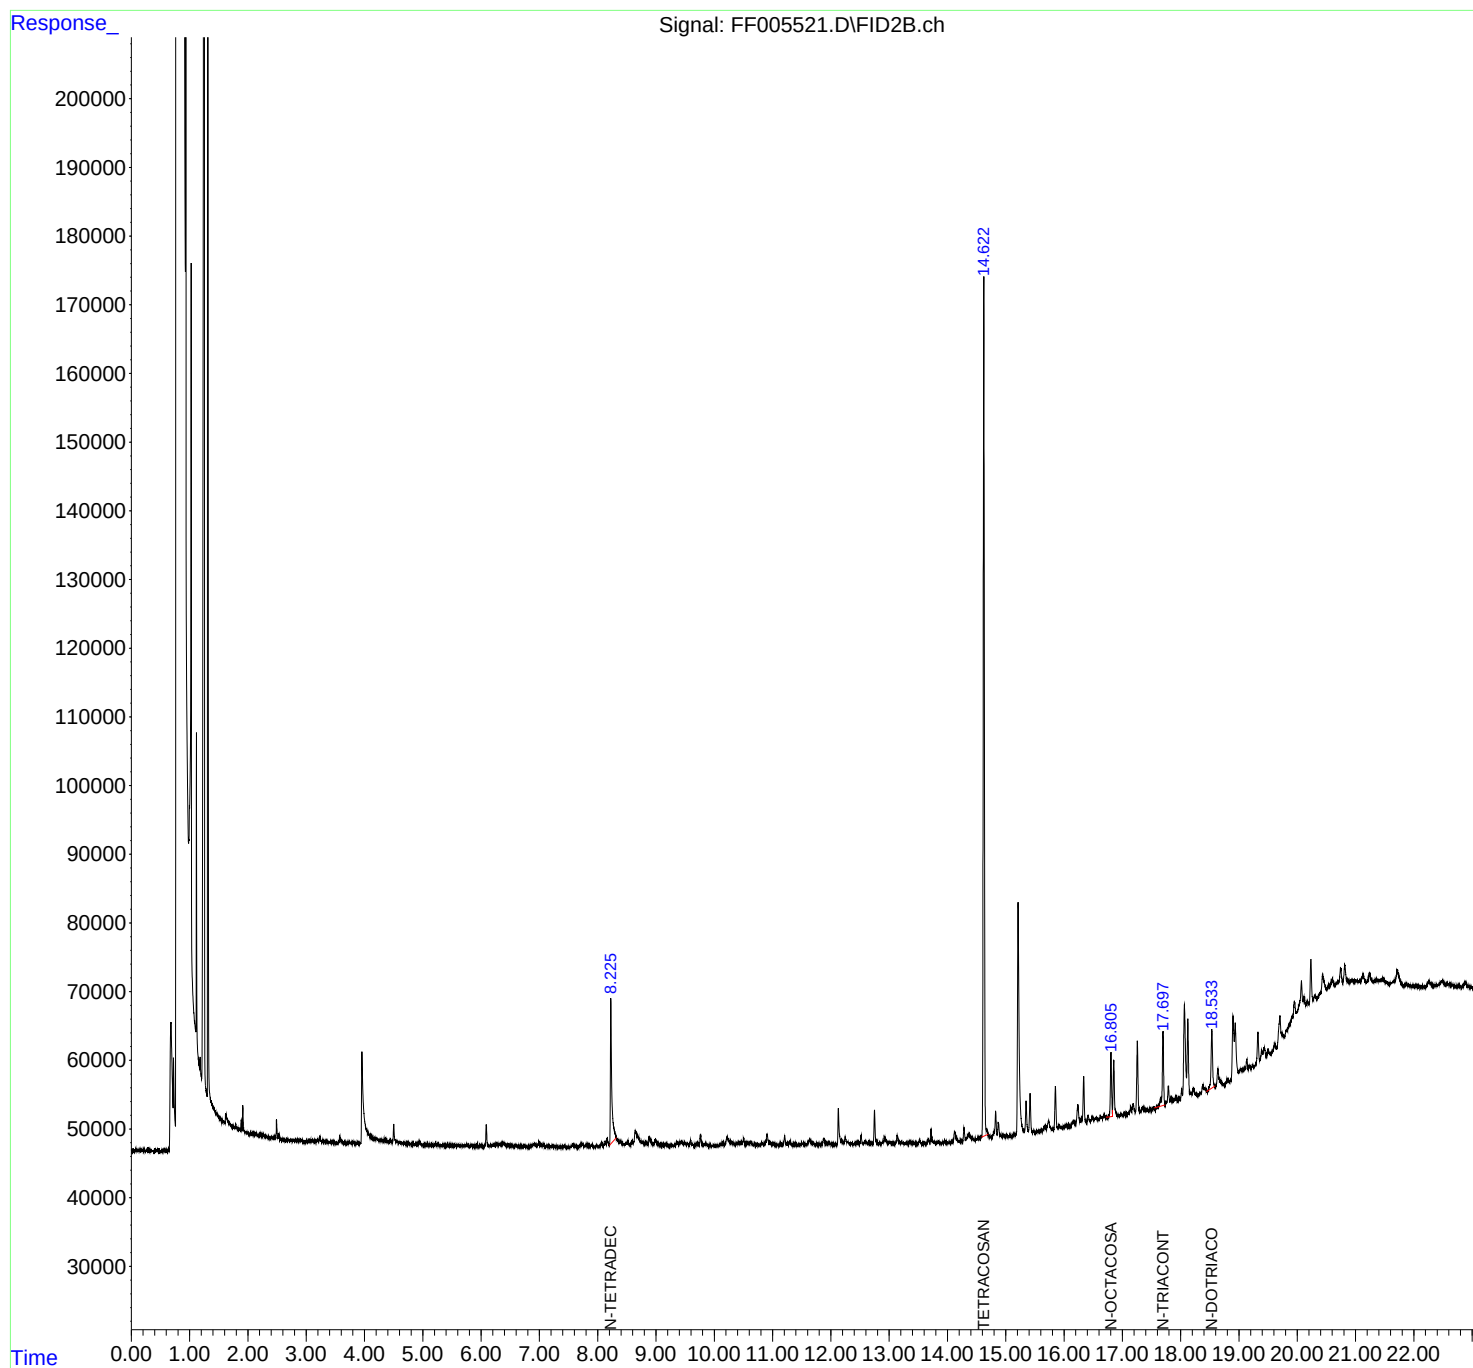


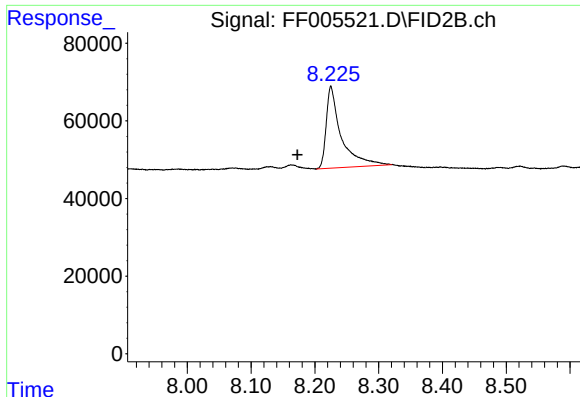

#4 N-TETRADECANE


R.T.: 8.225 min
Delta R.T.: 0.053 min
Response: 343594
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

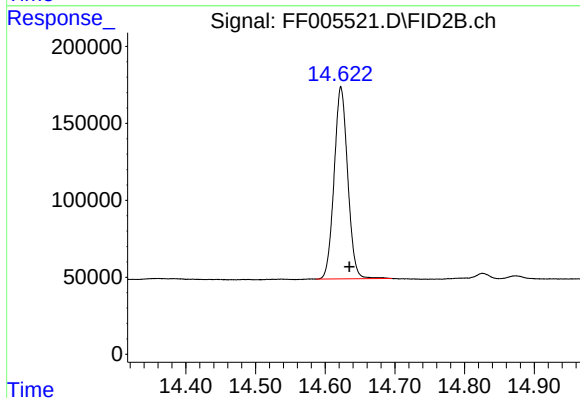


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.623 min
Delta R.T.: -0.012 min
Response: 1691740
Conc: 15.81 ug/ml

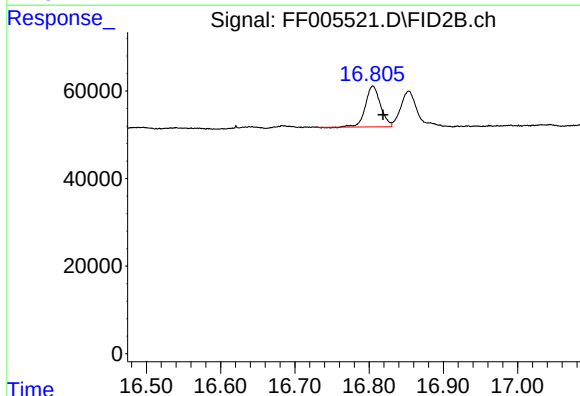


#12 N-OCTACOSANE

R.T.: 16.805 min
Delta R.T.: -0.014 min
Response: 130826
Conc: 1.10 ug/ml

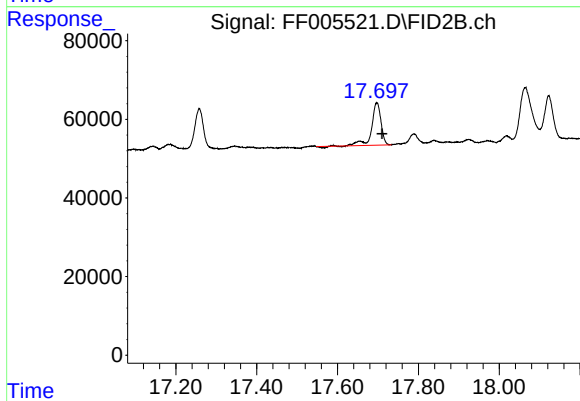

#13 N-TRIACONTANE

R.T.: 17.698 min
Delta R.T.: -0.013 min
Response: 172810
Conc: 1.43 ug/ml

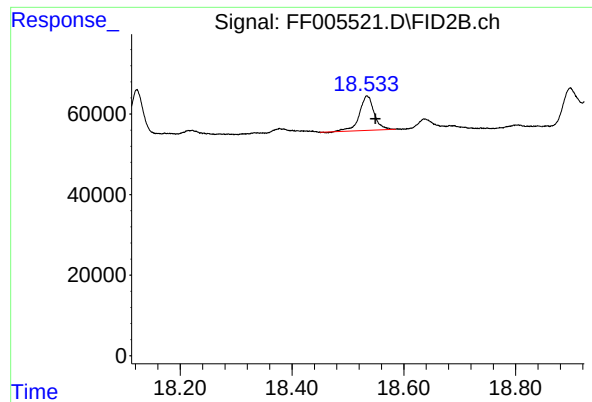

#14 N-DOTRIACONTANE

R.T.: 18.534 min
Delta R.T.: -0.015 min
Response: 155080
Conc: 1.25 ug/ml

Instrument :
FID_F
ClientSampleId :