

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
 Data File : FF005522.D
 Signal(s) : FID2B.ch
 Acq On : 10 Sep 2019 18:28
 Operator : DD\AJ
 Sample : K4764-08
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 ROLL-OFF-TPH-2

Integration File: autoint1.e
 Quant Time: Sep 11 01:51:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
 Quant Title :
 QLast Update : Wed Sep 04 03:16:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.622	1908035	17.831 ug/ml
Target Compounds			
4) N-TETRADECANE	8.225f	436894	3.099 ug/ml
10) N-TETRACOSANE	14.826	149608	1.223 ug/ml
11) N-HEXACOSANE	15.851	259747	2.170 ug/ml
12) N-OCTACOSANE	16.805	361993	3.034 ug/ml
13) N-TRIACONTANE	17.697	441609	3.651 ug/ml
14) N-DOTRIACONTANE	18.534	415969	3.356 ug/ml
16) N-HEXATRIACONTANE	20.113	239875	1.999 ug/ml
18) N-TETRACONTANE	21.751	454903	3.578 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005522.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 18:28
Operator : DD\AJ
Sample : K4764-08
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
ROLL-OFF-TPH-2

Integration File: autoint1.e
Quant Time: Sep 11 01:51:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

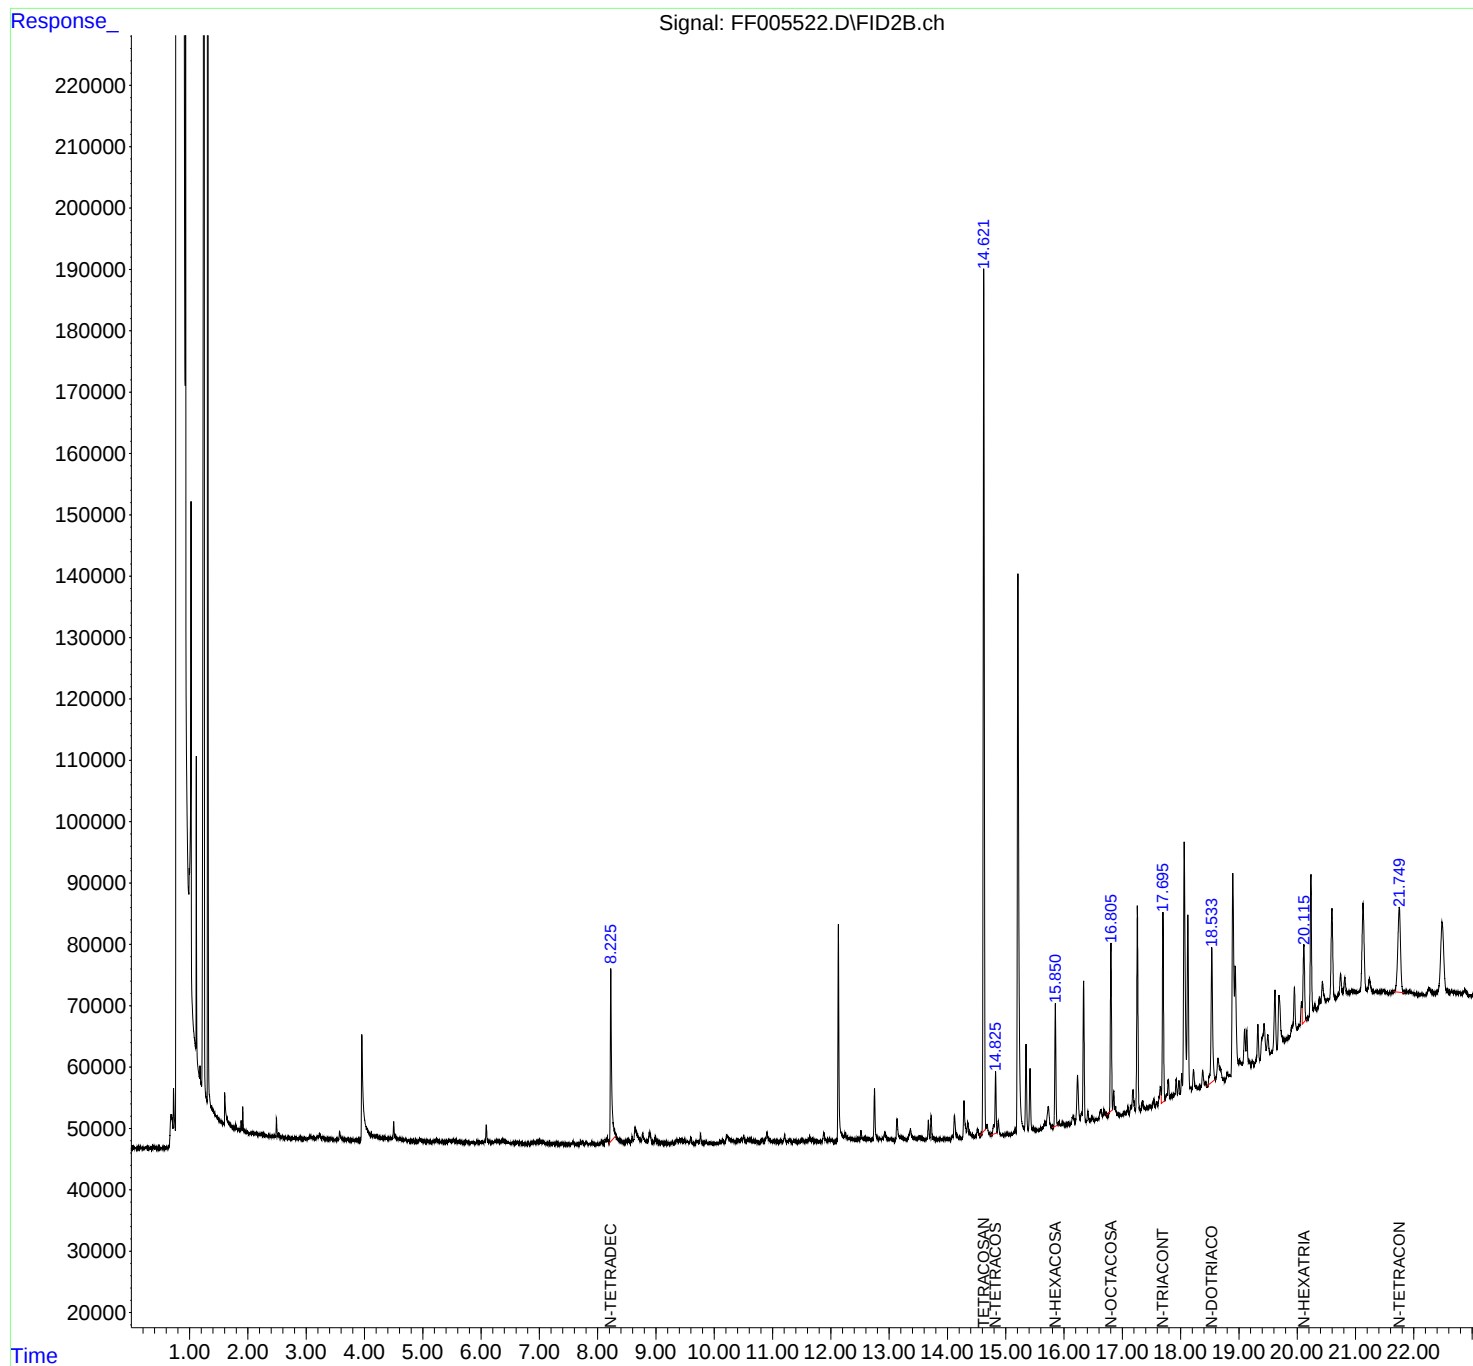


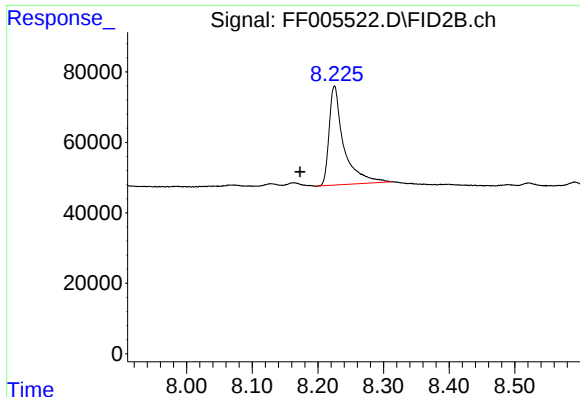

#4 N-TETRADECANE


R.T.: 8.225 min
Delta R.T.: 0.053 min
Response: 436894
Conc: 3.10 ug/ml

Instrument :
FID_F
ClientSampleId :
ROLL-OFF-TPH-2

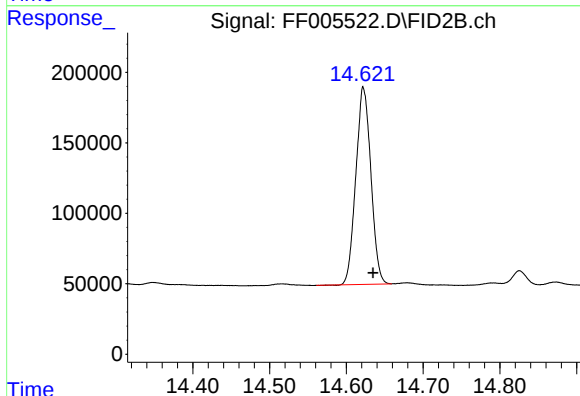


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.622 min
Delta R.T.: -0.012 min
Response: 1908035
Conc: 17.83 ug/ml

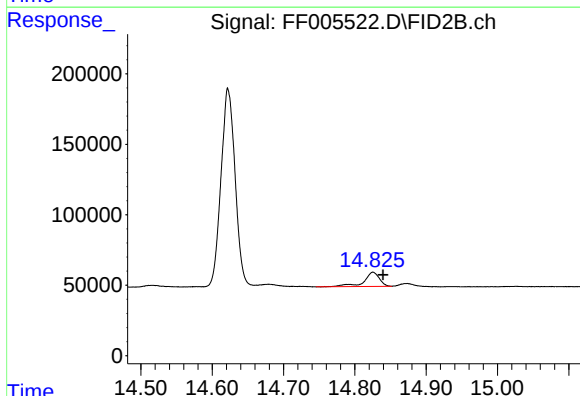


#10 N-TETRACOSANE

R.T.: 14.826 min
Delta R.T.: -0.014 min
Response: 149608
Conc: 1.22 ug/ml

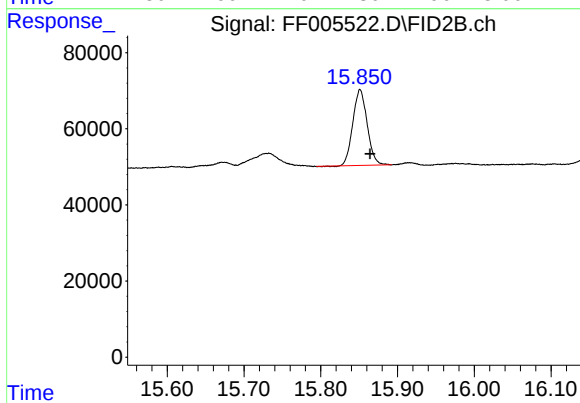

#11 N-HEXACOSANE


R.T.: 15.851 min
Delta R.T.: -0.013 min
Response: 259747
Conc: 2.17 ug/ml

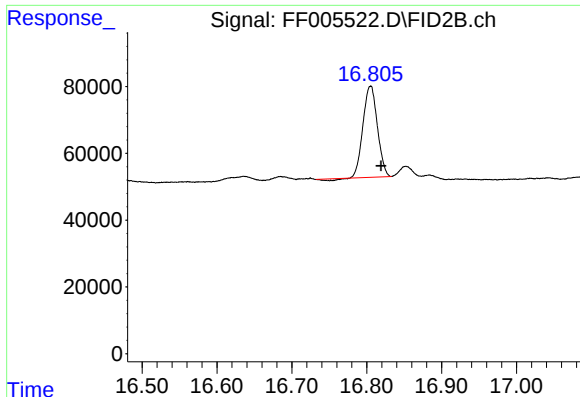

#12 N-OCTACOSANE


R.T.: 16.805 min
Delta R.T.: -0.014 min
Response: 361993
Conc: 3.03 ug/ml

Instrument :
FID_F
ClientSampleId :
ROLL-OFF-TPH-2

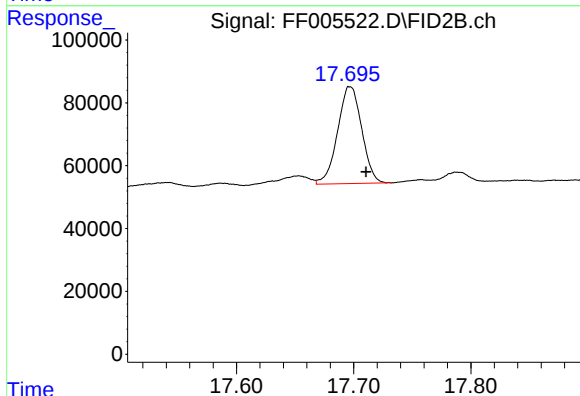


#13 N-TRIACONTANE

R.T.: 17.697 min
Delta R.T.: -0.014 min
Response: 441609
Conc: 3.65 ug/ml

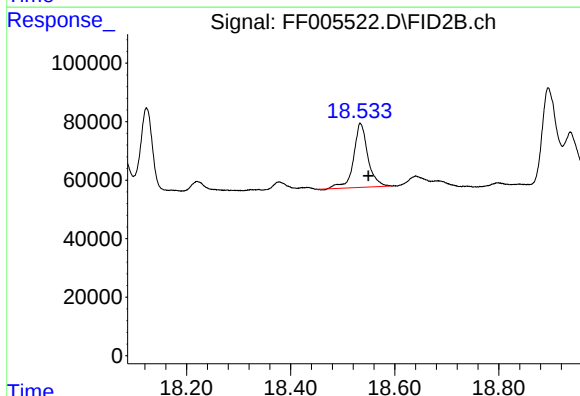


#14 N-DOTRIACONTANE

R.T.: 18.534 min
Delta R.T.: -0.015 min
Response: 415969
Conc: 3.36 ug/ml

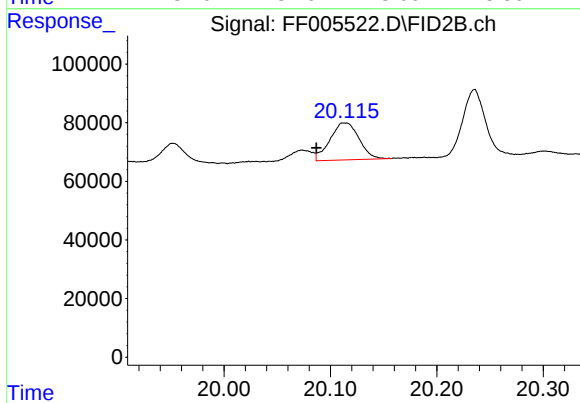

#16 N-HEXATRIACONTANE

R.T.: 20.113 min
Delta R.T.: 0.027 min
Response: 239875
Conc: 2.00 ug/ml

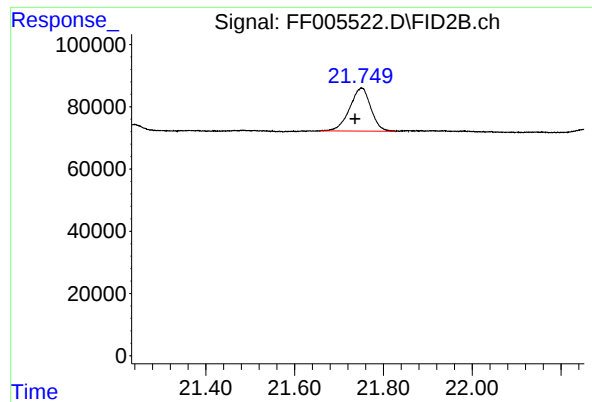

#18 N-TETRACONTANE

R.T.: 21.751 min
Delta R.T.: 0.014 min
Response: 454903
Conc: 3.58 ug/ml

Instrument :
FID_F
ClientSampleId :
ROLL-OFF-TPH-2