

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005526.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 20:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 11 01:52:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.623	1942825	18.156 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.537	123573	0.997 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005526.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 20:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 11 01:52:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

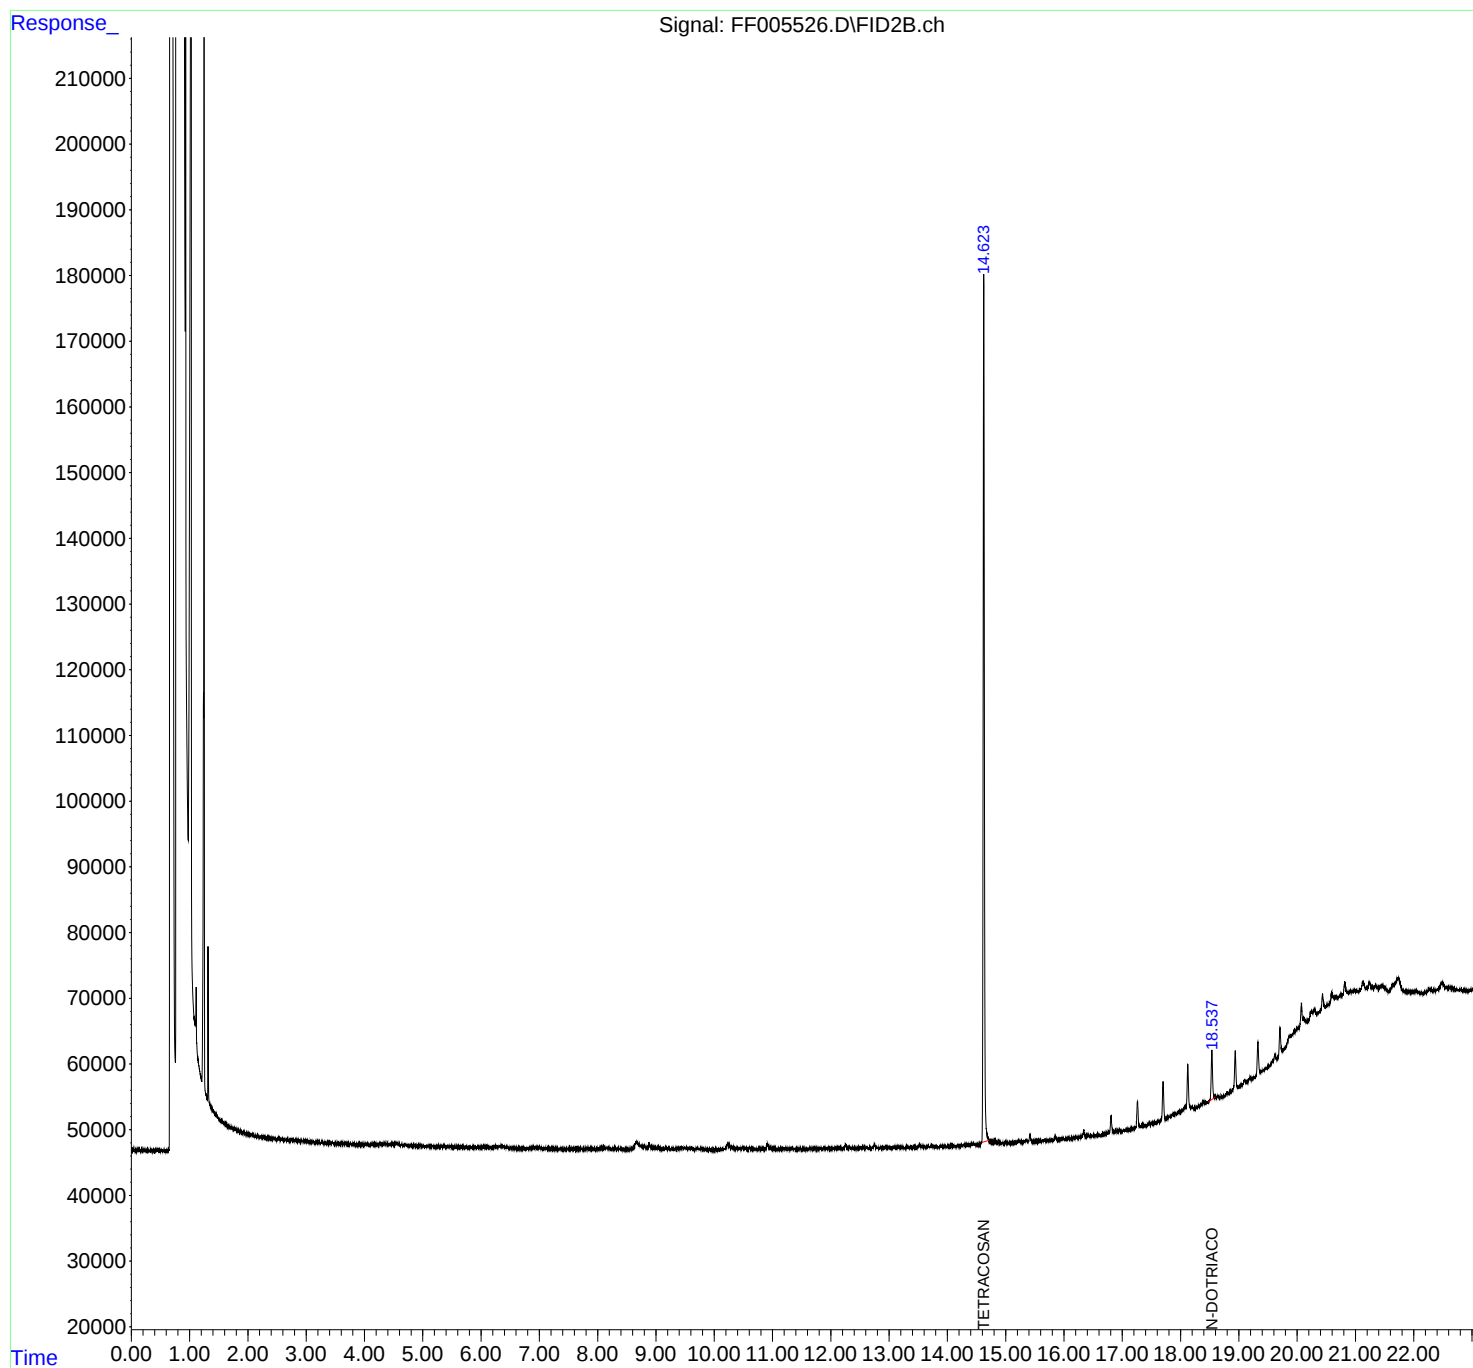


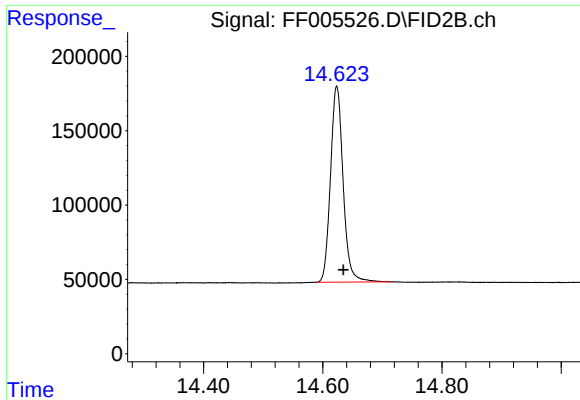

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.623 min
Delta R.T.: -0.011 min
Response: 1942825
Conc: 18.16 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

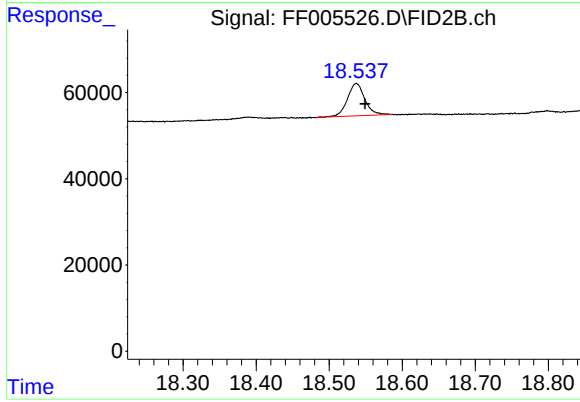

#14 N-DOTRIACONTANE

R.T.: 18.537 min
Delta R.T.: -0.012 min
Response: 123573
Conc: 1.00 ug/ml