

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005515.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 13:26
Operator : DD\AJ
Sample : PB122922BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB122922BL

Integration File: autoint1.e
Quant Time: Sep 11 01:48:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	2247135	21.000 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091019\
Data File : FF005515.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2019 13:26
Operator : DD\AJ
Sample : PB122922BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB122922BL

Integration File: autoint1.e
Quant Time: Sep 11 01:48:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

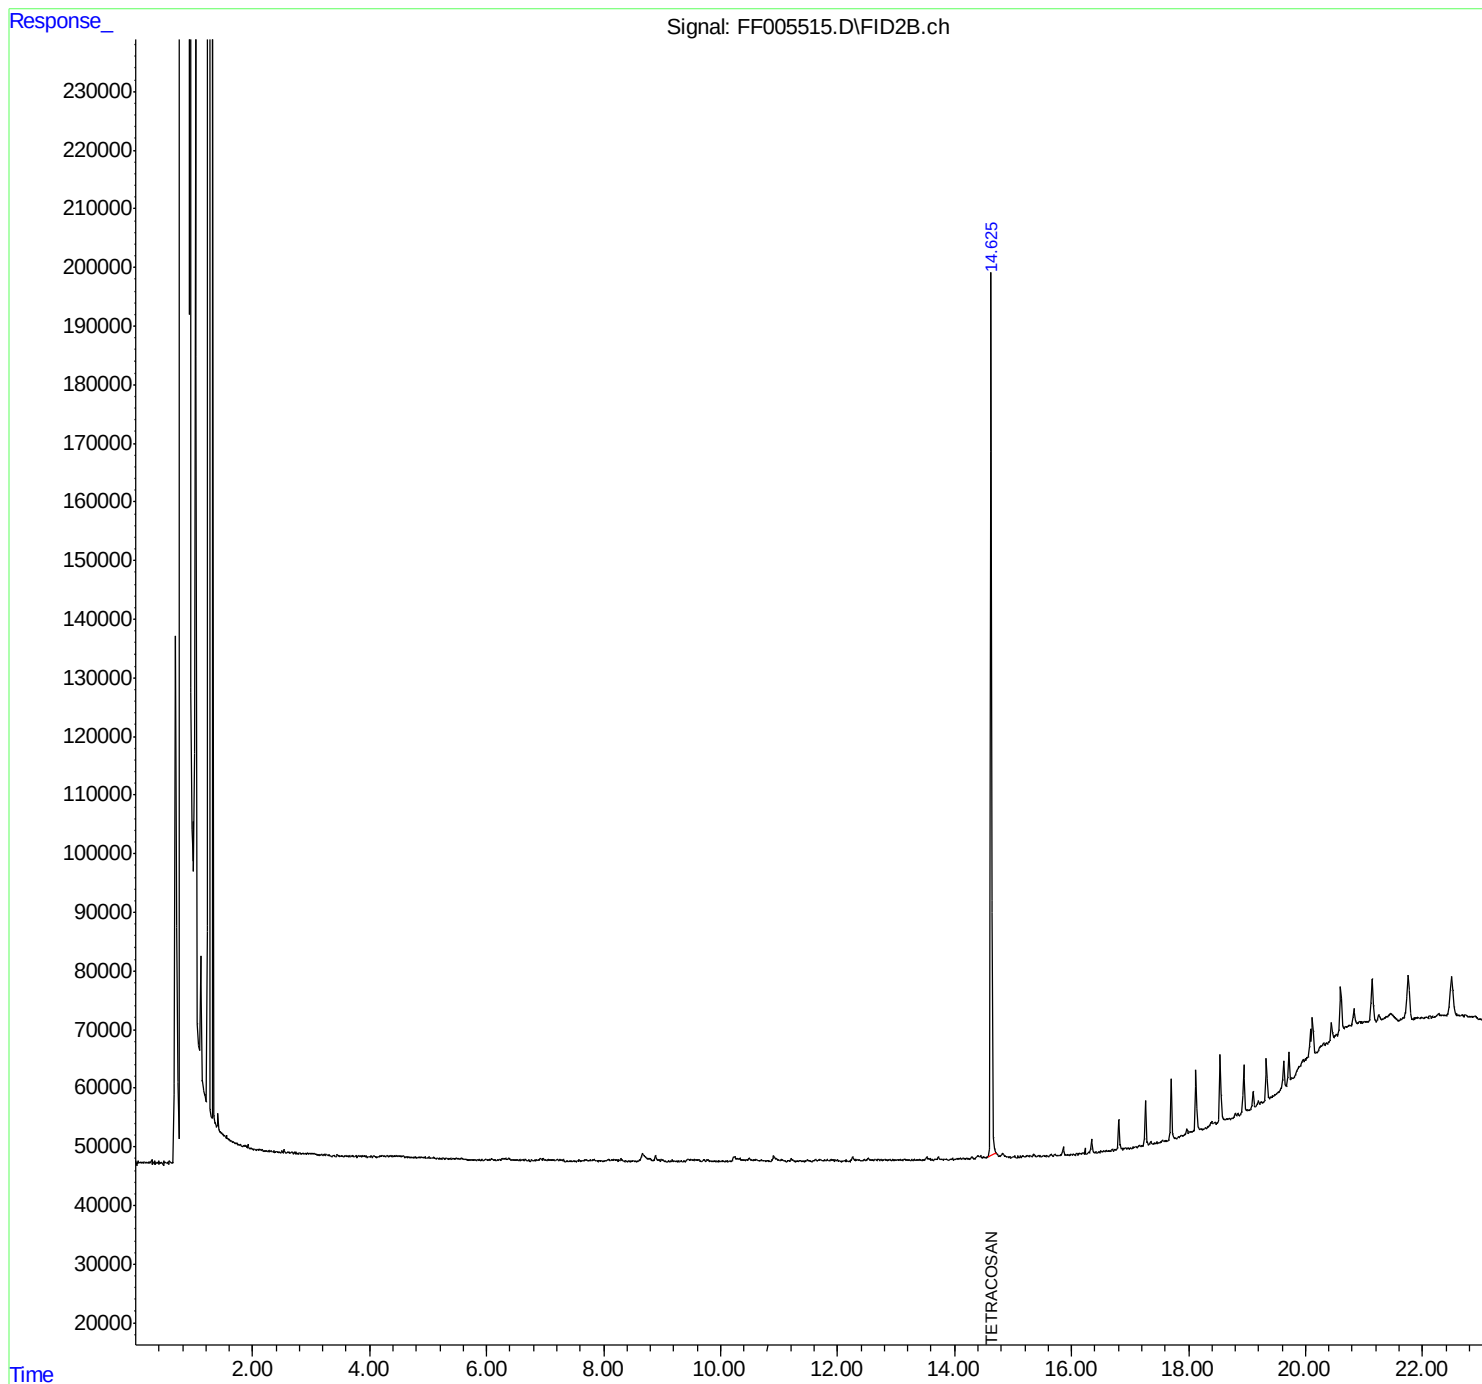

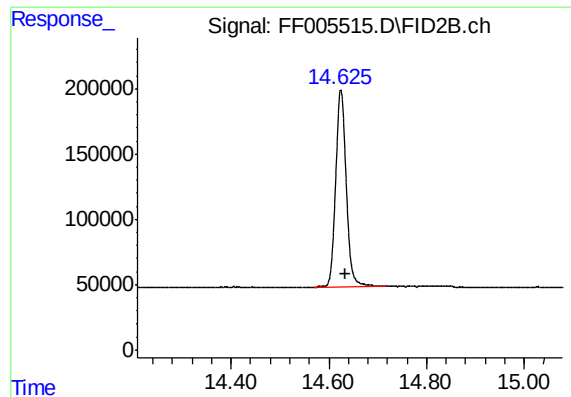

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.625 min
Delta R.T.: -0.010 min
Response: 2247135
Conc: 21.00 ug/ml

Instrument :
FID_F
ClientSampleId :
PB122922BL