

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091020\
 Data File : FF007499.D
 Signal(s) : FID2B.ch
 Acq On : 10 Sep 2020 14:39
 Operator : DD\AJ
 Sample : L3939-03MS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 11 03:37:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.741	2833888	19.268 ug/ml
Target Compounds			
2) N-DECANE	4.455	3966609	24.868 ug/ml
3) N-DODECANE	6.480	4122553	25.341 ug/ml
4) N-TETRADECANE	8.277	4177622	25.388 ug/ml
5) N-HEXADECANE	9.881	4173734	24.732 ug/ml
6) N-OCTADECANE	11.325	4105159	24.091 ug/mlm
7) N-EICOSANE	12.639	4181874	24.873 ug/ml
8) N-DOCOSANE	13.840	4108234	24.935 ug/ml
10) N-TETRACOSANE	14.946	4375191	26.826 ug/ml
11) N-HEXACOSANE	15.971	3584136	22.673 ug/ml
12) N-OCTACOSANE	16.923	3693149	24.065 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091020\
Data File : FF007499.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2020 14:39
Operator : DD\AJ
Sample : L3939-03MS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 11 03:37:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

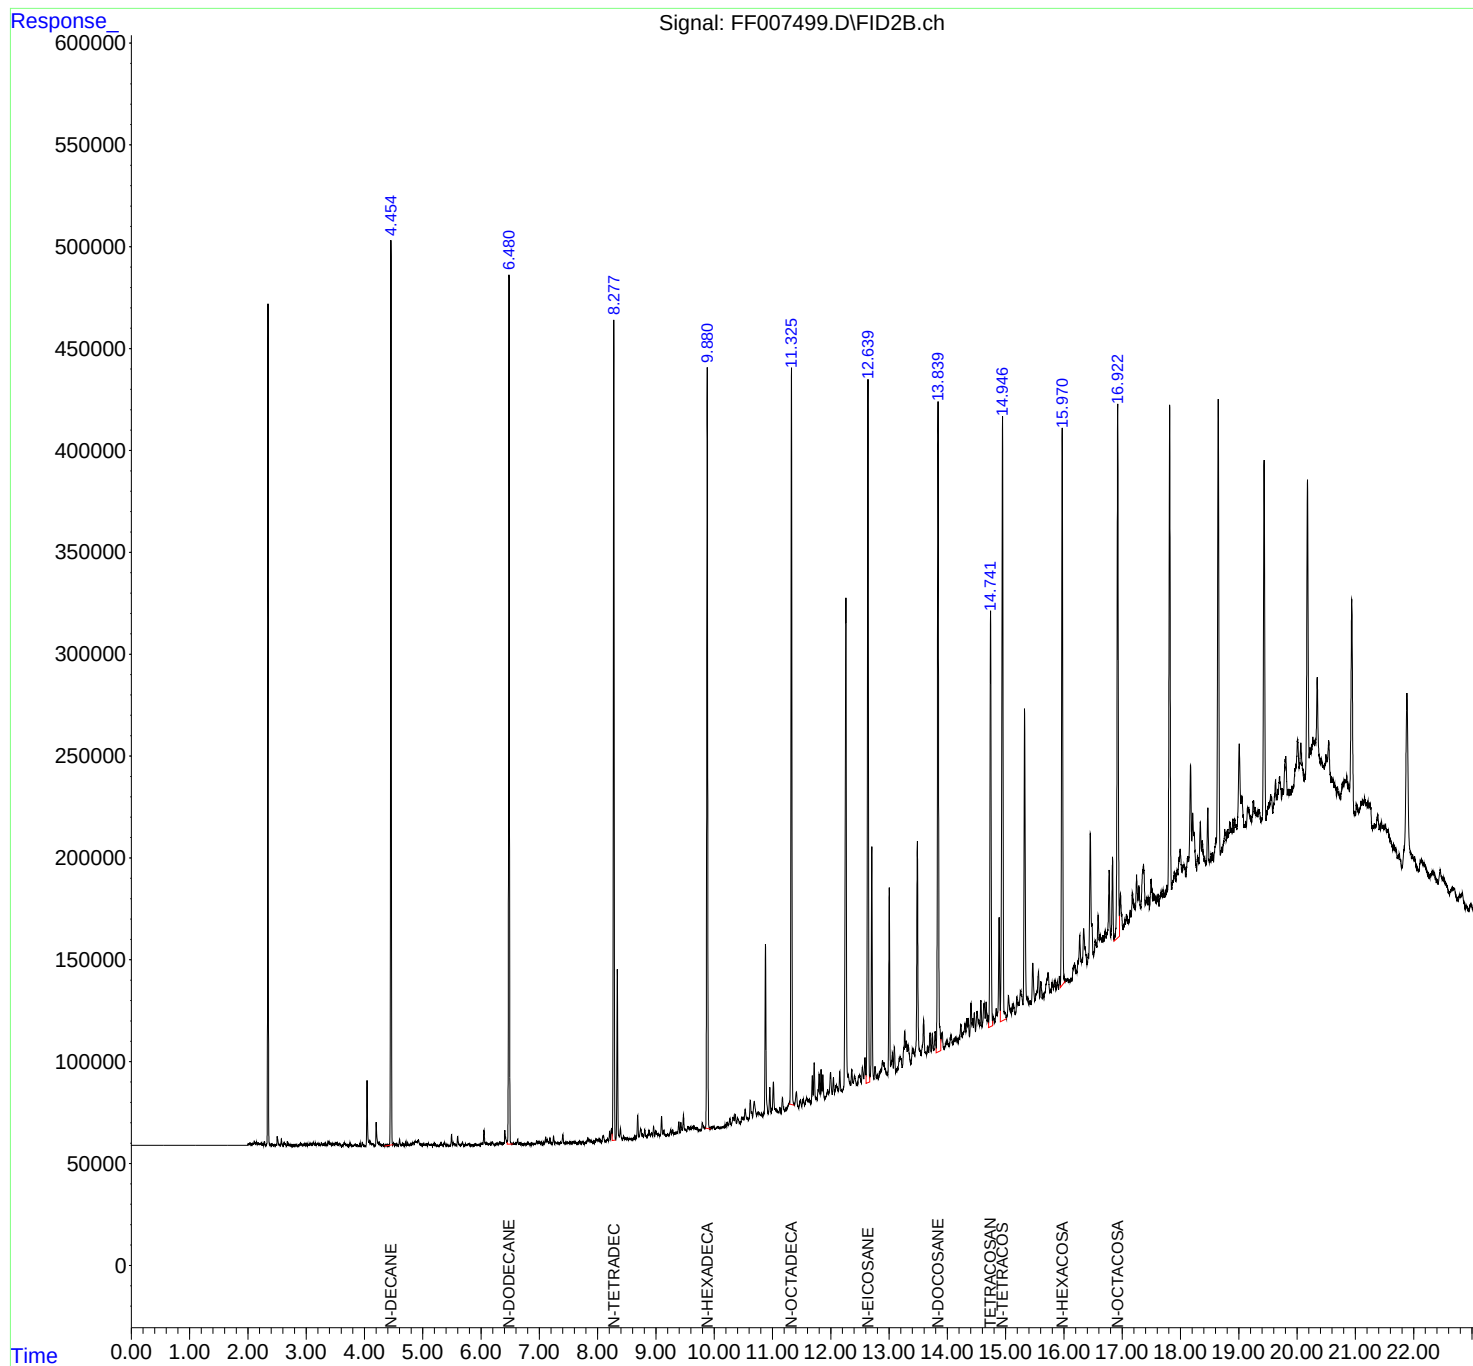

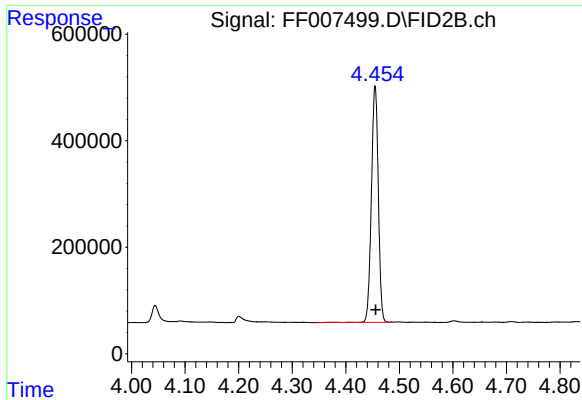


#2 N-DECANE

R.T.: 4.455 min
Delta R.T.: -0.001 min
Response: 3966609
Conc: 24.87 ug/ml

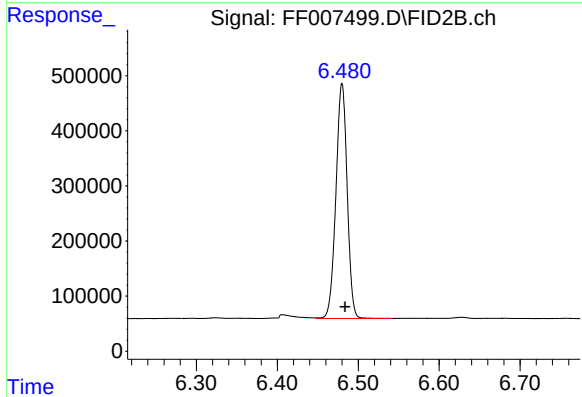


#3 N-DODECANE

R.T.: 6.480 min
Delta R.T.: -0.003 min
Response: 4122553
Conc: 25.34 ug/ml

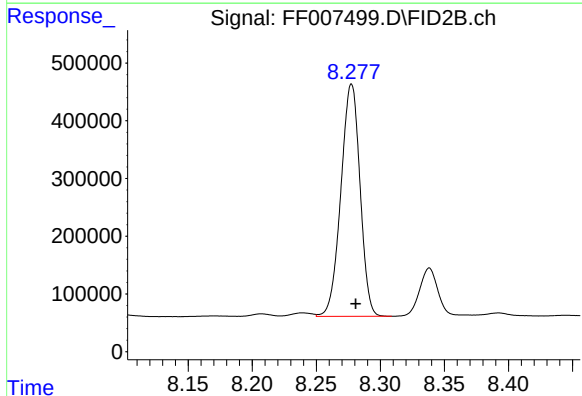


#4 N-TETRADECANE

R.T.: 8.277 min
Delta R.T.: -0.003 min
Response: 4177622
Conc: 25.39 ug/ml

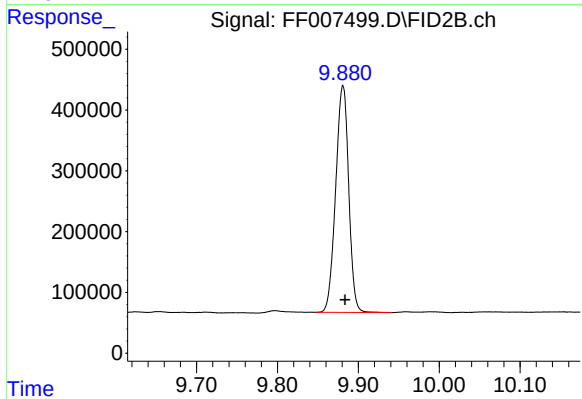


#5 N-HEXADECANE

R.T.: 9.881 min
Delta R.T.: -0.003 min
Response: 4173734
Conc: 24.73 ug/ml

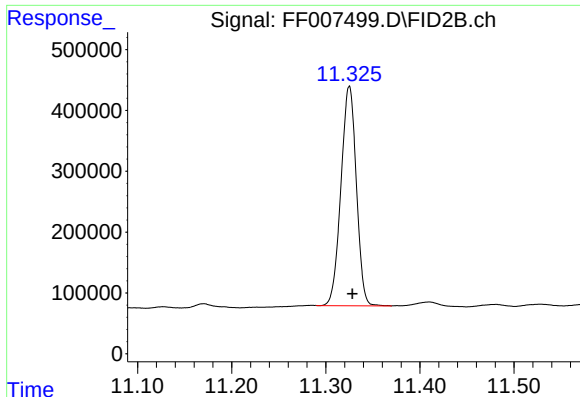


#6 N-OCTADECANE

R.T.: 11.325 min
Delta R.T.: -0.003 min
Response: 4105159
Conc: 24.09 ug/ml m

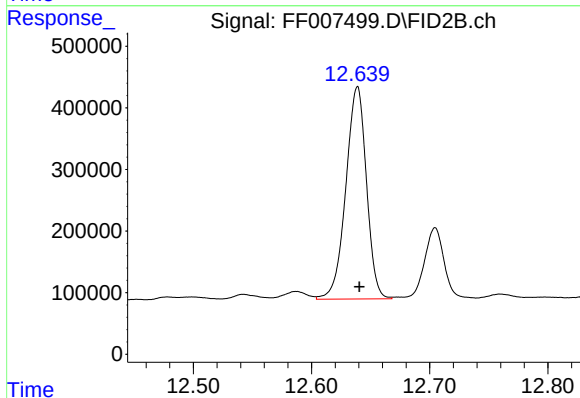


#7 N-EICOSANE

R.T.: 12.639 min
Delta R.T.: -0.002 min
Response: 4181874
Conc: 24.87 ug/ml

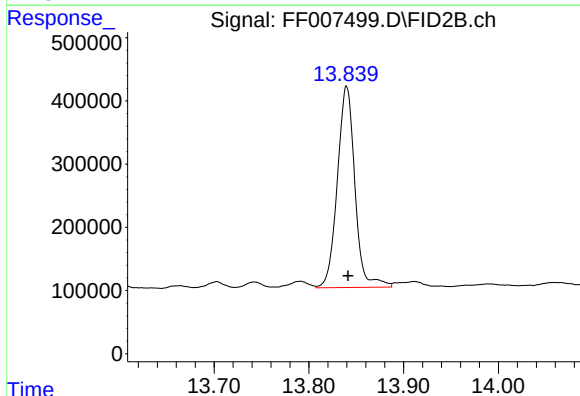


#8 N-DOCOSANE

R.T.: 13.840 min
Delta R.T.: -0.002 min
Response: 4108234
Conc: 24.93 ug/ml

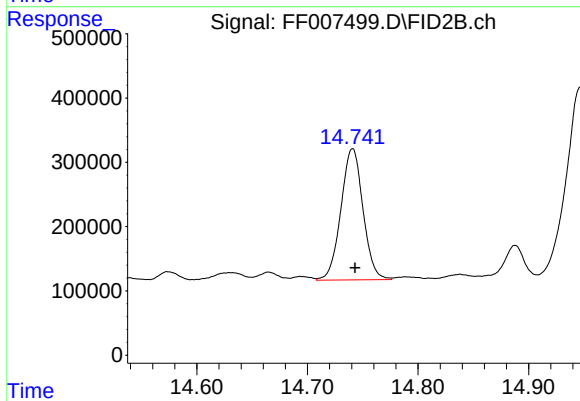


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.741 min
Delta R.T.: -0.002 min
Response: 2833888
Conc: 19.27 ug/ml

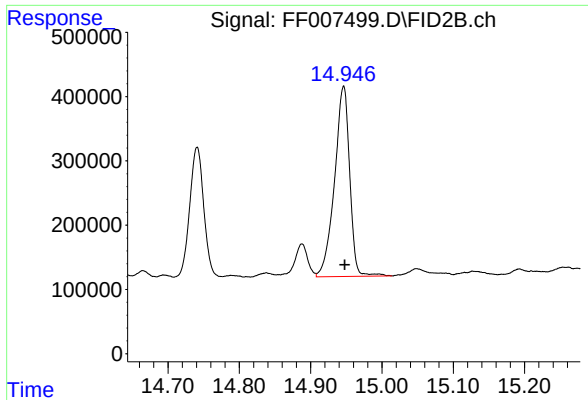


#10 N-TETRACOSANE

R.T.: 14.946 min
Delta R.T.: -0.002 min
Response: 4375191
Conc: 26.83 ug/ml

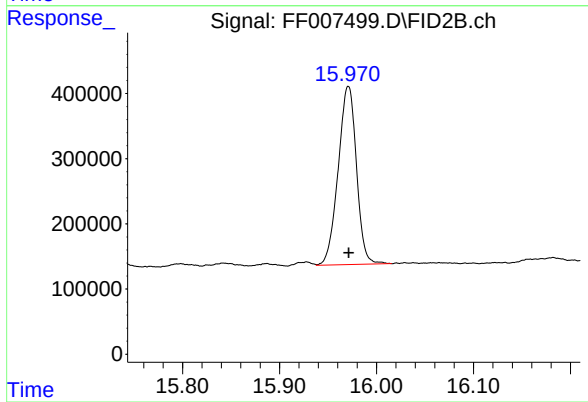

#11 N-HEXACOSANE

R.T.: 15.971 min
Delta R.T.: 0.000 min
Response: 3584136
Conc: 22.67 ug/ml

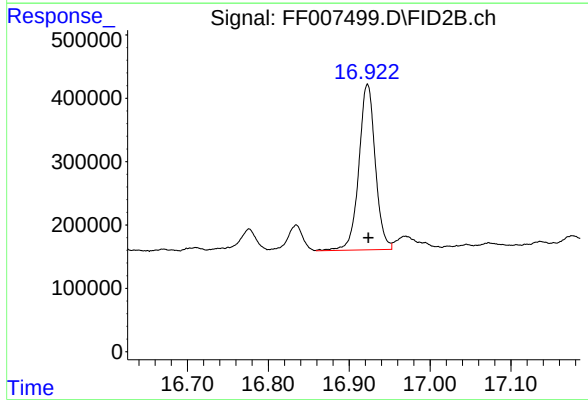

#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: 0.000 min
Response: 3693149
Conc: 24.06 ug/ml