

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091020\
 Data File : FF007500.D
 Signal(s) : FID2B.ch
 Acq On : 10 Sep 2020 15:10
 Operator : DD\AJ
 Sample : L3939-03MSD
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 11 03:37:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2615275	17.782 ug/ml
Target Compounds			
2) N-DECANE	4.455	3796706	23.803 ug/ml
3) N-DODECANE	6.481	3920857	24.101 ug/ml
4) N-TETRADECANE	8.278	3945072	23.974 ug/ml
5) N-HEXADECANE	9.881	3909429	23.166 ug/ml
6) N-OCTADECANE	11.325	3819935	22.417 ug/mlm
7) N-EICOSANE	12.638	3900018	23.197 ug/ml
8) N-DOCOSANE	13.840	3830304	23.248 ug/ml
10) N-TETRACOSANE	14.945	4024477	24.675 ug/ml
11) N-HEXACOSANE	15.970	3423452	21.657 ug/ml
12) N-OCTACOSANE	16.923	3467282	22.593 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091020\
Data File : FF007500.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2020 15:10
Operator : DD\AJ
Sample : L3939-03MSD
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 11 03:37:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

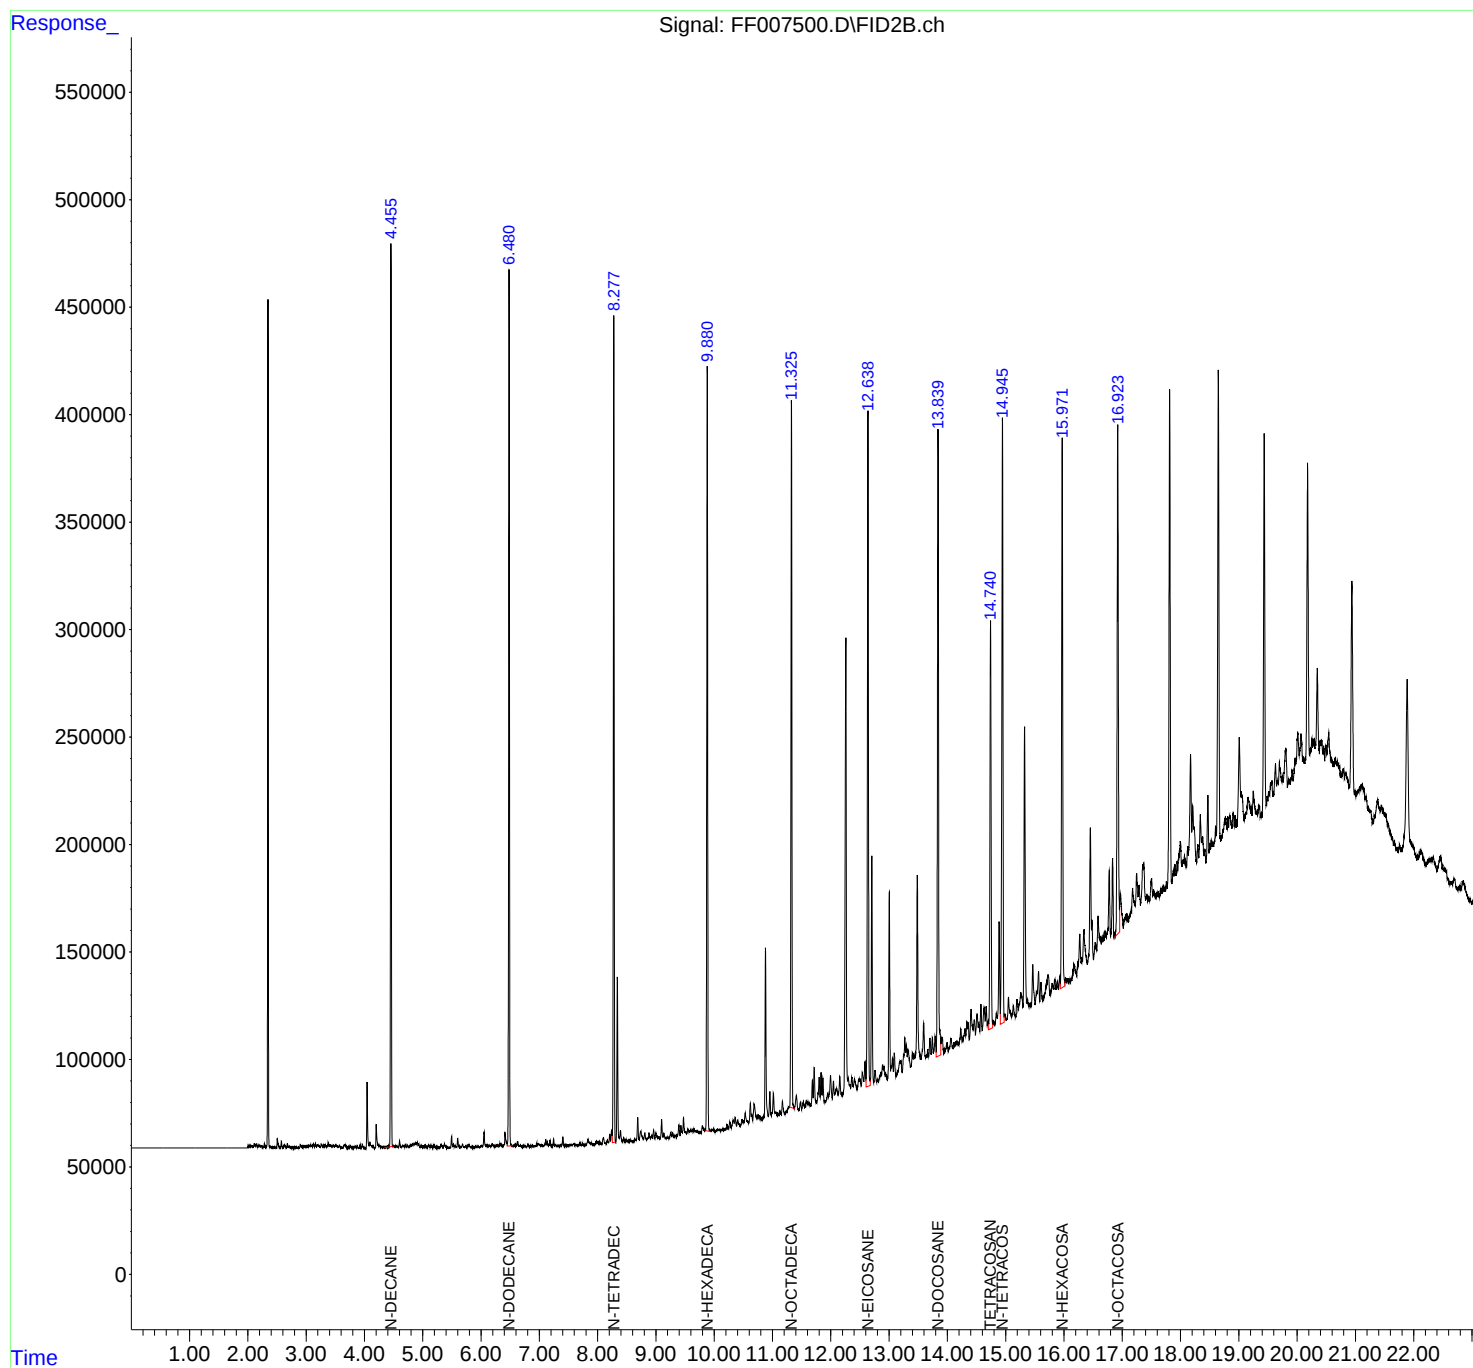

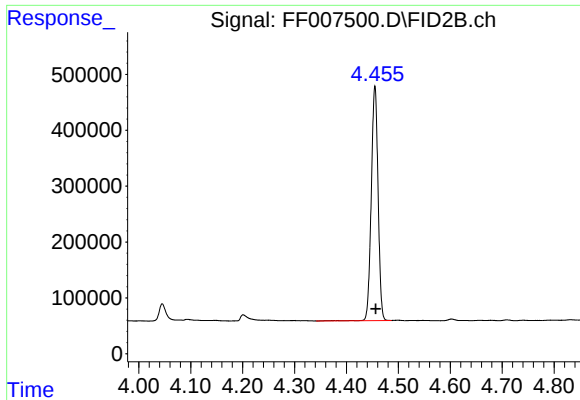


#2 N-DECANE

R.T.: 4.455 min
Delta R.T.: -0.001 min
Response: 3796706
Conc: 23.80 ug/ml

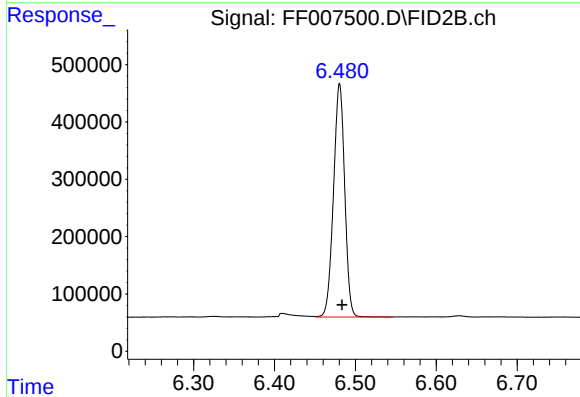


#3 N-DODECANE

R.T.: 6.481 min
Delta R.T.: -0.003 min
Response: 3920857
Conc: 24.10 ug/ml

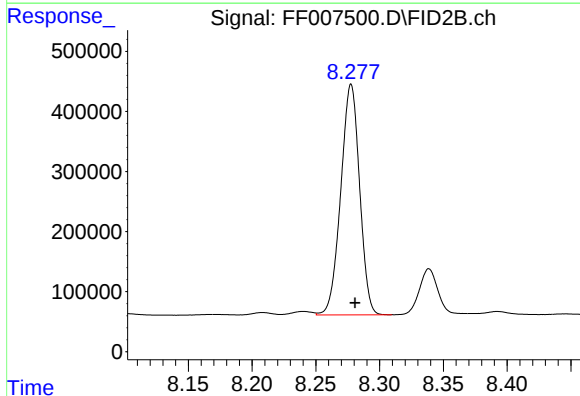


#4 N-TETRADECANE

R.T.: 8.278 min
Delta R.T.: -0.003 min
Response: 3945072
Conc: 23.97 ug/ml

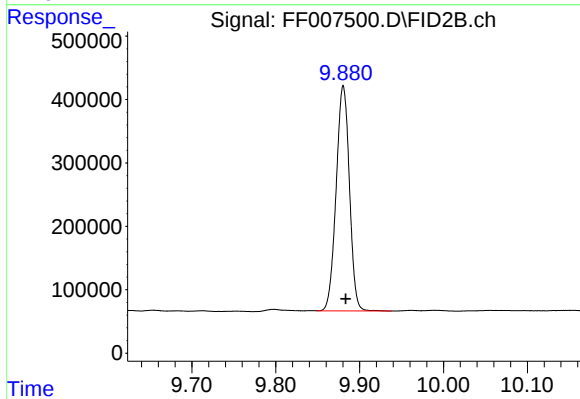


#5 N-HEXADECANE

R.T.: 9.881 min
Delta R.T.: -0.003 min
Response: 3909429
Conc: 23.17 ug/ml

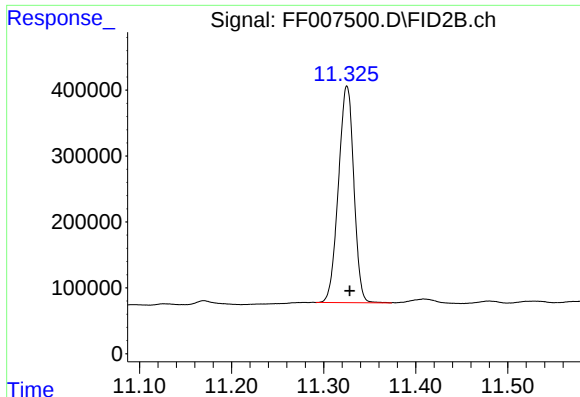


#6 N-OCTADECANE

R.T.: 11.325 min
Delta R.T.: -0.003 min
Response: 3819935
Conc: 22.42 ug/ml m

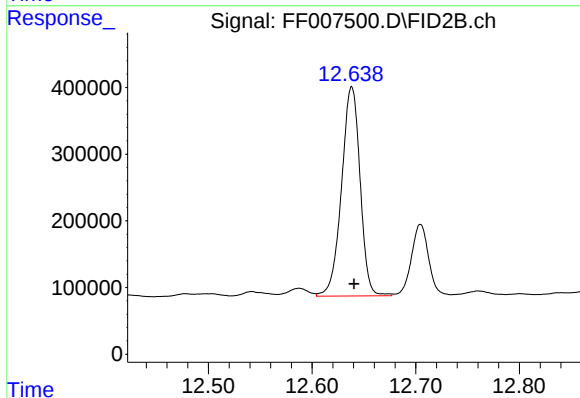


#7 N-EICOSANE

R.T.: 12.638 min
Delta R.T.: -0.002 min
Response: 3900018
Conc: 23.20 ug/ml

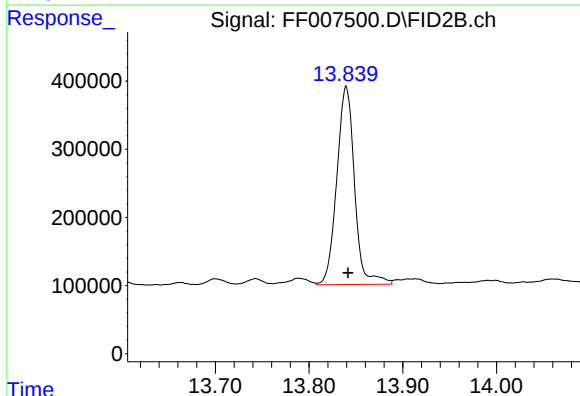


#8 N-DOCOSANE

R.T.: 13.840 min
Delta R.T.: -0.002 min
Response: 3830304
Conc: 23.25 ug/ml

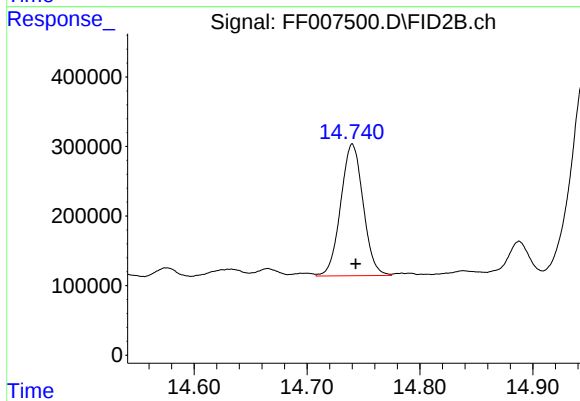


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.003 min
Response: 2615275
Conc: 17.78 ug/ml

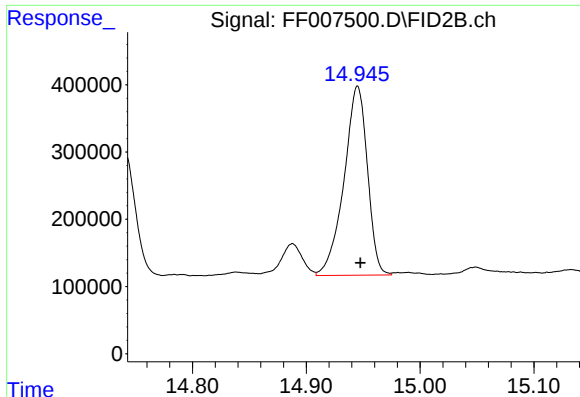


#10 N-TETRACOSANE

R.T.: 14.945 min
Delta R.T.: -0.003 min
Response: 4024477
Conc: 24.68 ug/ml

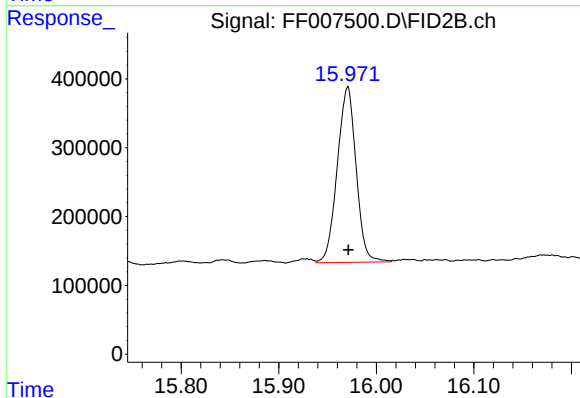

#11 N-HEXACOSANE

R.T.: 15.970 min
Delta R.T.: 0.000 min
Response: 3423452
Conc: 21.66 ug/ml

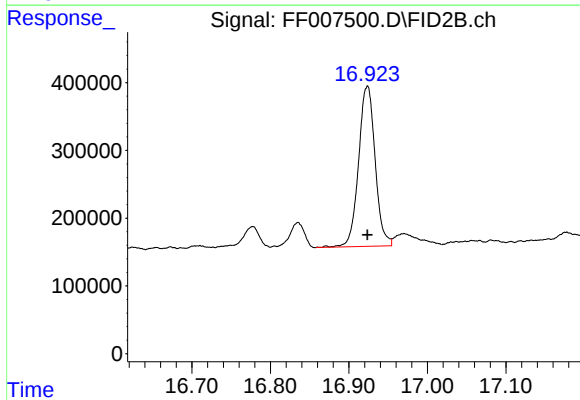

#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: 0.000 min
Response: 3467282
Conc: 22.59 ug/ml