

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014468.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 06:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 01:30:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.815	77762	0.592 ug/ml
16)	N-HEXATRIACONTANE	20.370	116638	1.052 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014468.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 06:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 11 01:30:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

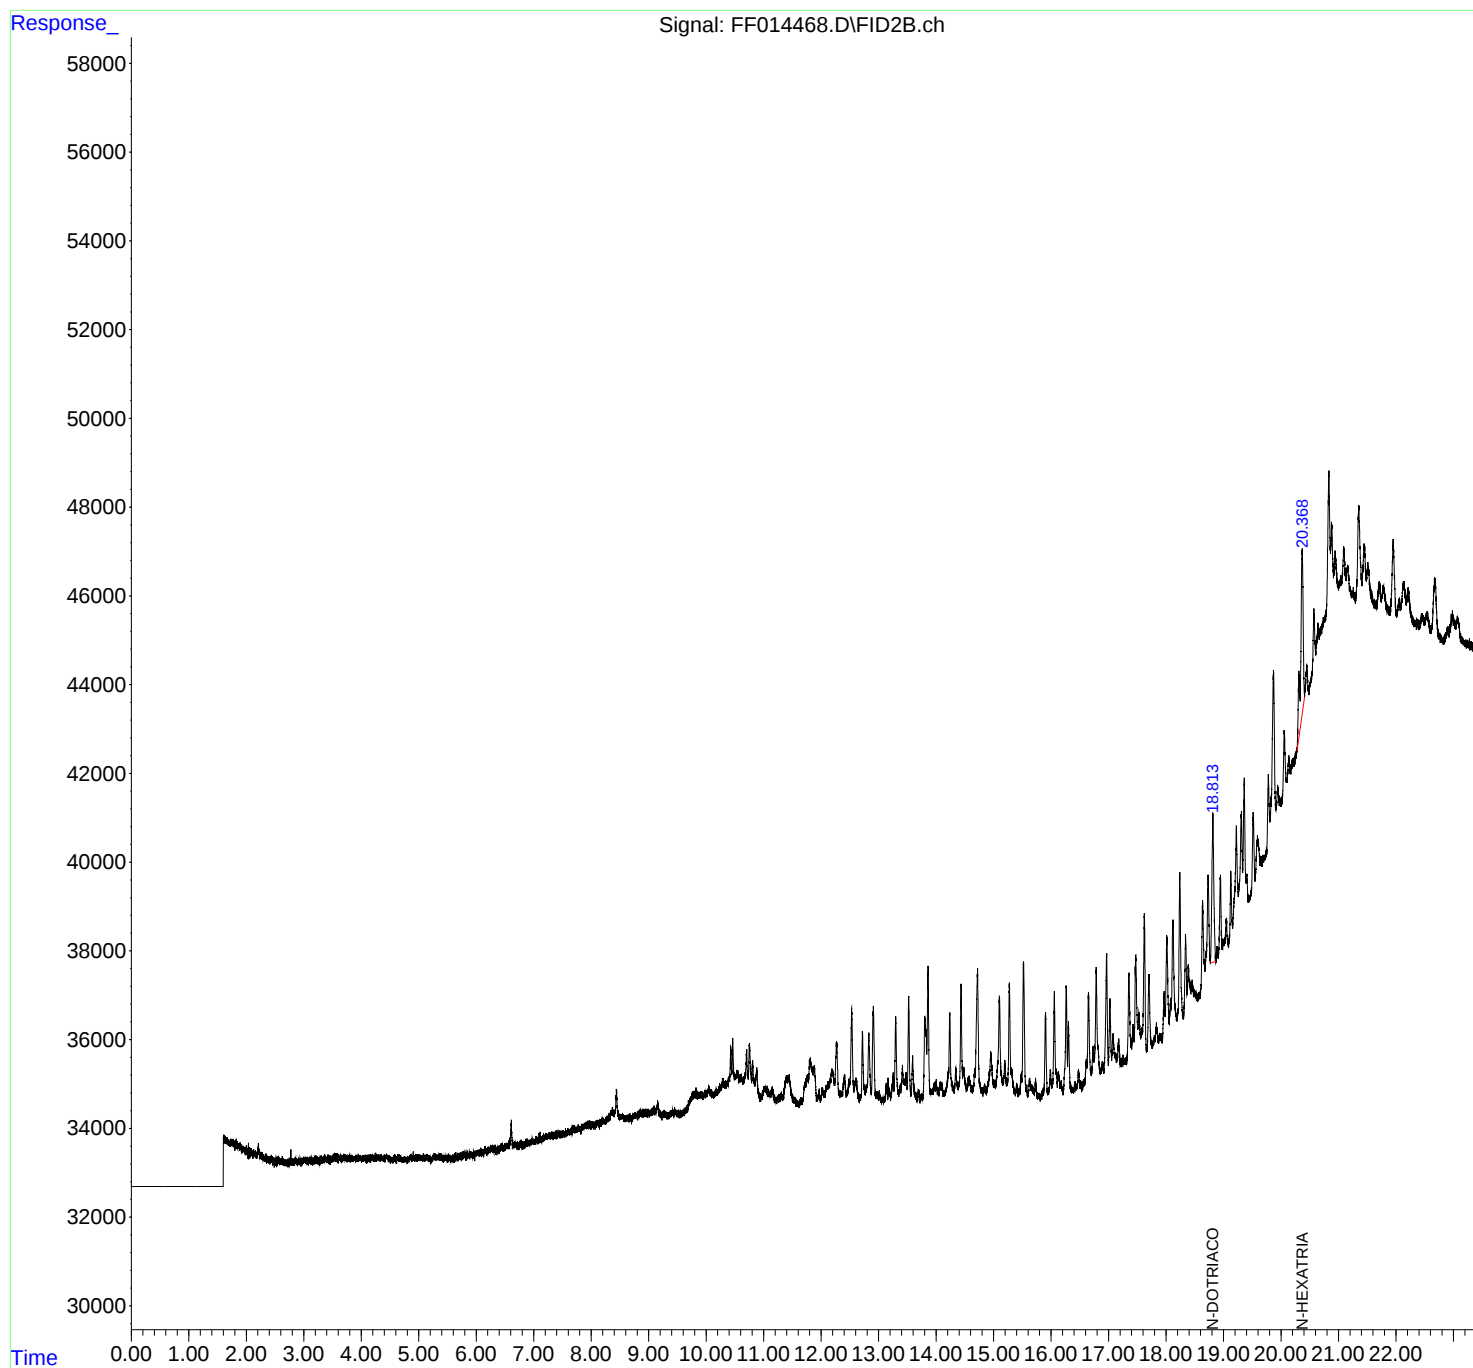


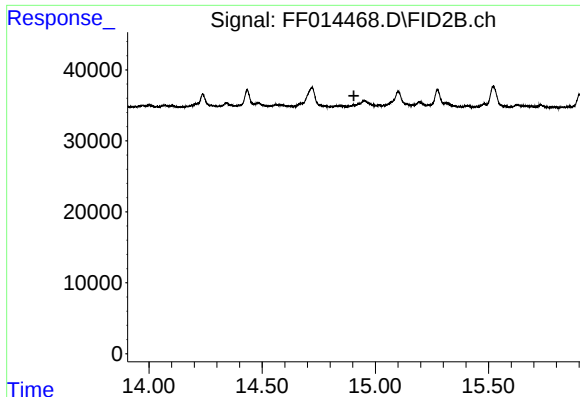

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.905 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

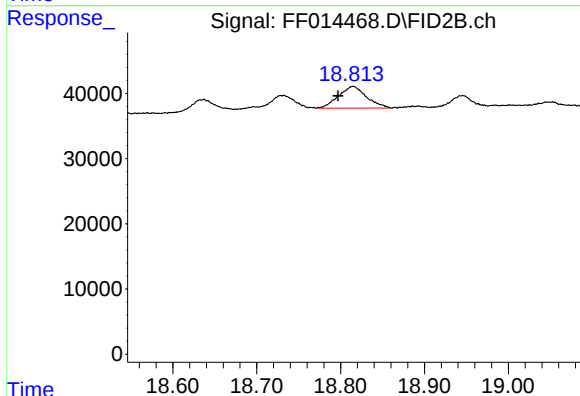

#14 N-DOTRIACONTANE

R.T.: 18.815 min
Delta R.T.: 0.018 min
Response: 77762
Conc: 0.59 ug/ml

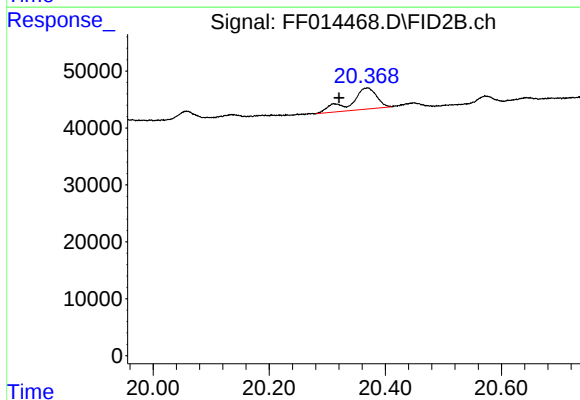

#16 N-HEXATRIACONTANE

R.T.: 20.370 min
Delta R.T.: 0.050 min
Response: 116638
Conc: 1.05 ug/ml