

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014472.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 08:42
Operator : YP\AJ
Sample : P3845-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 11 01:30:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.898	2217062	18.784 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014472.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 08:42
Operator : YP\AJ
Sample : P3845-19
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 11 01:30:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

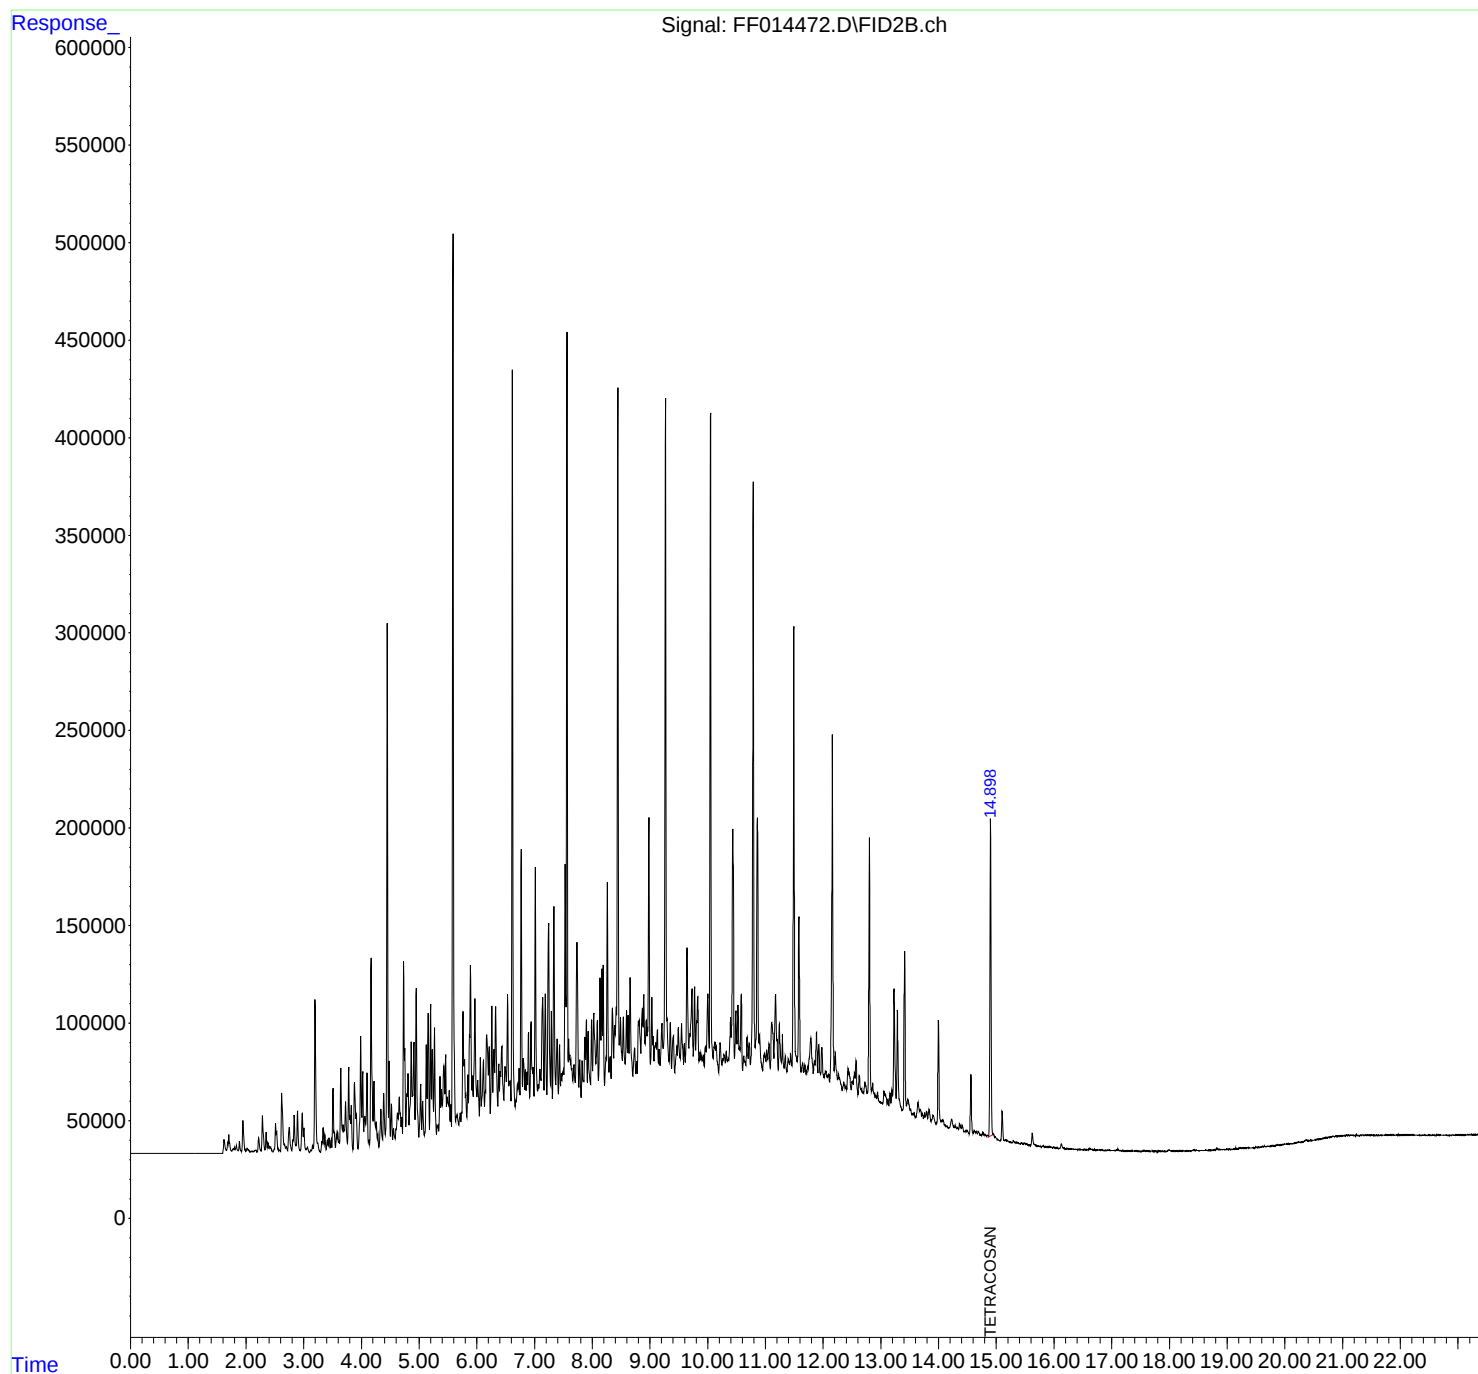

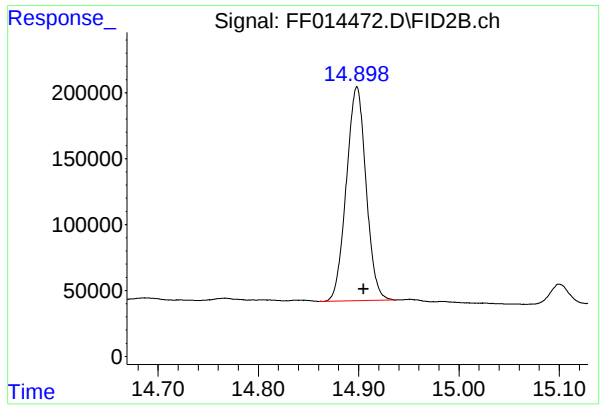

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.898 min
Delta R.T.: -0.007 min
Response: 2217062
Conc: 18.78 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP