

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014475.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 10:09
Operator : YP\AJ
Sample : P3845-19 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 11 01:31:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.900	369155	3.128 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014475.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 10:09
Operator : YP\AJ
Sample : P3845-19 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 11 01:31:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

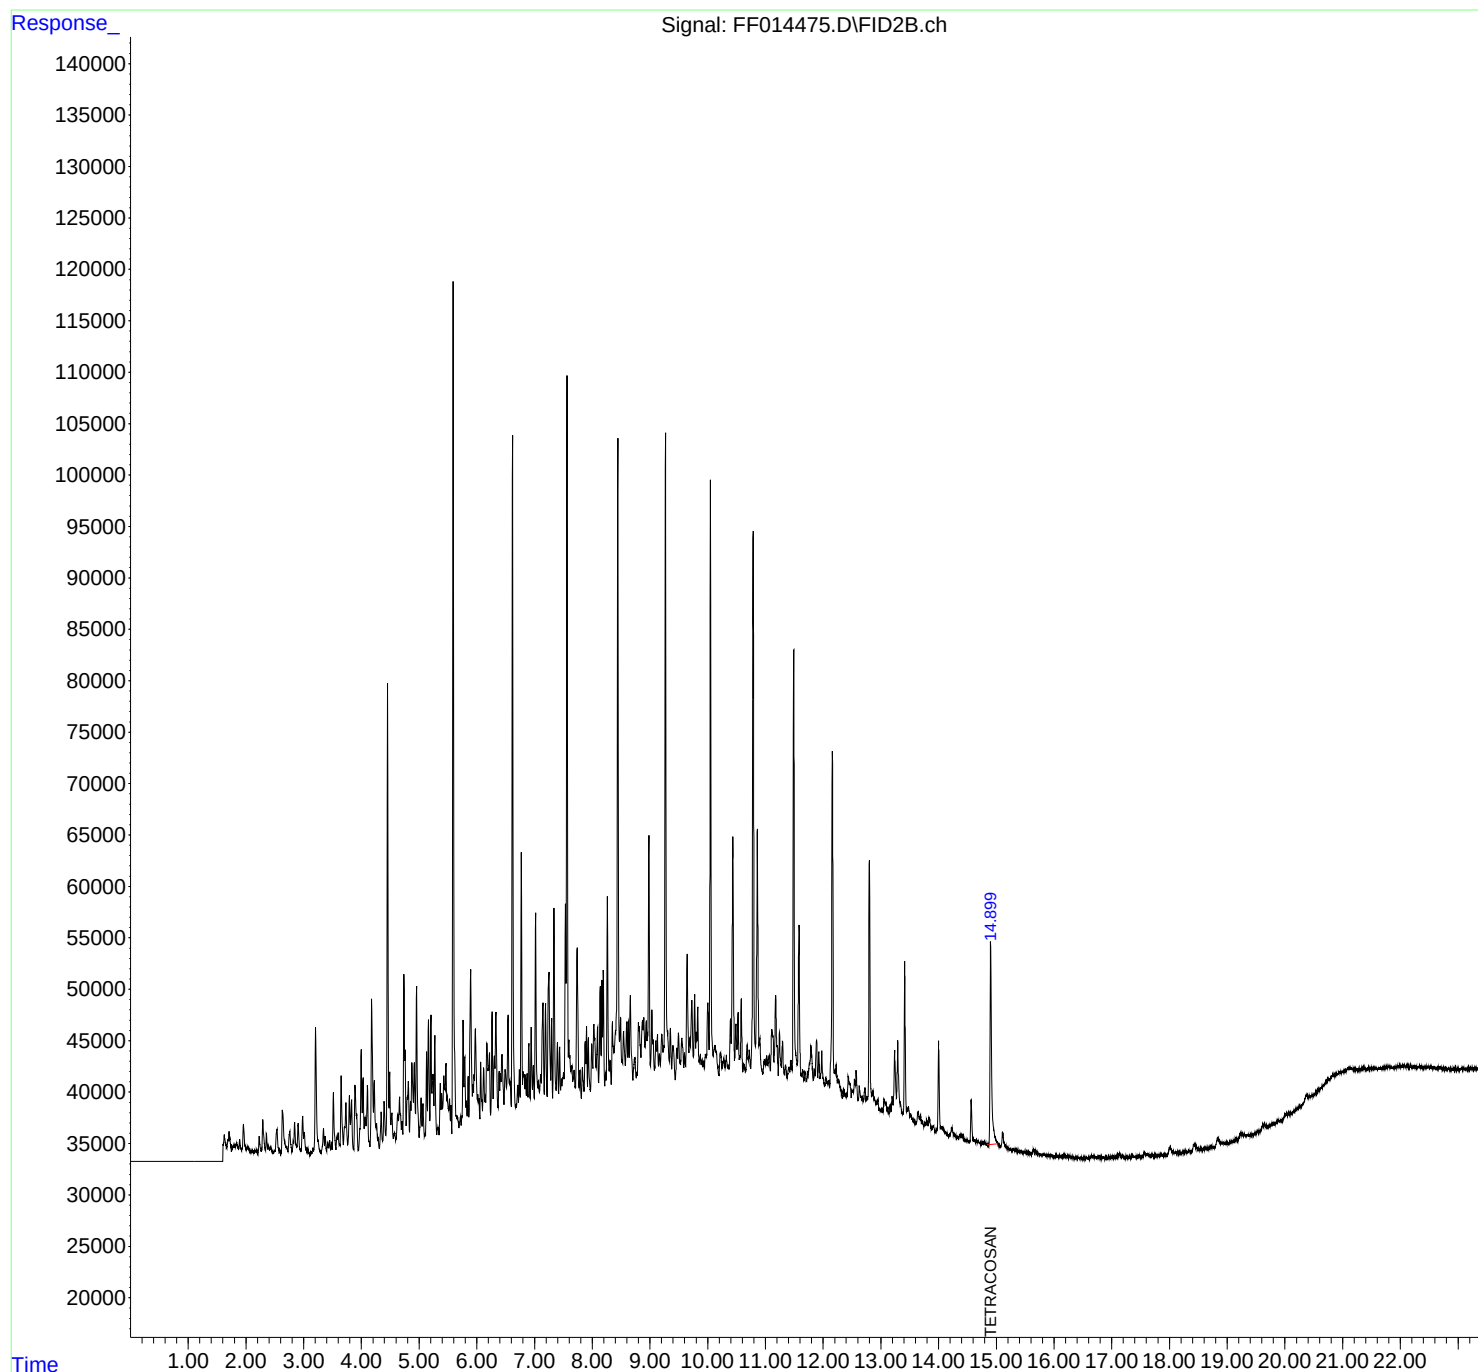

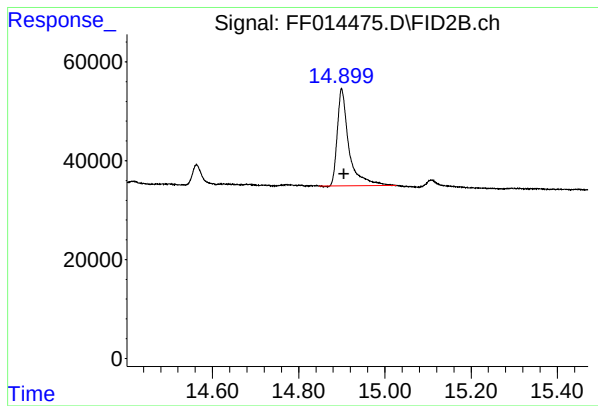

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.900 min
Delta R.T.: -0.005 min
Response: 369155
Conc: 3.13 ug/ml

Instrument :
FID_F
ClientSampleId :
RR-DIES-WP