

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
 Data File : FF014477.D
 Signal(s) : FID2B.ch
 Acq On : 10 Sep 2024 12:08
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Sep 11 01:31:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
 Quant Title :
 QLast Update : Fri Aug 16 11:11:51 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.900	5610528	47.534 ug/ml
Target Compounds			
2) N-DECANE	4.453	6073216	49.211 ug/ml
3) N-DODECANE	6.620	6173927	49.800 ug/ml
4) N-TETRADECANE	8.446	6242598	49.726 ug/ml
5) N-HEXADECANE	10.052	6304219	51.012 ug/ml
6) N-OCTADECANE	11.493	6473464	49.816 ug/ml
7) N-EICOSANE	12.803	6547542	48.503 ug/ml
8) N-DOCOSANE	14.001	6336890	48.166 ug/ml
10) N-TETRACOSANE	15.103	6276981	47.431 ug/ml
11) N-HEXACOSANE	16.123	6178677	47.098 ug/ml
12) N-OCTACOSANE	17.072	6038879	46.764 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091024\
Data File : FF014477.D
Signal(s) : FID2B.ch
Acq On : 10 Sep 2024 12:08
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Sep 11 01:31:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF081624.M
Quant Title :
QLast Update : Fri Aug 16 11:11:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

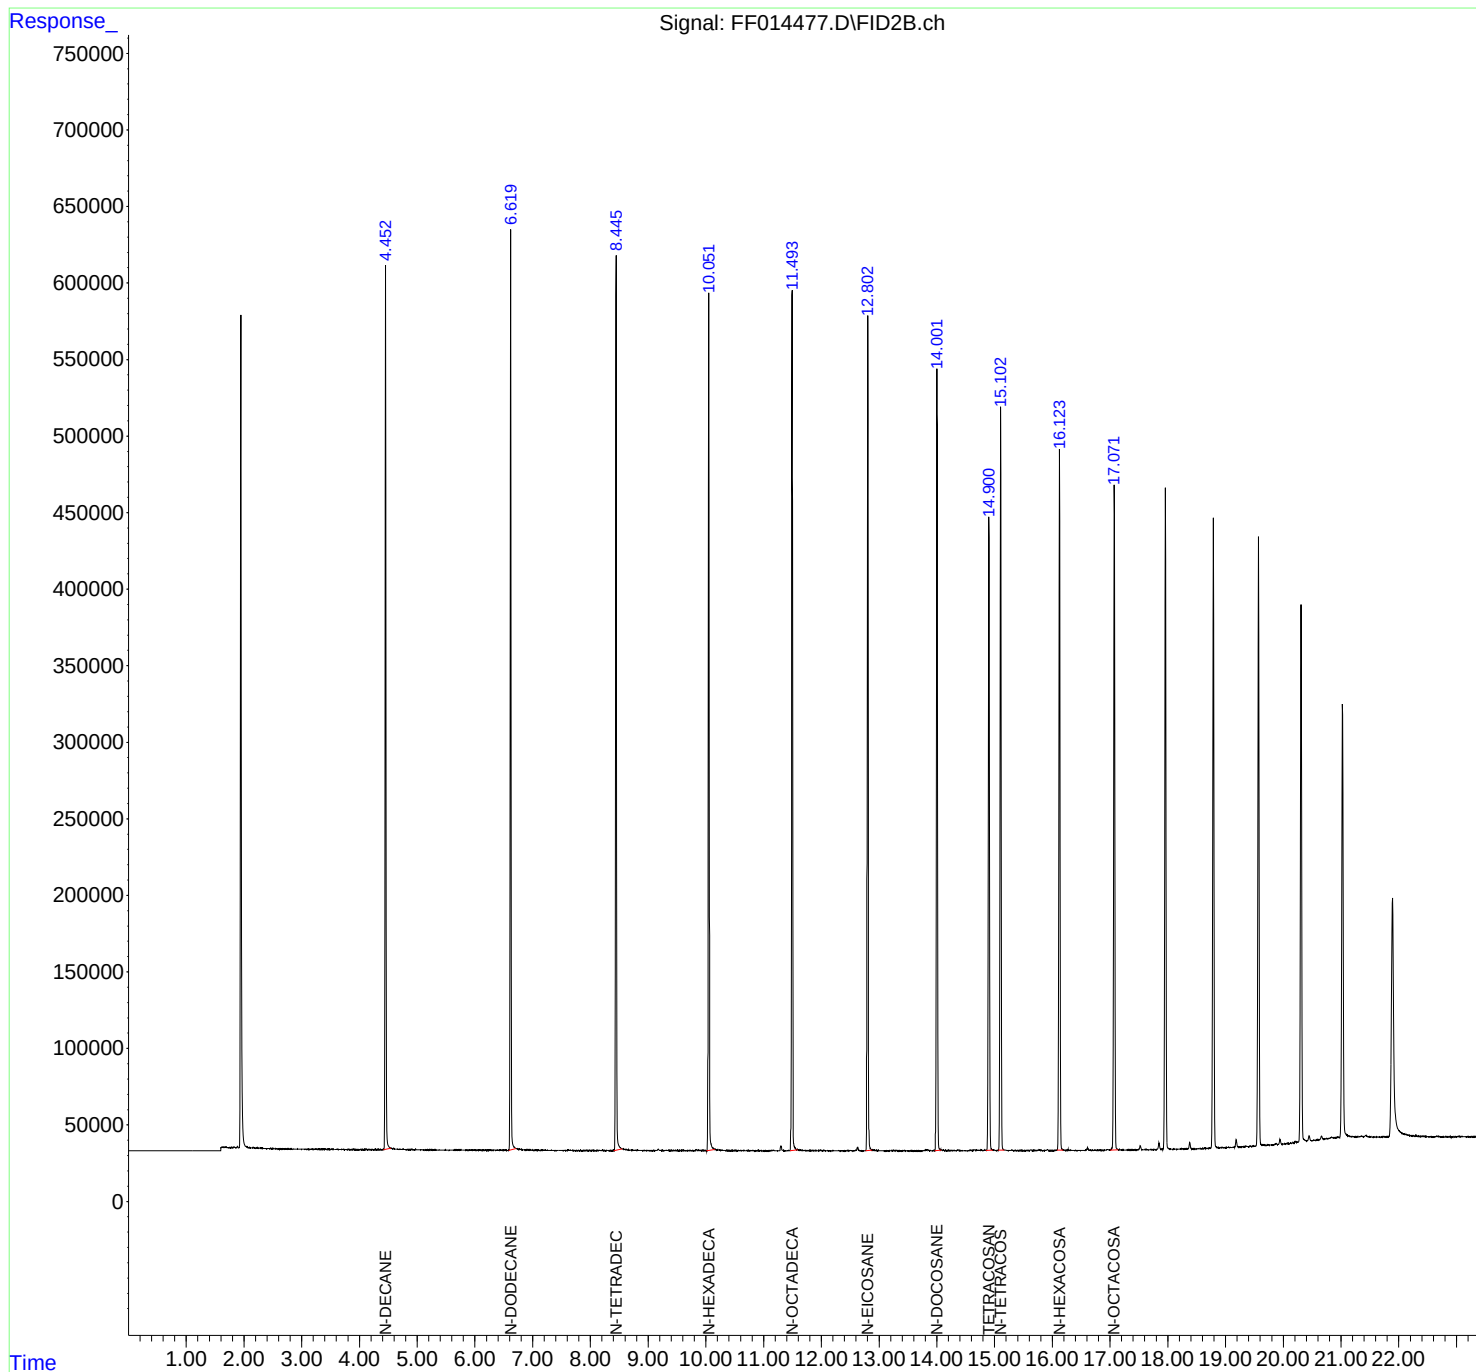


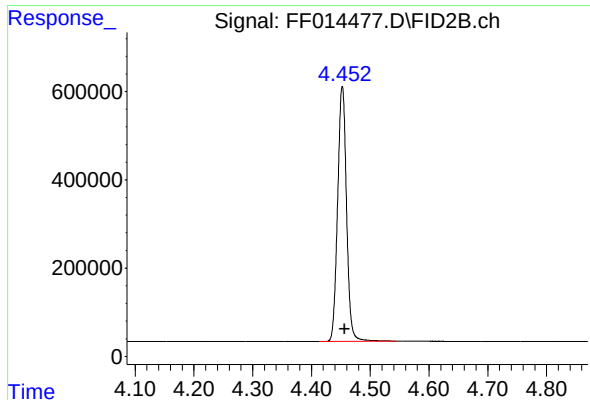

#2 N-DECANE


R.T.: 4.453 min
Delta R.T.: -0.004 min
Response: 6073216
Conc: 49.21 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

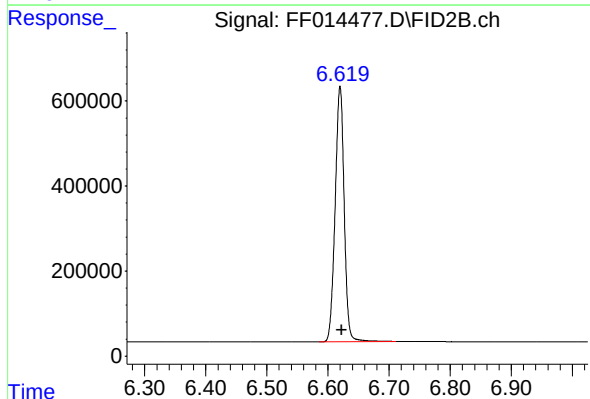


#3 N-DODECANE

R.T.: 6.620 min
Delta R.T.: -0.002 min
Response: 6173927
Conc: 49.80 ug/ml

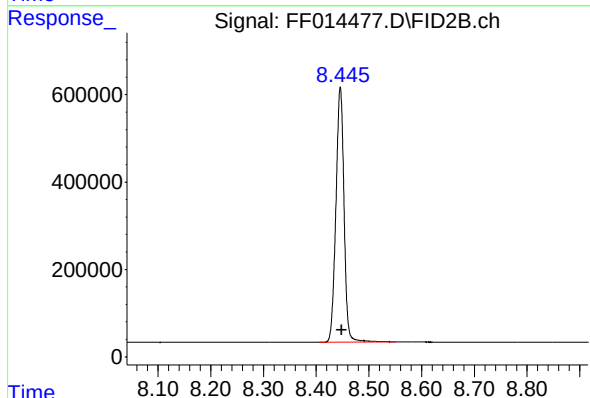


#4 N-TETRADECANE

R.T.: 8.446 min
Delta R.T.: -0.003 min
Response: 6242598
Conc: 49.73 ug/ml

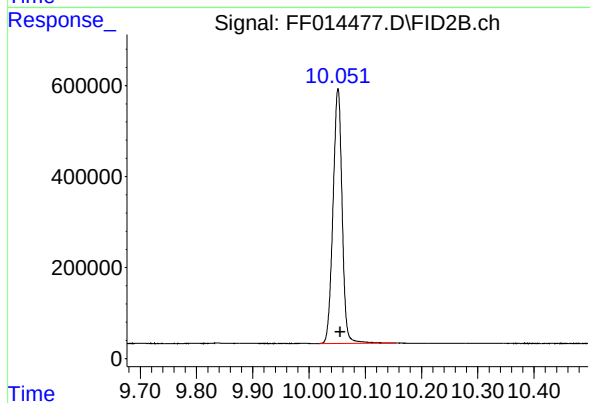

#5 N-HEXADECANE


R.T.: 10.052 min
Delta R.T.: -0.004 min
Response: 6304219
Conc: 51.01 ug/ml

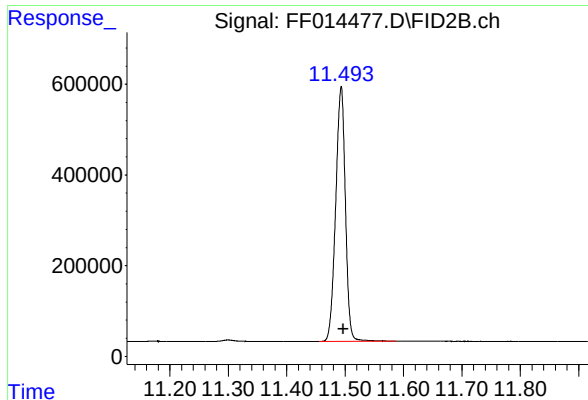

#6 N-OCTADECANE


R.T.: 11.493 min
Delta R.T.: -0.004 min
Response: 6473464
Conc: 49.82 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

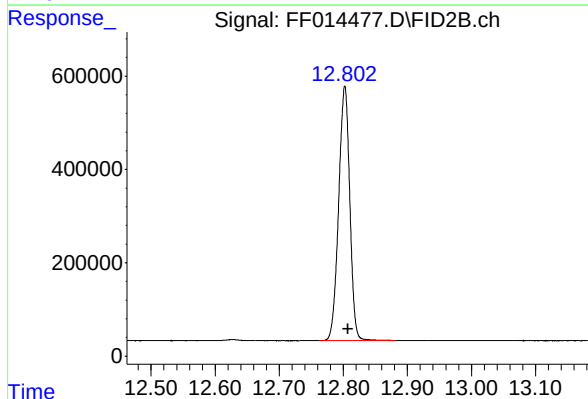


#7 N-EICOSANE

R.T.: 12.803 min
Delta R.T.: -0.005 min
Response: 6547542
Conc: 48.50 ug/ml

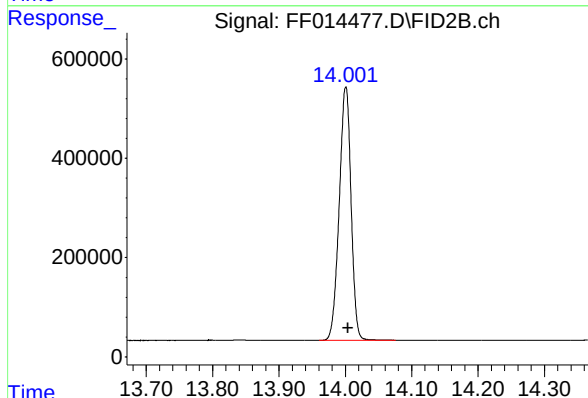


#8 N-DOCOSANE

R.T.: 14.001 min
Delta R.T.: -0.003 min
Response: 6336890
Conc: 48.17 ug/ml

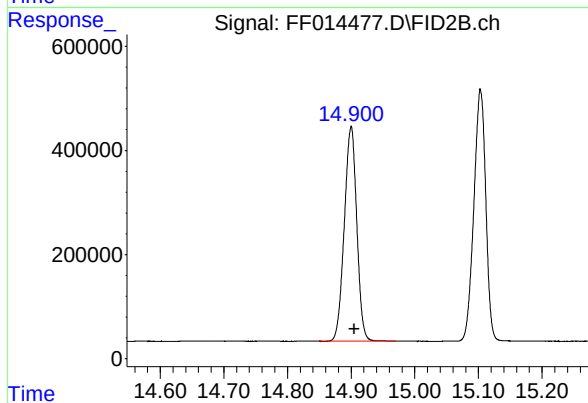

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.900 min
Delta R.T.: -0.005 min
Response: 5610528
Conc: 47.53 ug/ml

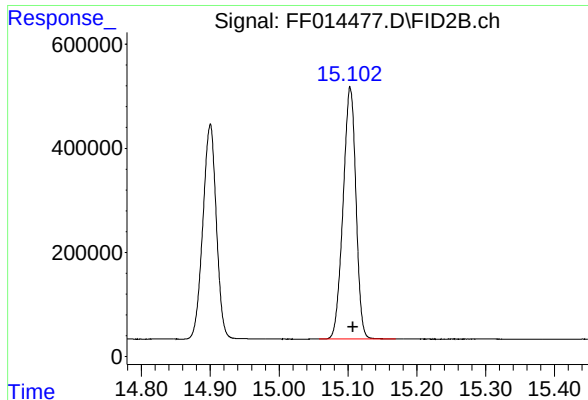

#10 N-TETRACOSANE


R.T.: 15.103 min
Delta R.T.: -0.004 min
Response: 6276981
Conc: 47.43 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

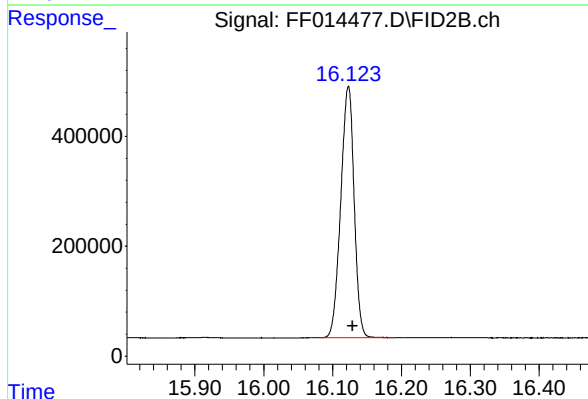

#11 N-HEXACOSANE

R.T.: 16.123 min
Delta R.T.: -0.006 min
Response: 6178677
Conc: 47.10 ug/ml

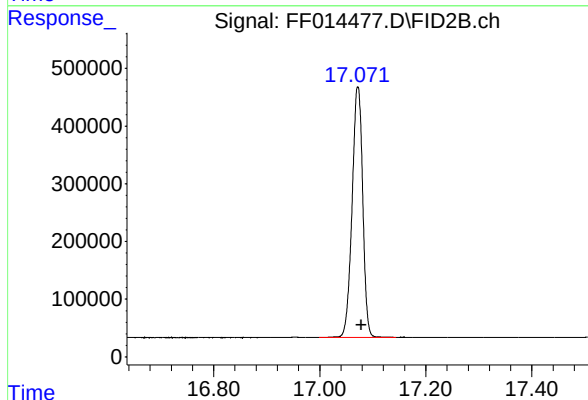

#12 N-OCTACOSANE

R.T.: 17.072 min
Delta R.T.: -0.007 min
Response: 6038879
Conc: 46.76 ug/ml