

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091120\
 Data File : FF007527.D
 Signal(s) : FID2B.ch
 Acq On : 11 Sep 2020 18:55
 Operator : DD\AJ
 Sample : L3975-04
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 12 00:13:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1743130	11.852 ug/ml
Target Compounds			
4) N-TETRADECANE	8.240	142491	0.866 ug/ml
7) N-EICOSANE	12.585f	116013	0.690 ug/ml
8) N-DOCOSANE	13.832	248432	1.508 ug/ml
10) N-TETRACOSANE	14.926	2538655	15.565 ug/ml
11) N-HEXACOSANE	15.920f	204839	1.296 ug/ml
12) N-OCTACOSANE	16.930	696345	4.537 ug/ml
13) N-TRIACONTANE	17.808	230354	1.559 ug/ml
14) N-DOTRIACONTANE	18.632	85941	0.619 ug/ml
15) N-TETRATRIACONTANE	19.495f	103291	0.818 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091120\
Data File : FF007527.D
Signal(s) : FID2B.ch
Acq On : 11 Sep 2020 18:55
Operator : DD\AJ
Sample : L3975-04
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 12 00:13:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

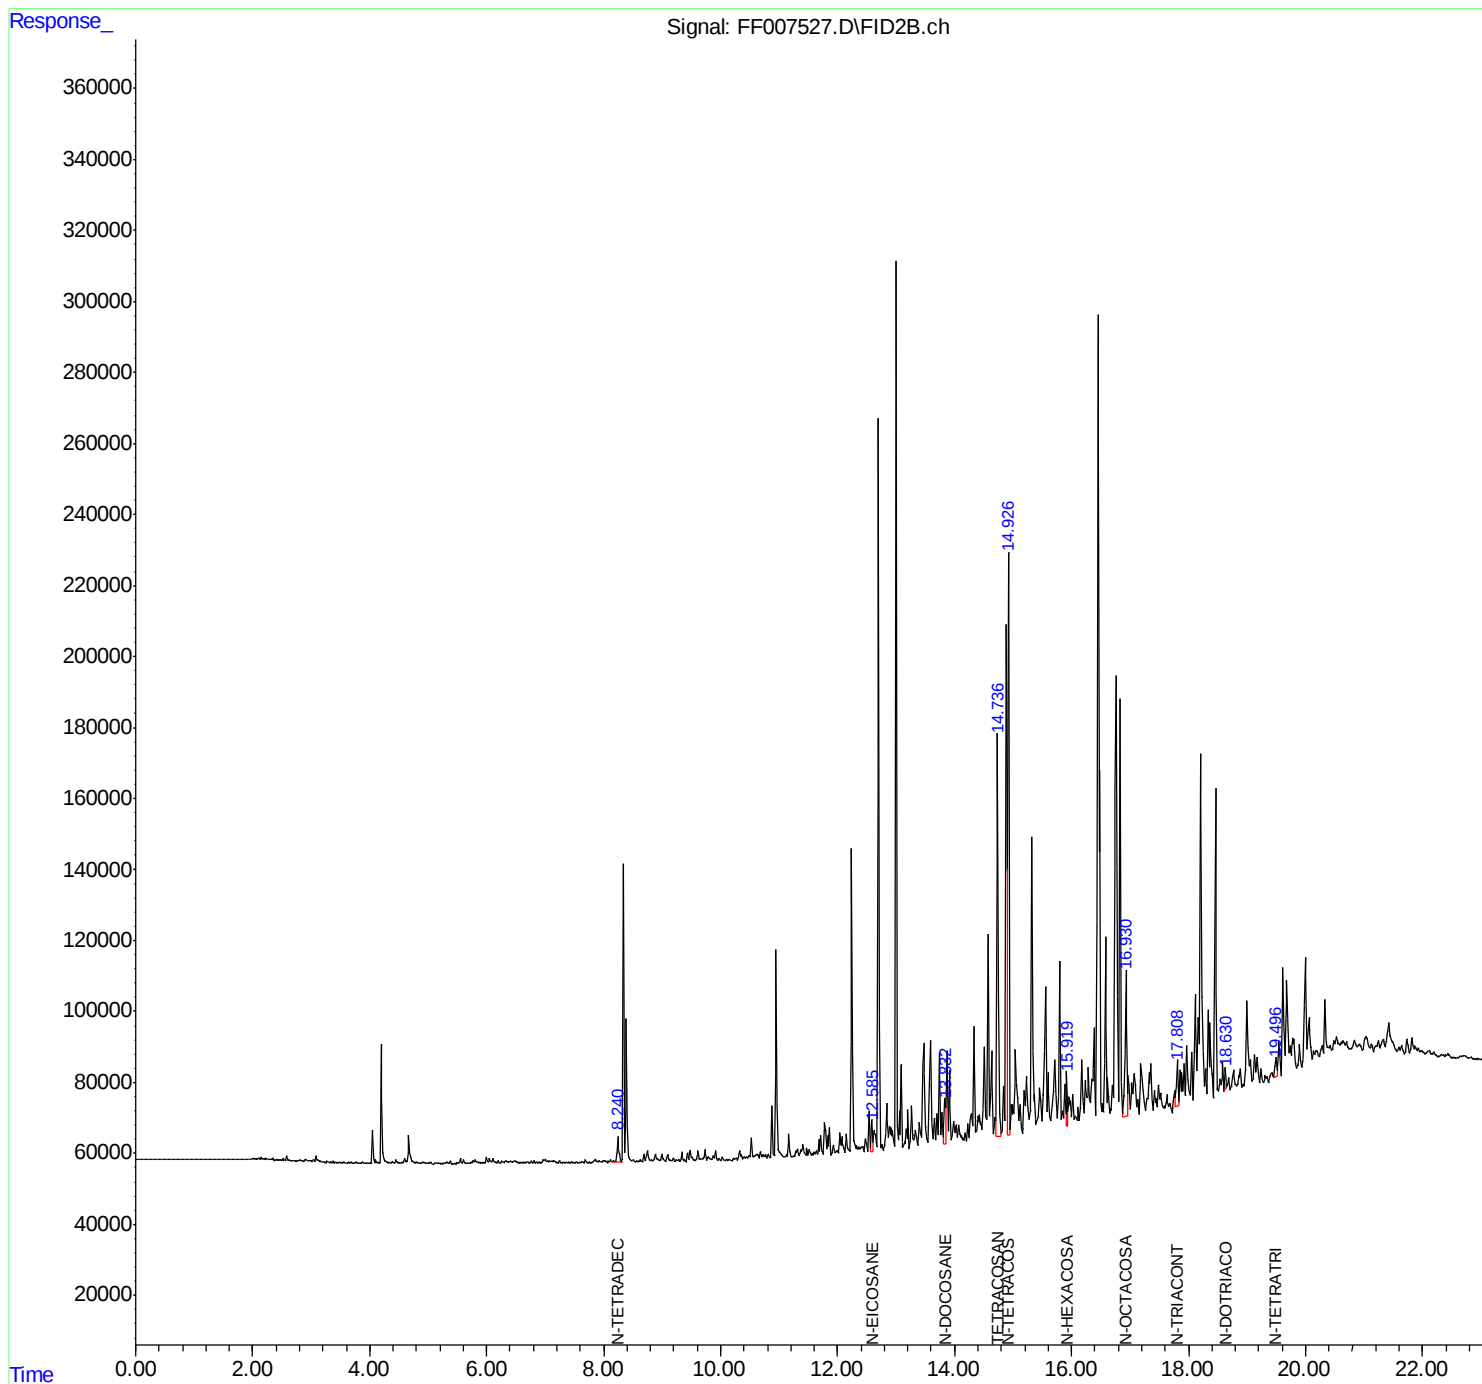

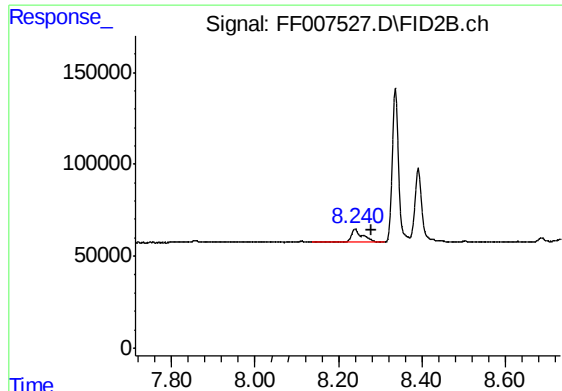


#4 N-TETRADECANE

R.T.: 8.240 min
Delta R.T.: -0.041 min
Response: 142491
Conc: 0.87 ug/ml

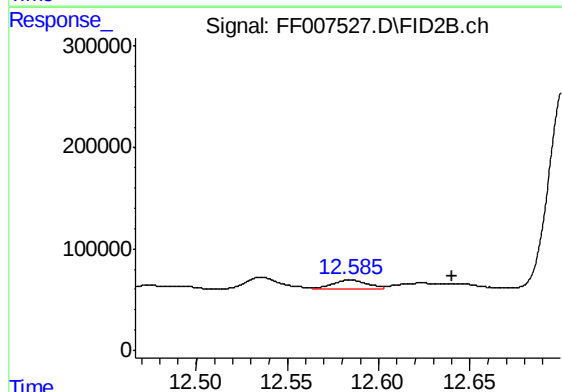


#7 N-EICOSANE

R.T.: 12.585 min
Delta R.T.: -0.056 min
Response: 116013
Conc: 0.69 ug/ml

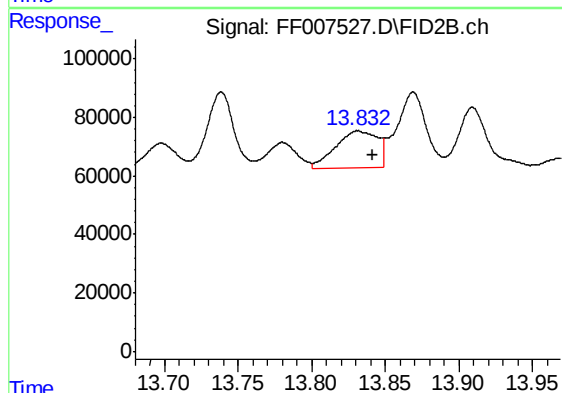


#8 N-DOCOSANE

R.T.: 13.832 min
Delta R.T.: -0.010 min
Response: 248432
Conc: 1.51 ug/ml

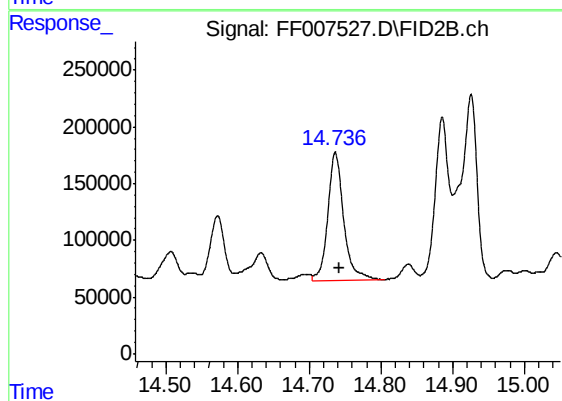


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.736 min
Delta R.T.: -0.007 min
Response: 1743130
Conc: 11.85 ug/ml

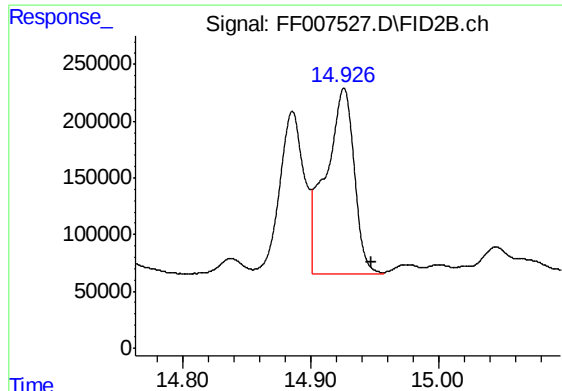


#10 N-TETRACOSANE

R.T.: 14.926 min
Delta R.T.: -0.022 min
Response: 2538655
Conc: 15.57 ug/ml

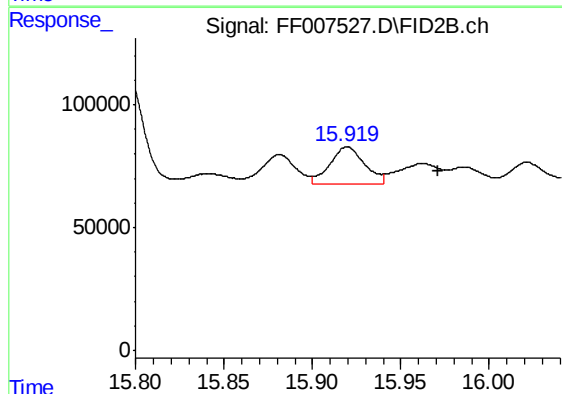


#11 N-HEXACOSANE

R.T.: 15.920 min
Delta R.T.: -0.052 min
Response: 204839
Conc: 1.30 ug/ml

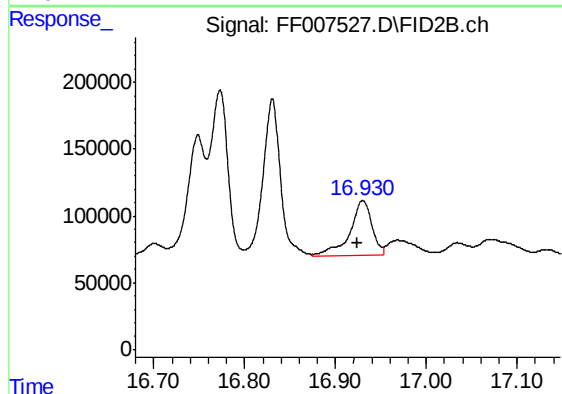


#12 N-OCTACOSANE

R.T.: 16.930 min
Delta R.T.: 0.007 min
Response: 696345
Conc: 4.54 ug/ml

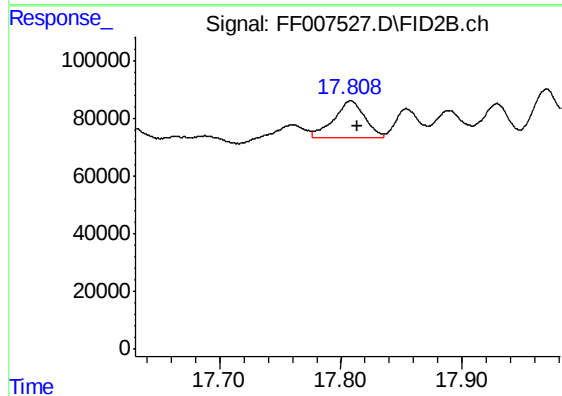


#13 N-TRIACONTANE

R.T.: 17.808 min
Delta R.T.: -0.005 min
Response: 230354
Conc: 1.56 ug/ml

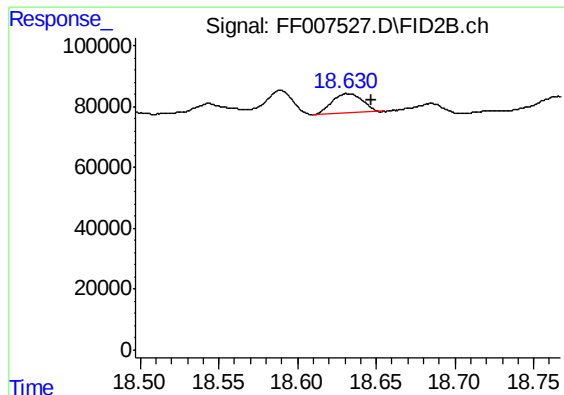

#14 N-DOTRIACONTANE

R.T.: 18.632 min
Delta R.T.: -0.015 min
Response: 85941
Conc: 0.62 ug/ml

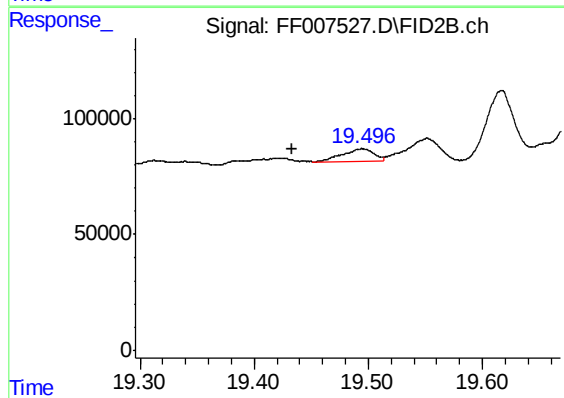

#15 N-TETRATRIACONTANE

R.T.: 19.495 min
Delta R.T.: 0.061 min
Response: 103291
Conc: 0.82 ug/ml