

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091120\
 Data File : FF007513.D
 Signal(s) : FID2B.ch
 Acq On : 11 Sep 2020 11:42
 Operator : DD\AJ
 Sample : L3939-03MS 2X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 12 00:09:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
 Quant Title :
 QLast Update : Wed Sep 02 11:29:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	1501384	10.208 ug/ml
Target Compounds			
2) N-DECANE	4.454	2102352	13.181 ug/ml
3) N-DODECANE	6.479	2177501	13.385 ug/ml
4) N-TETRADECANE	8.277	2189606	13.306 ug/ml
5) N-HEXADECANE	9.880	2183404	12.938 ug/ml
6) N-OCTADECANE	11.324	2187486	12.837 ug/ml
7) N-EICOSANE	12.637	2181814	12.977 ug/ml
8) N-DOCOSANE	13.838	2113361	12.827 ug/ml
10) N-TETRACOSANE	14.944	2248424	13.786 ug/ml
11) N-HEXACOSANE	15.968	1896314	11.996 ug/ml
12) N-OCTACOSANE	16.921	2026317	13.204 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091120\
Data File : FF007513.D
Signal(s) : FID2B.ch
Acq On : 11 Sep 2020 11:42
Operator : DD\AJ
Sample : L3939-03MS 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 12 00:09:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090120.M
Quant Title :
QLast Update : Wed Sep 02 11:29:30 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

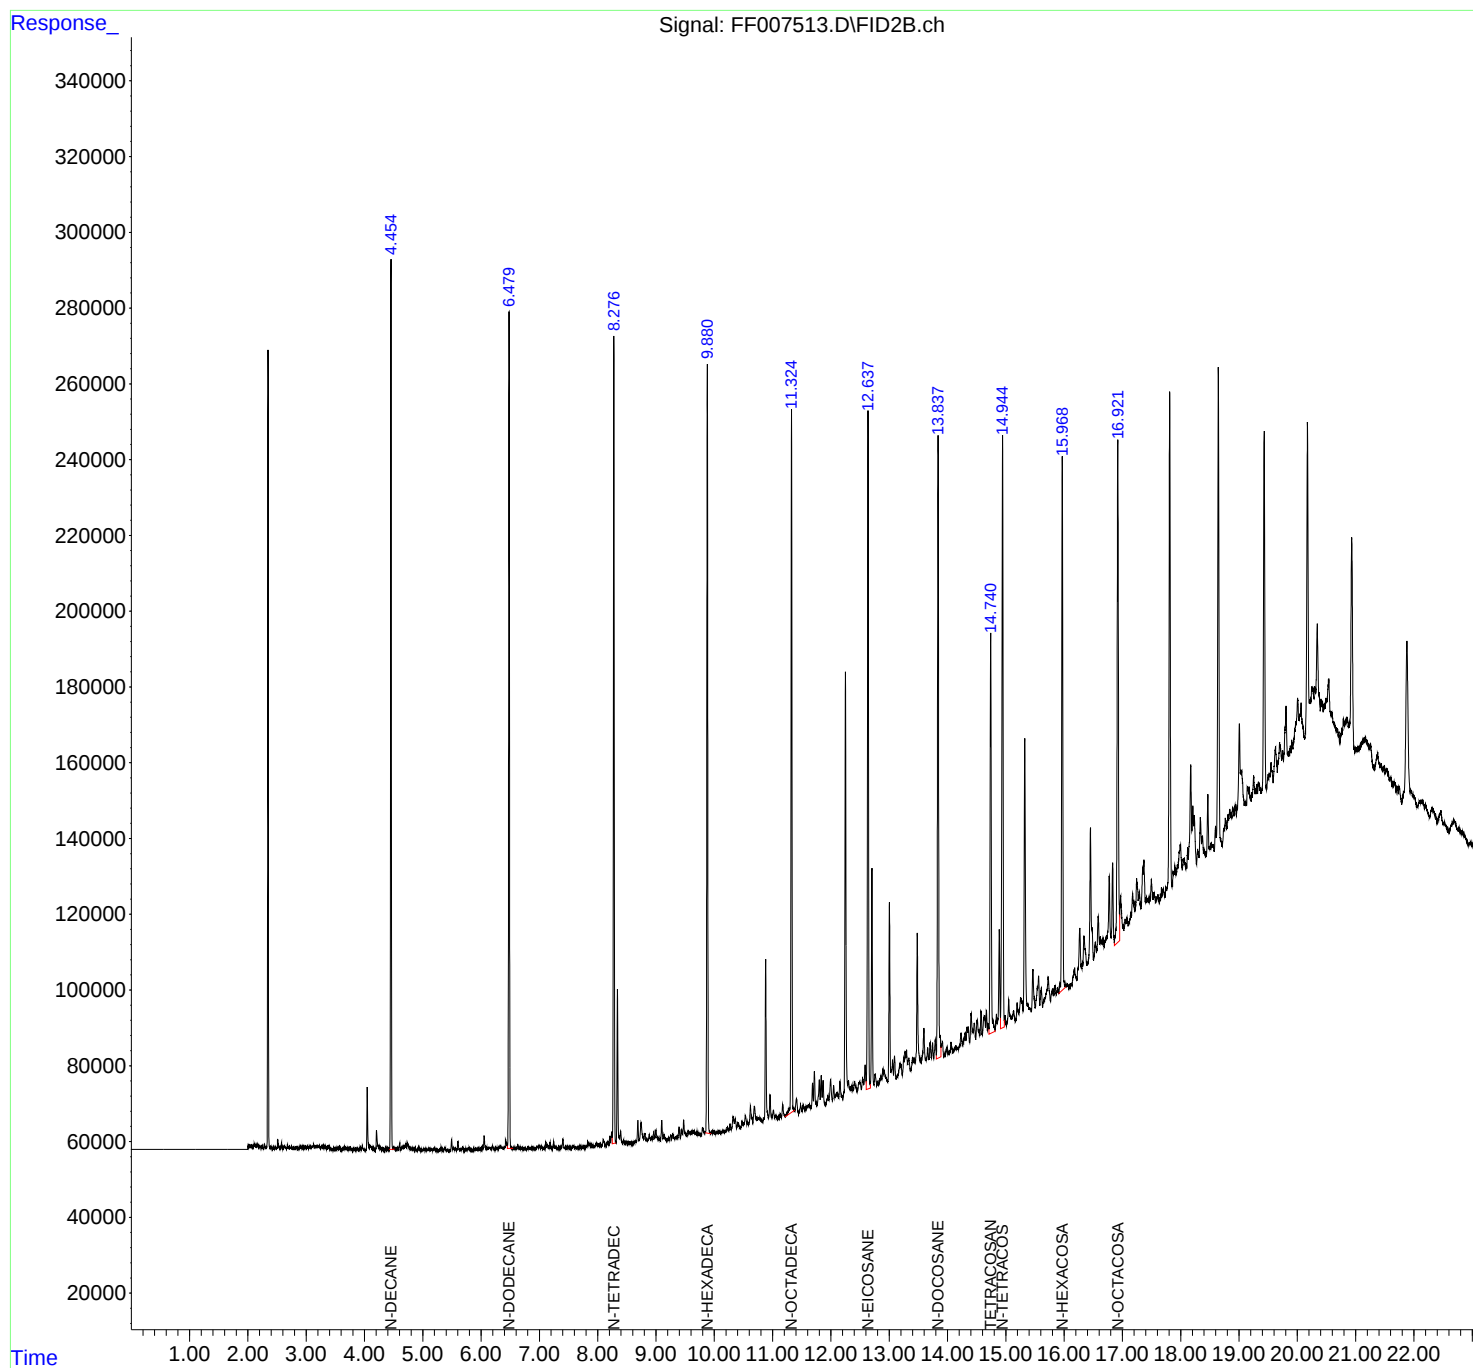

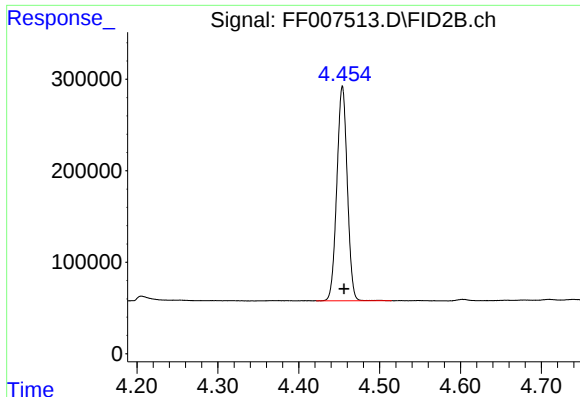


#2 N-DECANE

R.T.: 4.454 min
Delta R.T.: -0.002 min
Response: 2102352
Conc: 13.18 ug/ml

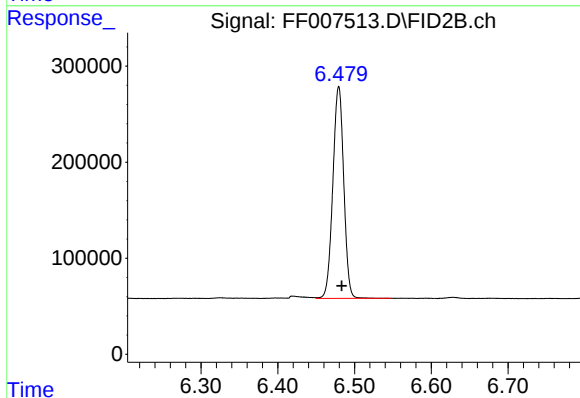


#3 N-DODECANE

R.T.: 6.479 min
Delta R.T.: -0.004 min
Response: 2177501
Conc: 13.38 ug/ml

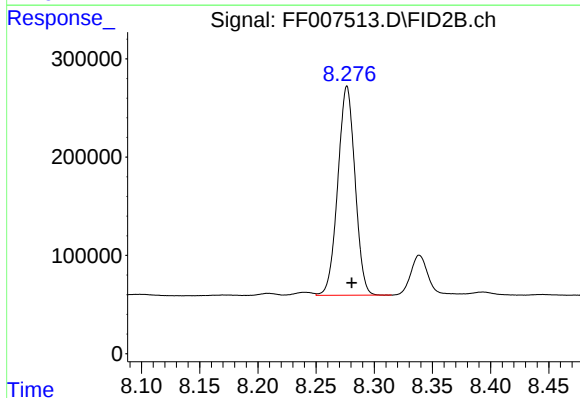


#4 N-TETRADECANE

R.T.: 8.277 min
Delta R.T.: -0.004 min
Response: 2189606
Conc: 13.31 ug/ml

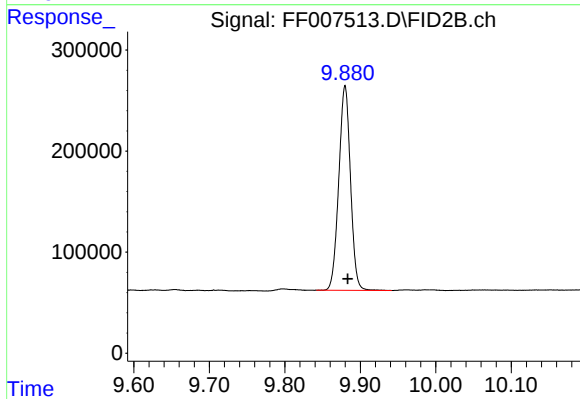


#5 N-HEXADECANE

R.T.: 9.880 min
Delta R.T.: -0.004 min
Response: 2183404
Conc: 12.94 ug/ml

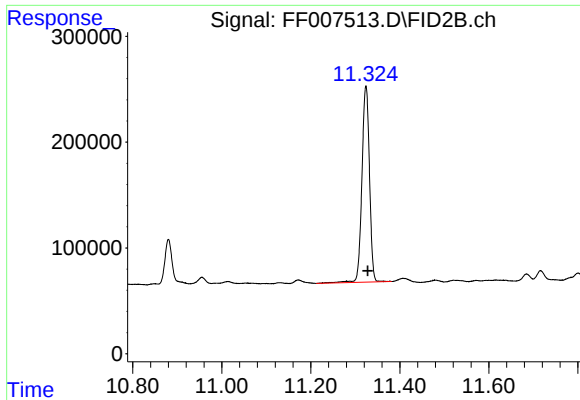


#6 N-OCTADECANE

R.T.: 11.324 min
Delta R.T.: -0.004 min
Response: 2187486
Conc: 12.84 ug/ml

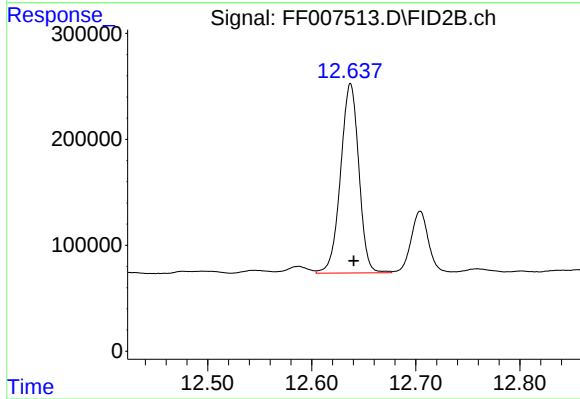


#7 N-EICOSANE

R.T.: 12.637 min
Delta R.T.: -0.003 min
Response: 2181814
Conc: 12.98 ug/ml

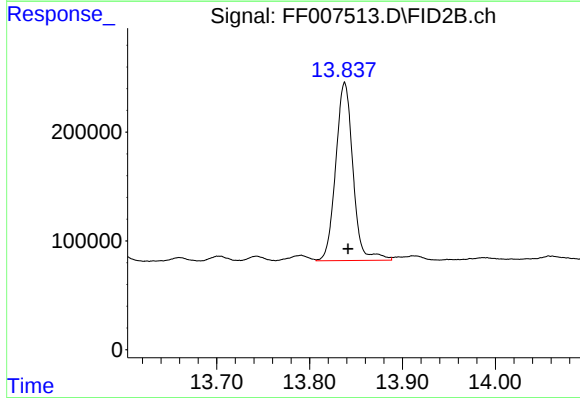


#8 N-DOCOSANE

R.T.: 13.838 min
Delta R.T.: -0.004 min
Response: 2113361
Conc: 12.83 ug/ml

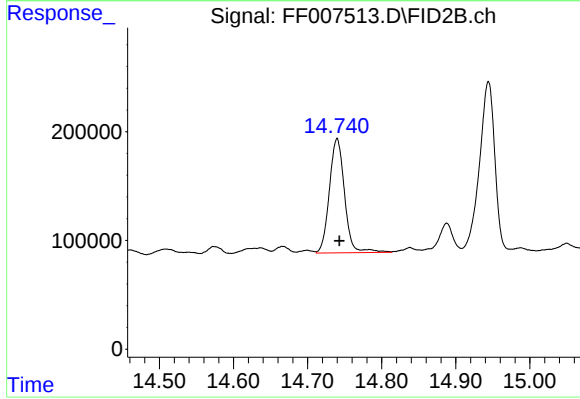


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.003 min
Response: 1501384
Conc: 10.21 ug/ml

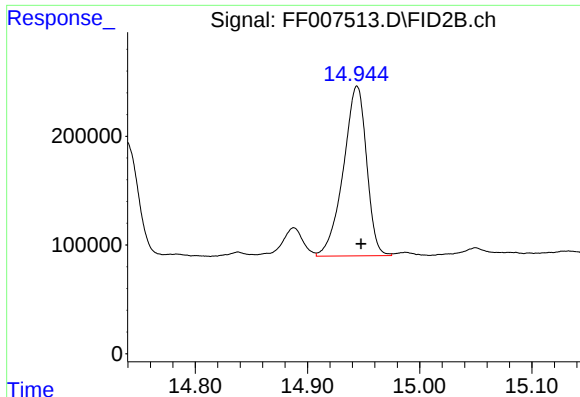


#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: -0.004 min
Response: 2248424
Conc: 13.79 ug/ml

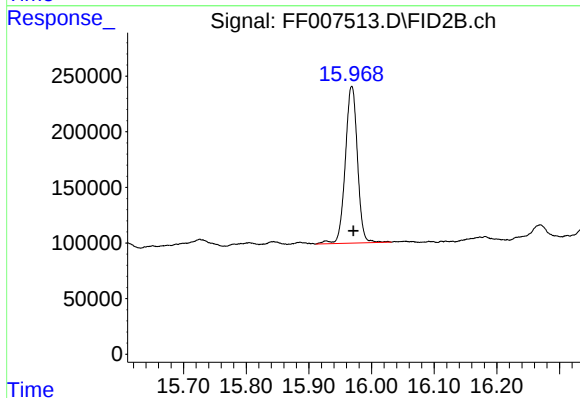

#11 N-HEXACOSANE

R.T.: 15.968 min
Delta R.T.: -0.003 min
Response: 1896314
Conc: 12.00 ug/ml

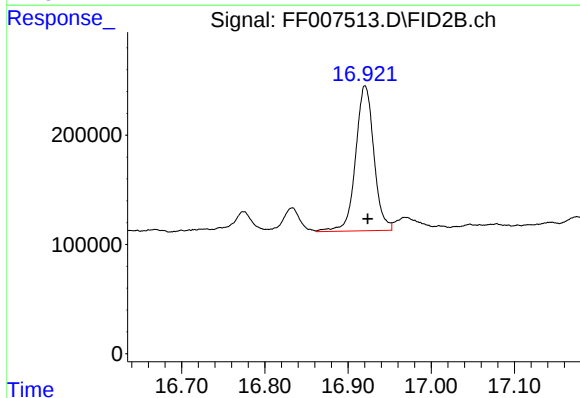

#12 N-OCTACOSANE

R.T.: 16.921 min
Delta R.T.: -0.003 min
Response: 2026317
Conc: 13.20 ug/ml