

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091219\
Data File : FF005531.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2019 15:57
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 13 02:22:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.359	2469707	17.229 ug/ml
12)	N-OCTACOSANE	16.805	2510050	21.035 ug/ml
13)	N-TRIACONTANE	17.698	122350	1.011 ug/ml
14)	N-DOTRIACONTANE	18.540	182278	1.470 ug/ml
15)	N-TETRATRIACONTANE	19.329	112243	0.931 ug/ml
16)	N-HEXATRIACONTANE	20.122	106893	0.891 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091219\
Data File : FF005531.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2019 15:57
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 13 02:22:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

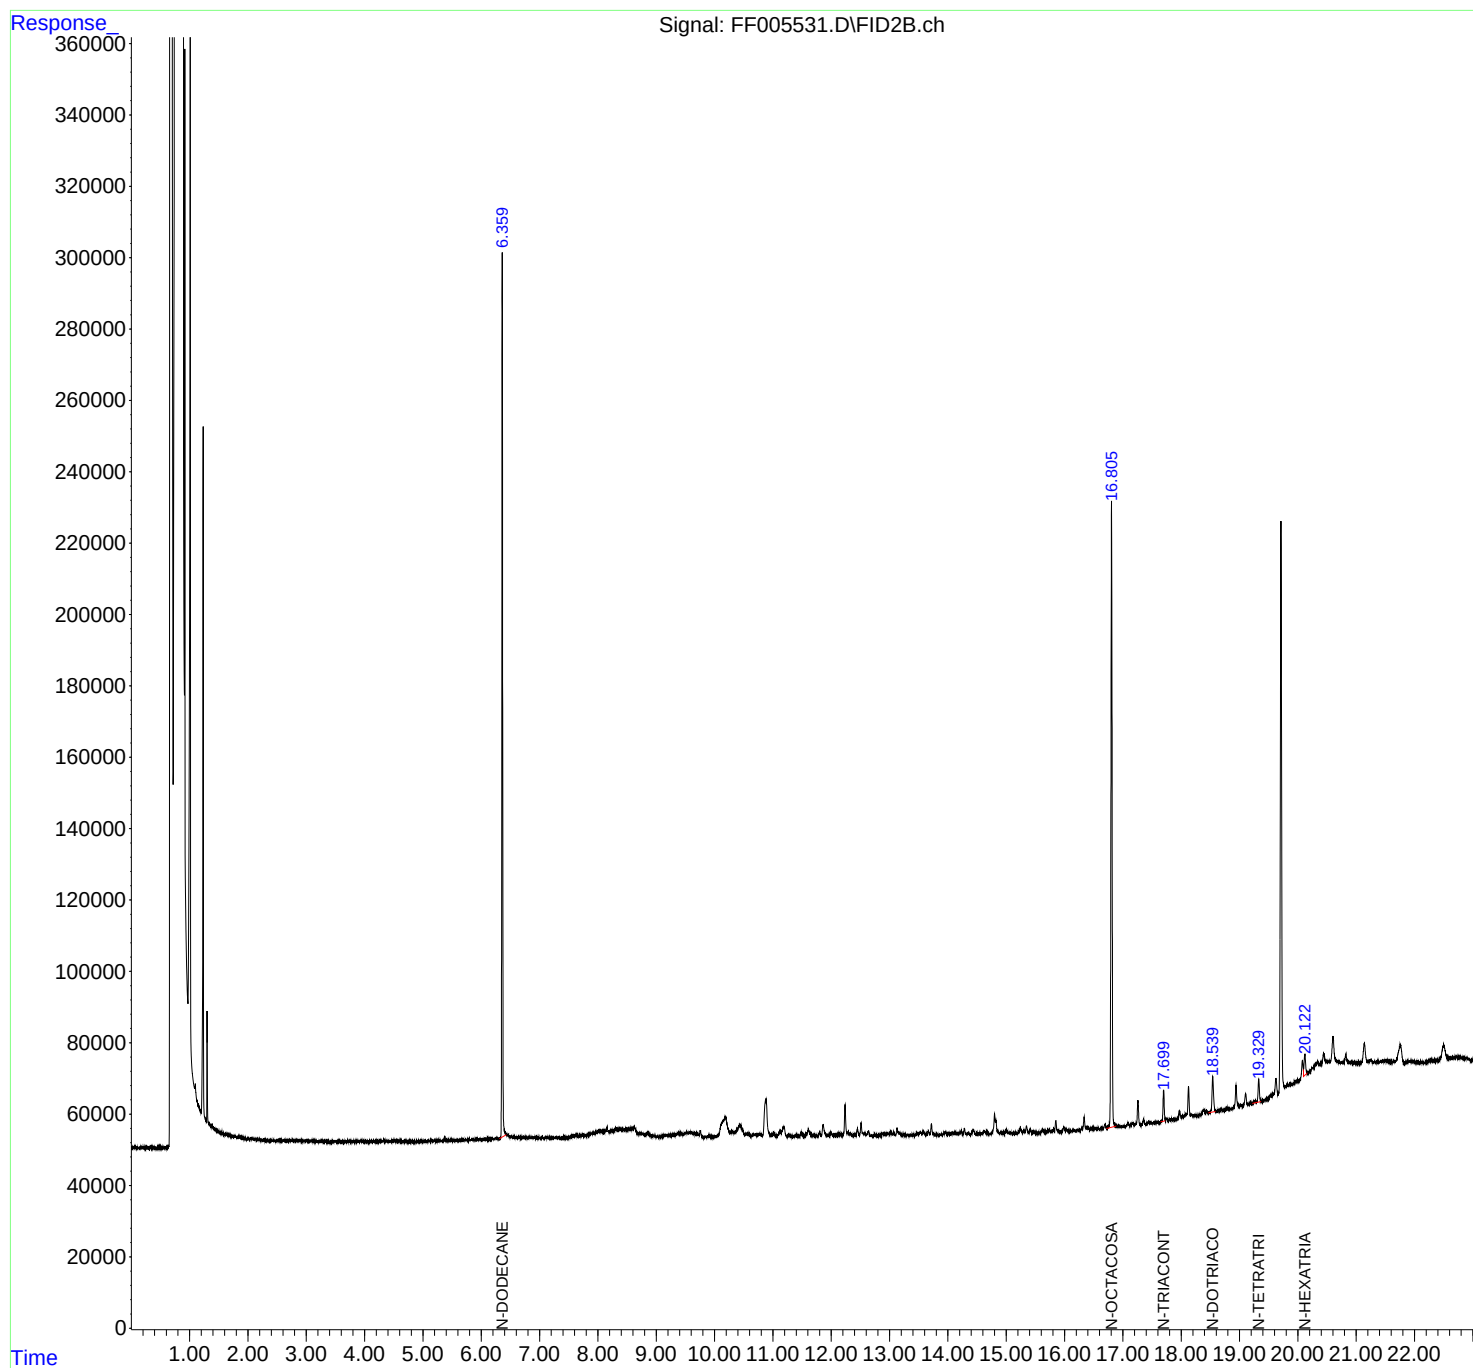


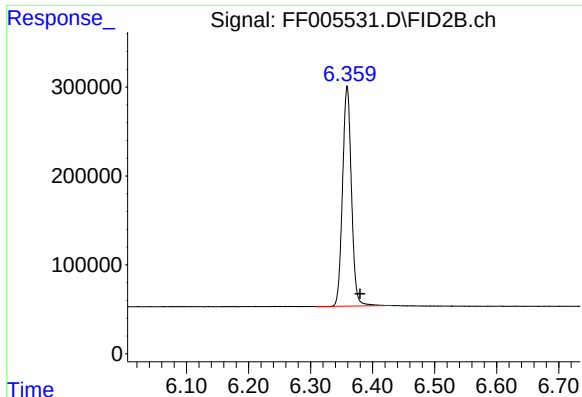

#3 N-DODECANE


R.T.: 6.359 min
Delta R.T.: -0.021 min
Response: 2469707
Conc: 17.23 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

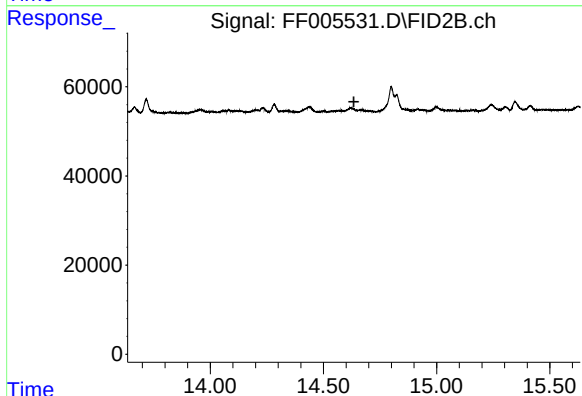


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.635 min
Response: 0
Conc: N.D.

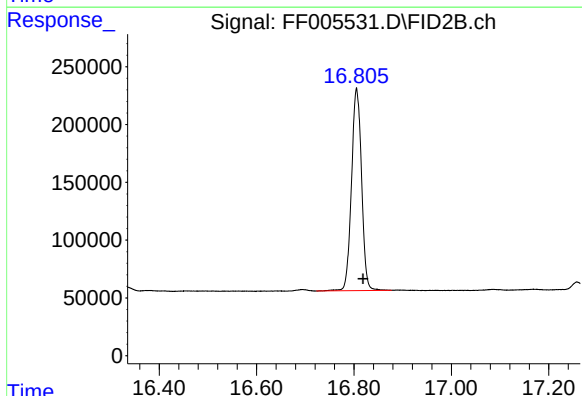


#12 N-OCTACOSANE

R.T.: 16.805 min
Delta R.T.: -0.014 min
Response: 2510050
Conc: 21.04 ug/ml

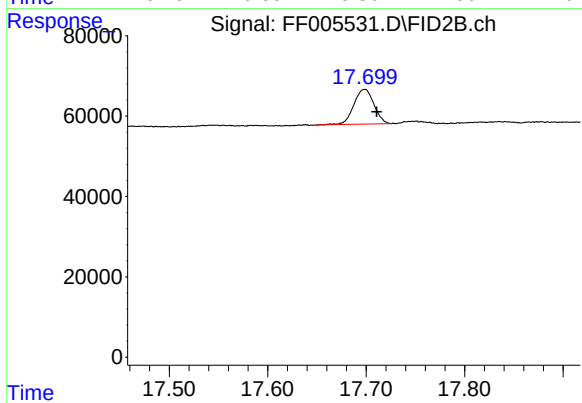

#13 N-TRIACONTANE


R.T.: 17.698 min
Delta R.T.: -0.012 min
Response: 122350
Conc: 1.01 ug/ml

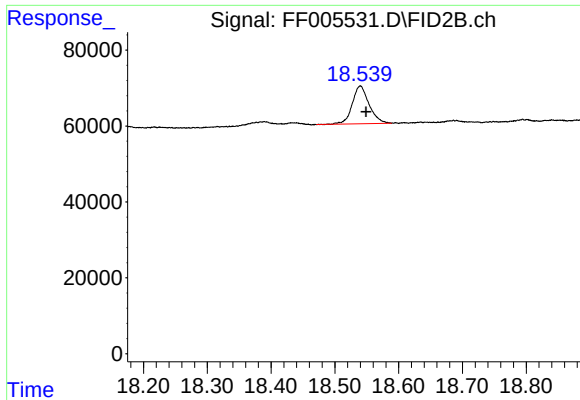

#14 N-DOTRIACONTANE


R.T.: 18.540 min
Delta R.T.: -0.009 min
Response: 182278
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

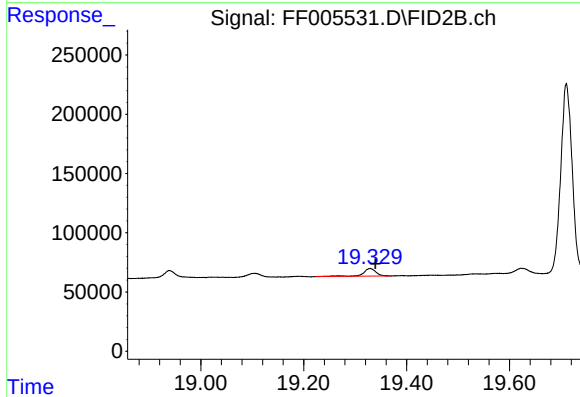

#15 N-TETRATRIACONTANE

R.T.: 19.329 min
Delta R.T.: -0.011 min
Response: 112243
Conc: 0.93 ug/ml

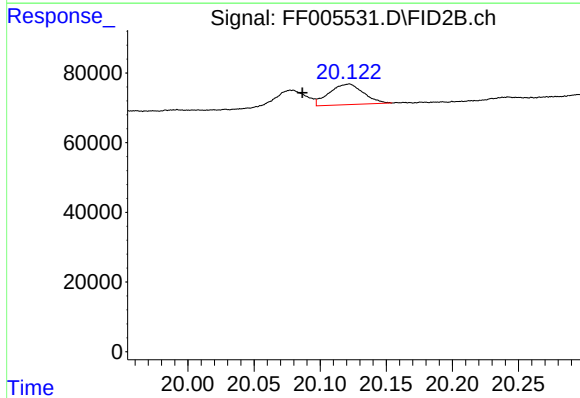

#16 N-HEXATRIACONTANE

R.T.: 20.122 min
Delta R.T.: 0.035 min
Response: 106893
Conc: 0.89 ug/ml