

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091219\
Data File : FF005539.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2019 19:55
Operator : DD\AJ
Sample : K4850-02 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AOC-7-(6)

Integration File: autoint1.e
Quant Time: Sep 13 02:25:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.642	1778485	16.620 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091219\
Data File : FF005539.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2019 19:55
Operator : DD\AJ
Sample : K4850-02 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AOC-7-(6)

Integration File: autoint1.e
Quant Time: Sep 13 02:25:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF090319.M
Quant Title :
QLast Update : Wed Sep 04 03:16:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

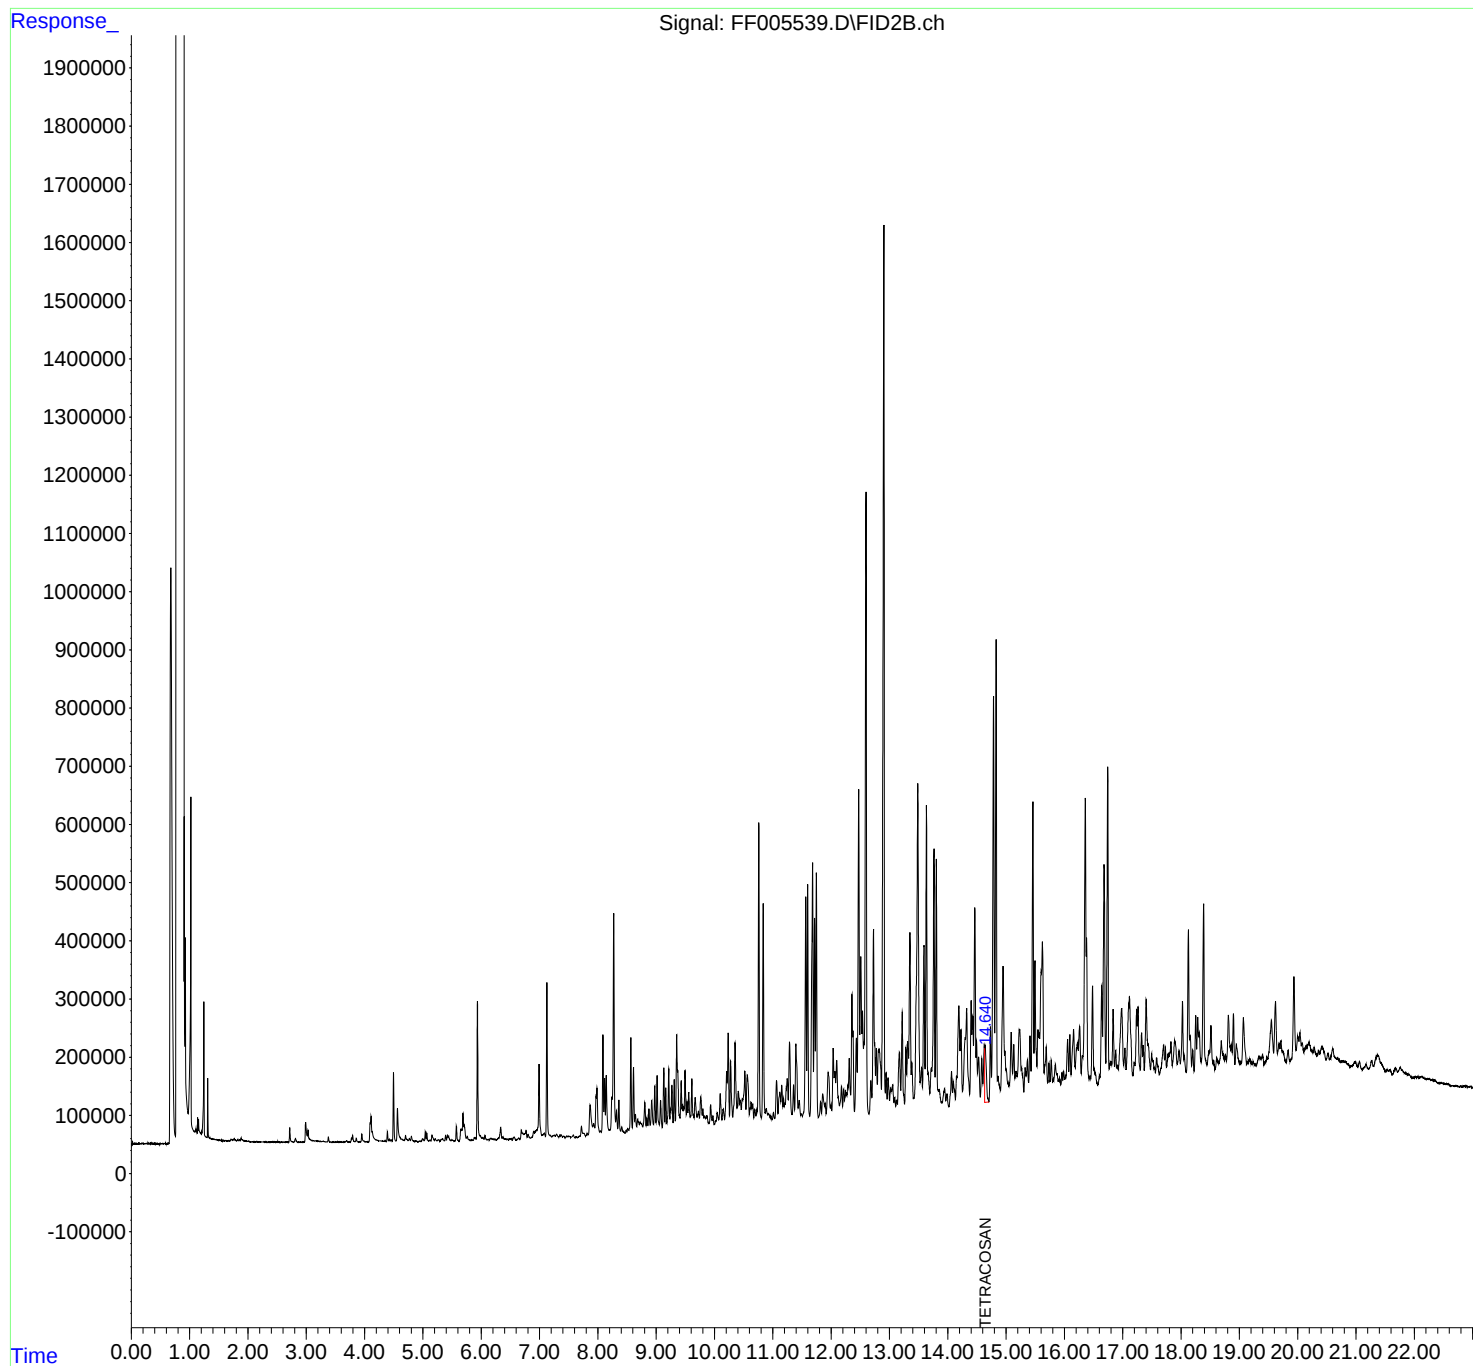

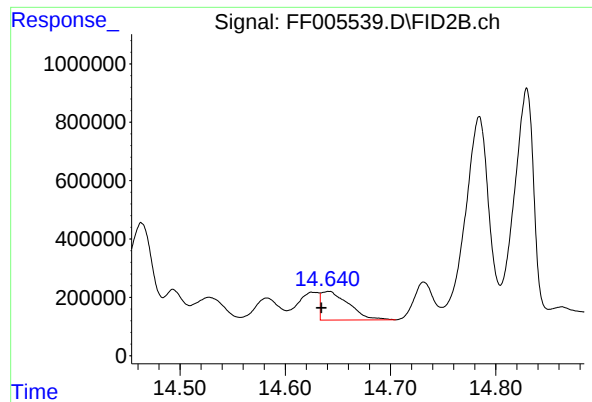

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.642 min
Delta R.T.: 0.007 min
Response: 1778485
Conc: 16.62 ug/ml

Instrument :
FID_F
ClientSampleId :
AOC-7-(6)