

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
 Data File : FF013484.D
 Signal(s) : FID2B.ch
 Acq On : 12 Sep 2023 07:48
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 13 01:47:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
 Quant Title :
 QLast Update : Fri Sep 01 02:22:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
8) N-DOCOSANE	14.064	103755	0.774 ug/ml
10) N-TETRACOSANE	15.172	98434	0.737 ug/ml
11) N-HEXACOSANE	16.195	63518	0.485 ug/ml
12) N-OCTACOSANE	17.145	57624	0.447 ug/ml
13) N-TRIACONTANE	18.033	69015	0.552 ug/ml
14) N-DOTRIACONTANE	18.881	186946	1.618 ug/ml
15) N-TETRATRIACONTANE	19.648	69390	0.674 ug/ml
16) N-HEXATRIACONTANE	20.385	62524	0.637 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013484.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 07:48
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 01:47:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

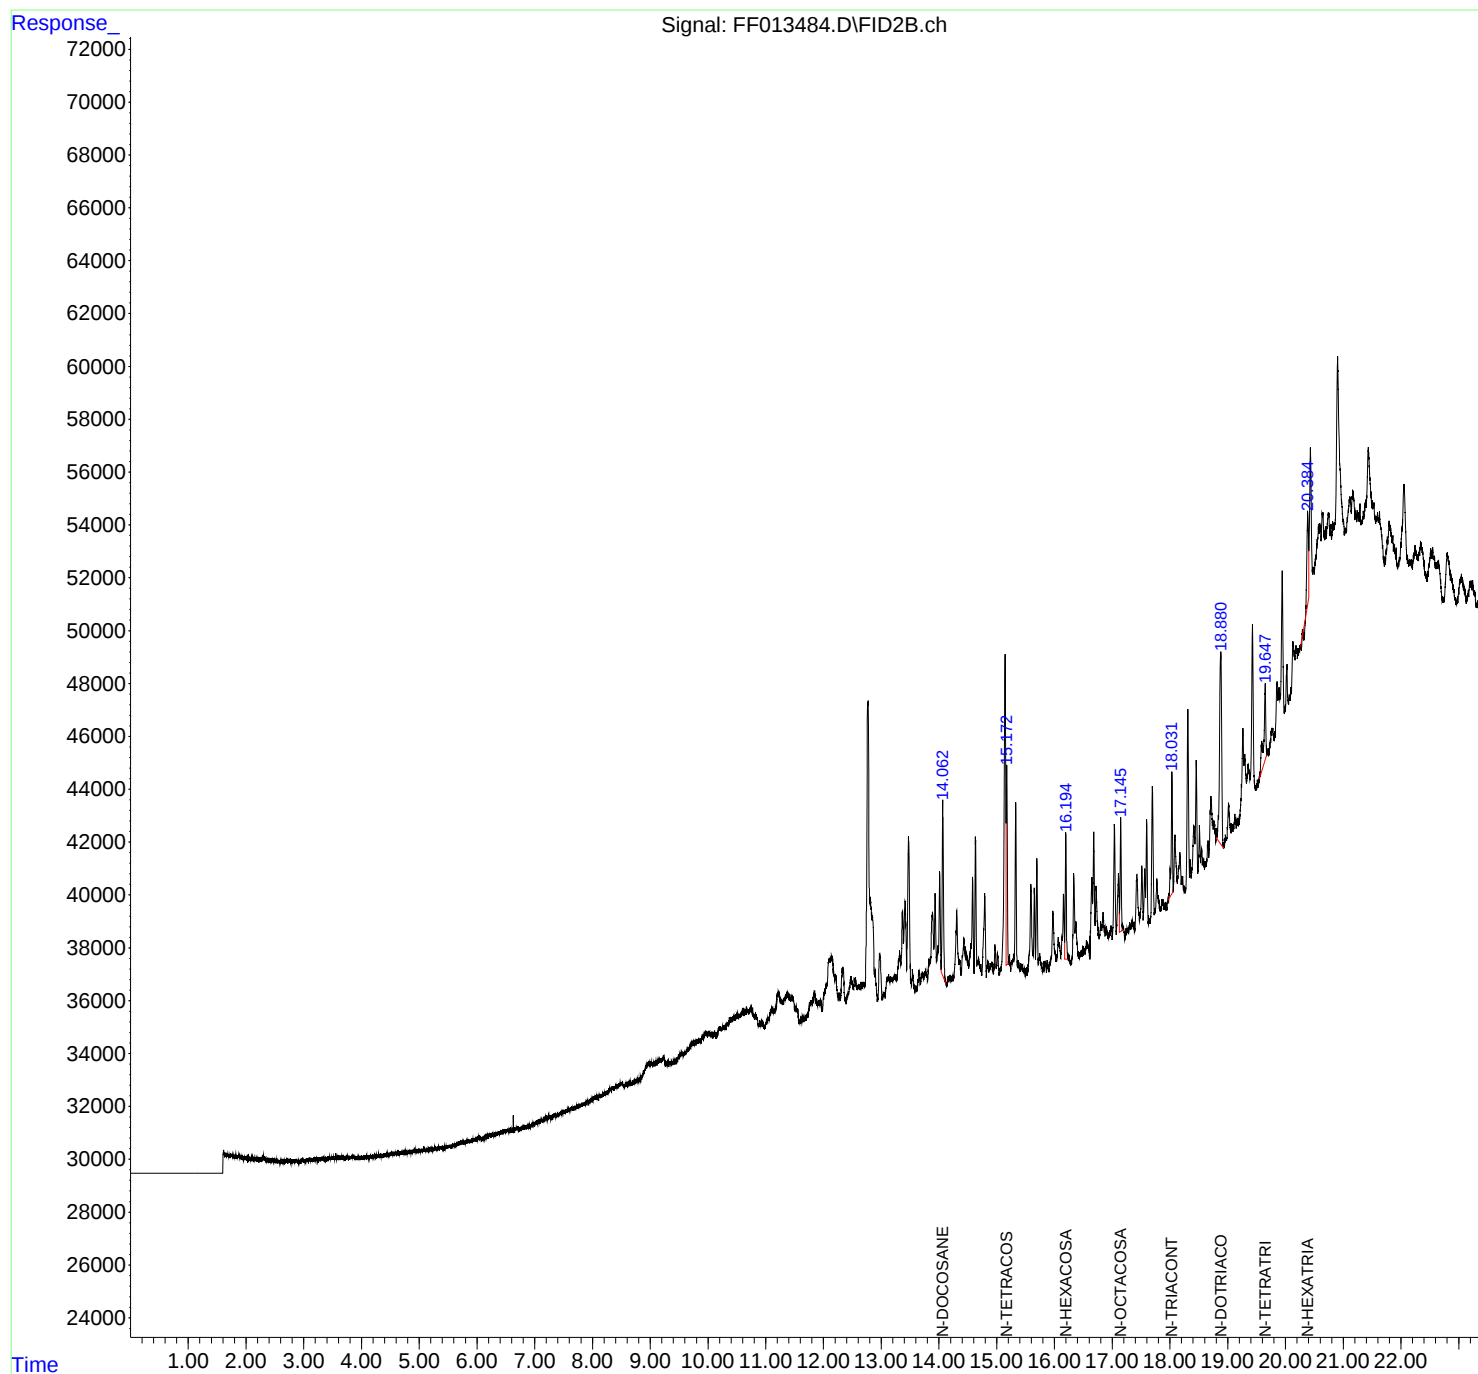


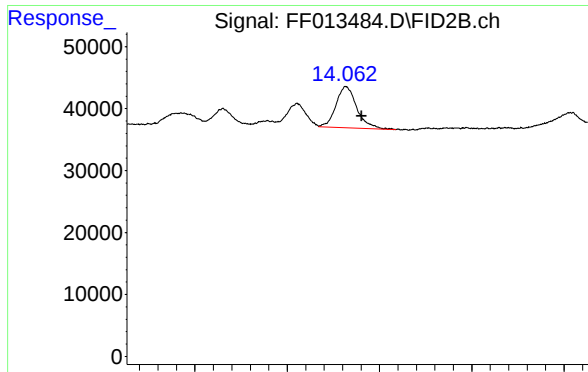

#8 N-DOCOSANE


R.T.: 14.064 min
Delta R.T.: -0.017 min
Response: 103755
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :

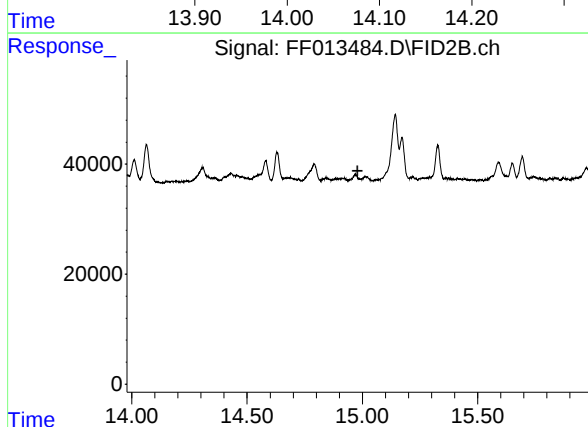


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.979 min
Response: 0
Conc: N.D.

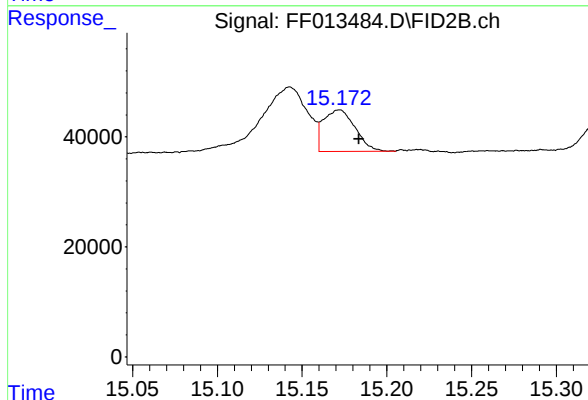


#10 N-TETRACOSANE

R.T.: 15.172 min
Delta R.T.: -0.012 min
Response: 98434
Conc: 0.74 ug/ml

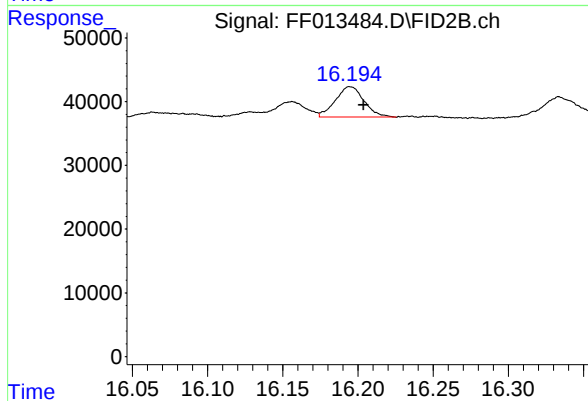

#11 N-HEXACOSANE


R.T.: 16.195 min
Delta R.T.: -0.009 min
Response: 63518
Conc: 0.48 ug/ml

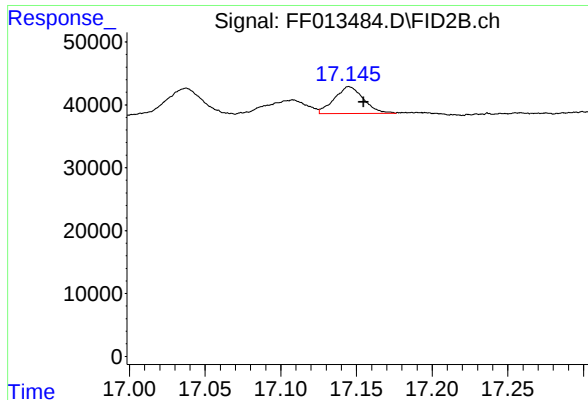

#12 N-OCTACOSANE


R.T.: 17.145 min
Delta R.T.: -0.009 min
Response: 57624
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :

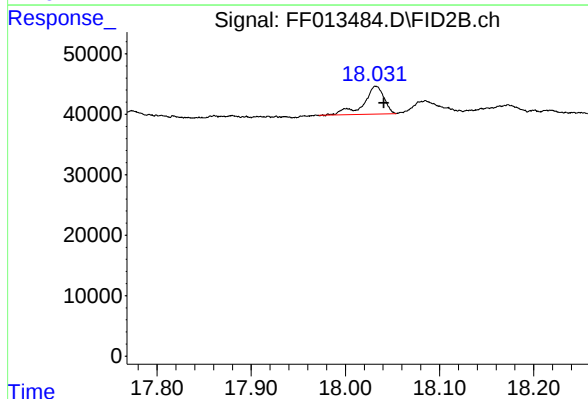


#13 N-TRIACONTANE

R.T.: 18.033 min
Delta R.T.: -0.008 min
Response: 69015
Conc: 0.55 ug/ml

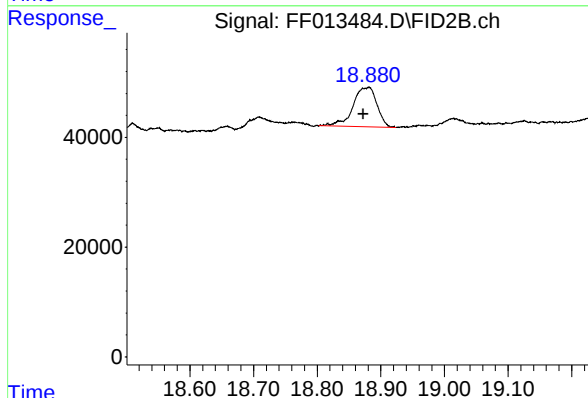


#14 N-DOTRIACONTANE

R.T.: 18.881 min
Delta R.T.: 0.009 min
Response: 186946
Conc: 1.62 ug/ml

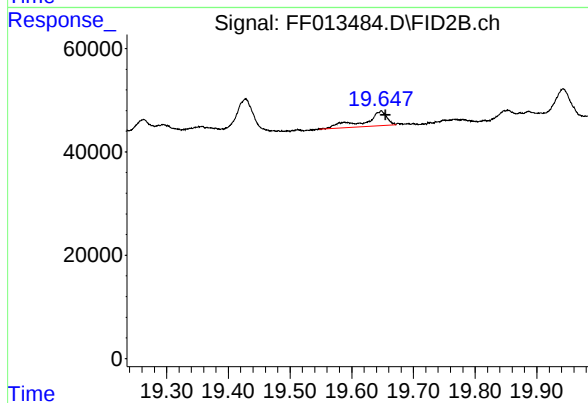

#15 N-TETRATRIACONTANE

R.T.: 19.648 min
Delta R.T.: -0.007 min
Response: 69390
Conc: 0.67 ug/ml

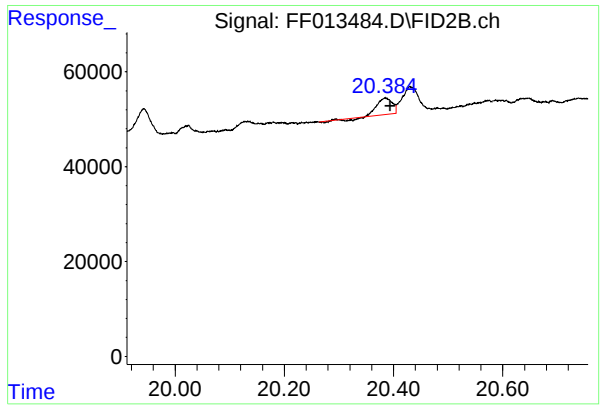

#16 N-HEXATRIACONTANE

R.T.: 20.385 min
Delta R.T.: -0.010 min
Response: 62524
Conc: 0.64 ug/ml

Instrument :

FID_F

ClientSampleId :