

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013487.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 09:46
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 01:48:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.693	2495497	18.708 ug/ml
12) N-OCTACOSANE	17.147	2400483	18.631 ug/ml
14) N-DOTRIACONTANE	18.865	59313	0.513 ug/ml
15) N-TETRATRIACONTANE	19.647	47375	0.460 ug/ml
16) N-HEXATRIACONTANE	20.384	77051	0.785 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF091223\
Data File : FF013487.D
Signal(s) : FID2B.ch
Acq On : 12 Sep 2023 09:46
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 13 01:48:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF083123.M
Quant Title :
QLast Update : Fri Sep 01 02:22:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

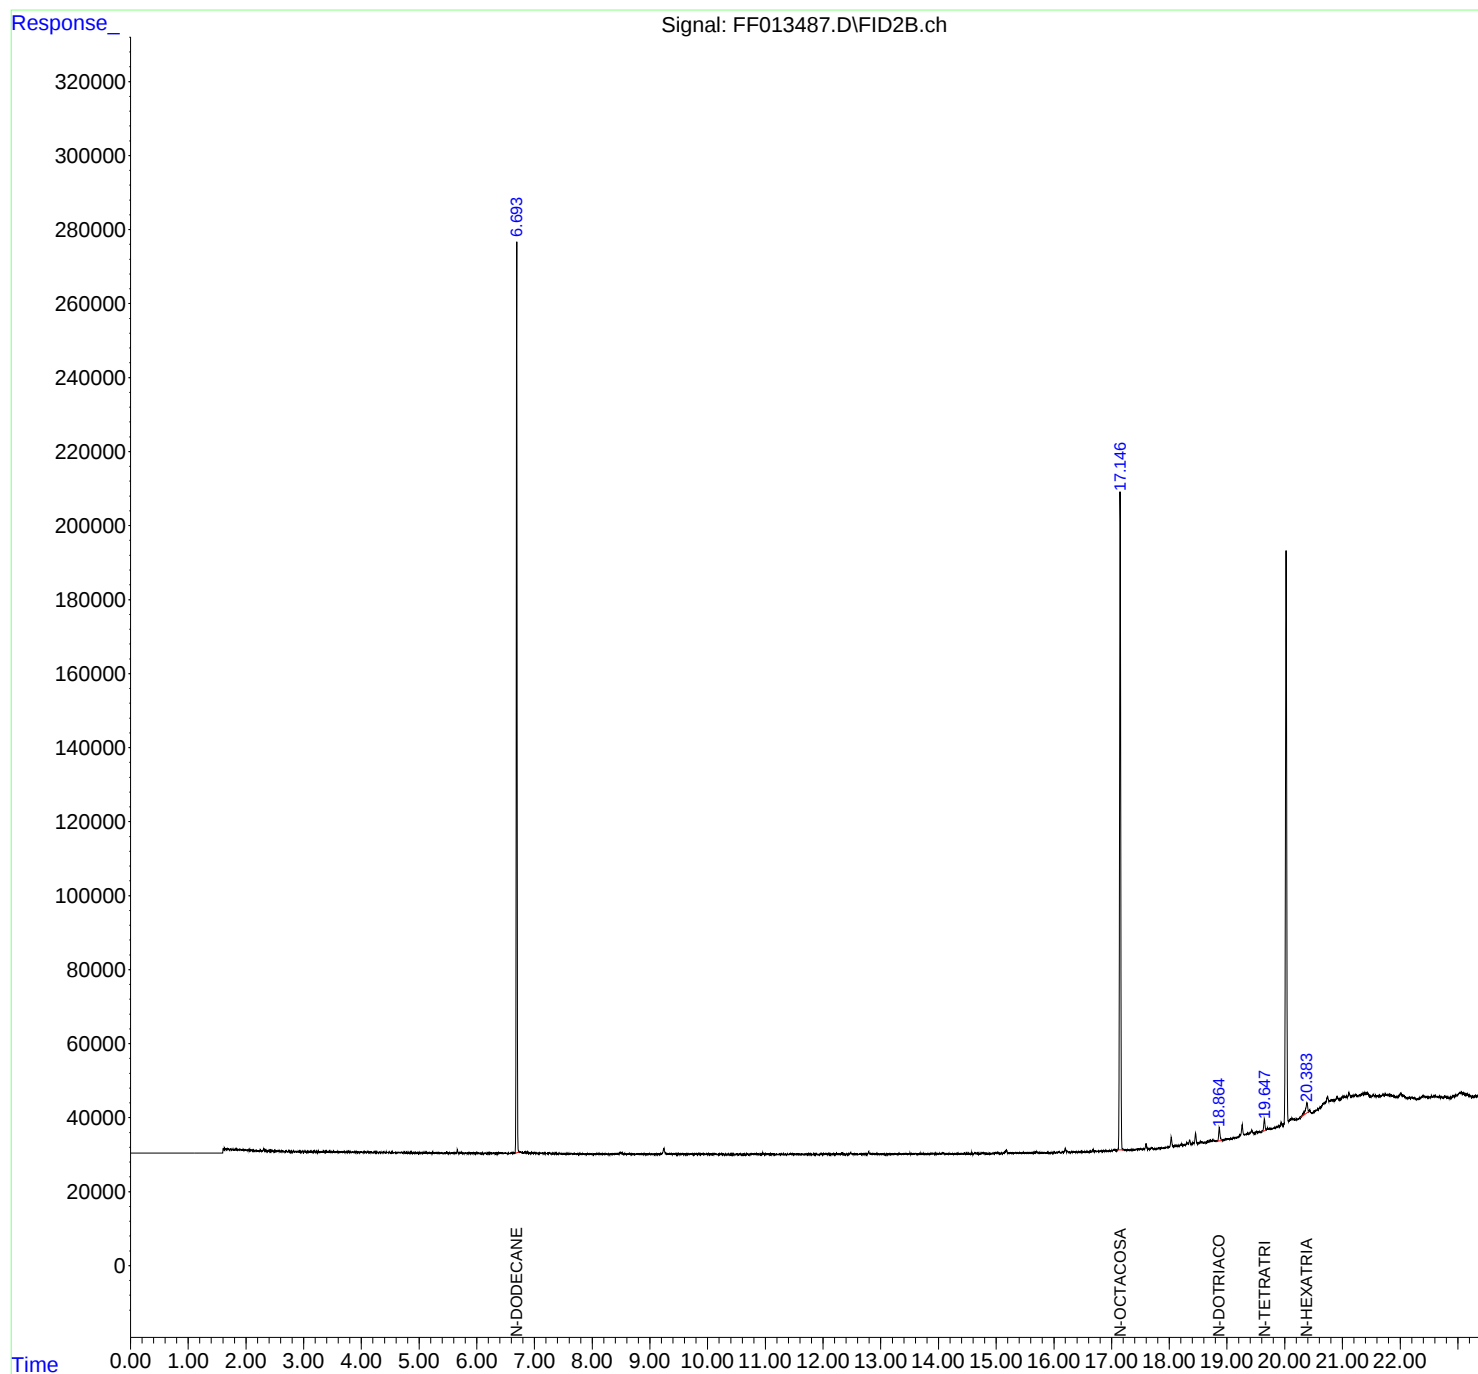


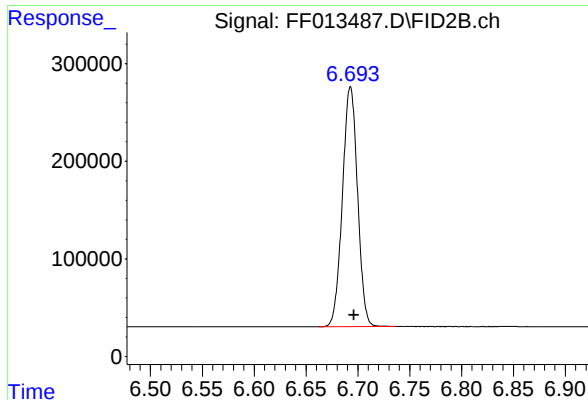

#3 N-DODECANE


R.T.: 6.693 min
Delta R.T.: -0.003 min
Response: 2495497
Conc: 18.71 ug/ml

Instrument :
FID_F
ClientSampleId :

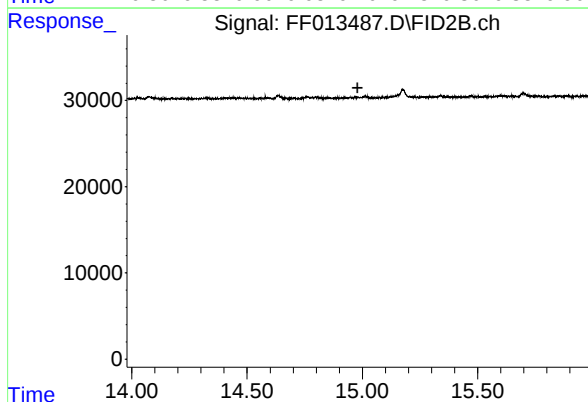


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.979 min
Response: 0
Conc: N.D.

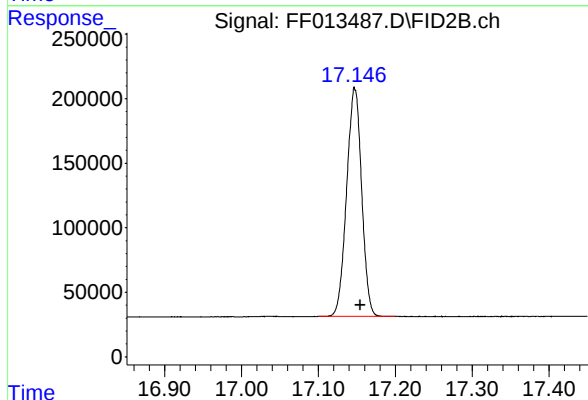


#12 N-OCTACOSANE

R.T.: 17.147 min
Delta R.T.: -0.007 min
Response: 2400483
Conc: 18.63 ug/ml

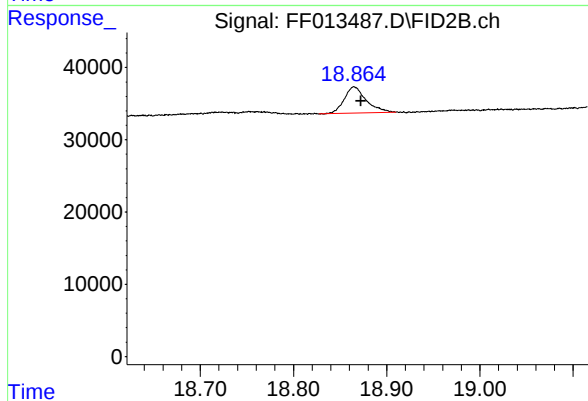

#14 N-DOTRIACONTANE


R.T.: 18.865 min
Delta R.T.: -0.007 min
Response: 59313
Conc: 0.51 ug/ml

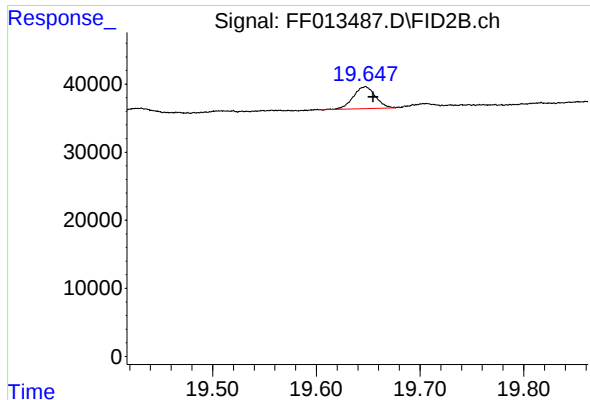

#15 N-TETRATRIACONTANE

R.T.: 19.647 min
Delta R.T.: -0.008 min
Response: 47375
Conc: 0.46 ug/ml

Instrument :
FID_F
ClientSampleId :

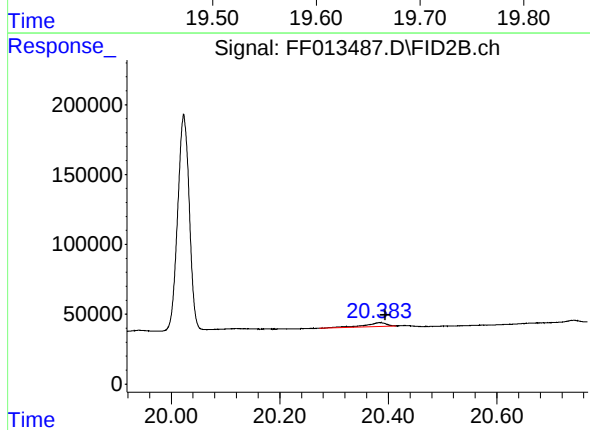

#16 N-HEXATRIACONTANE

R.T.: 20.384 min
Delta R.T.: -0.011 min
Response: 77051
Conc: 0.79 ug/ml